
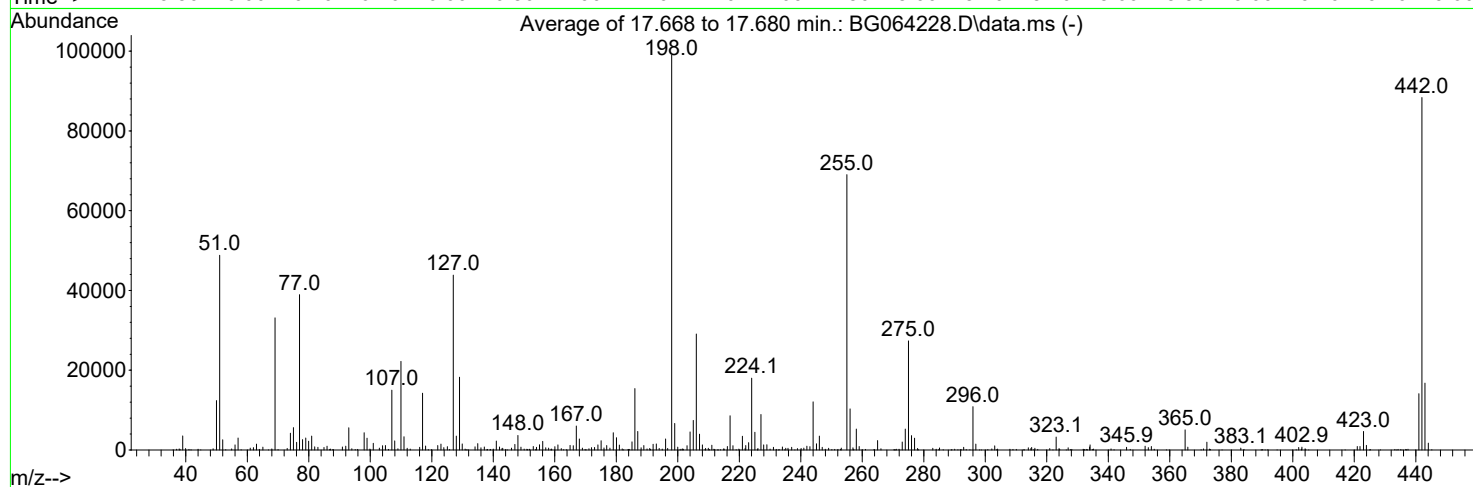


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082925\
Data File : BG064228.D
Acq On : 29 Aug 2025 13:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082825.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Aug 28 17:41:58 2025

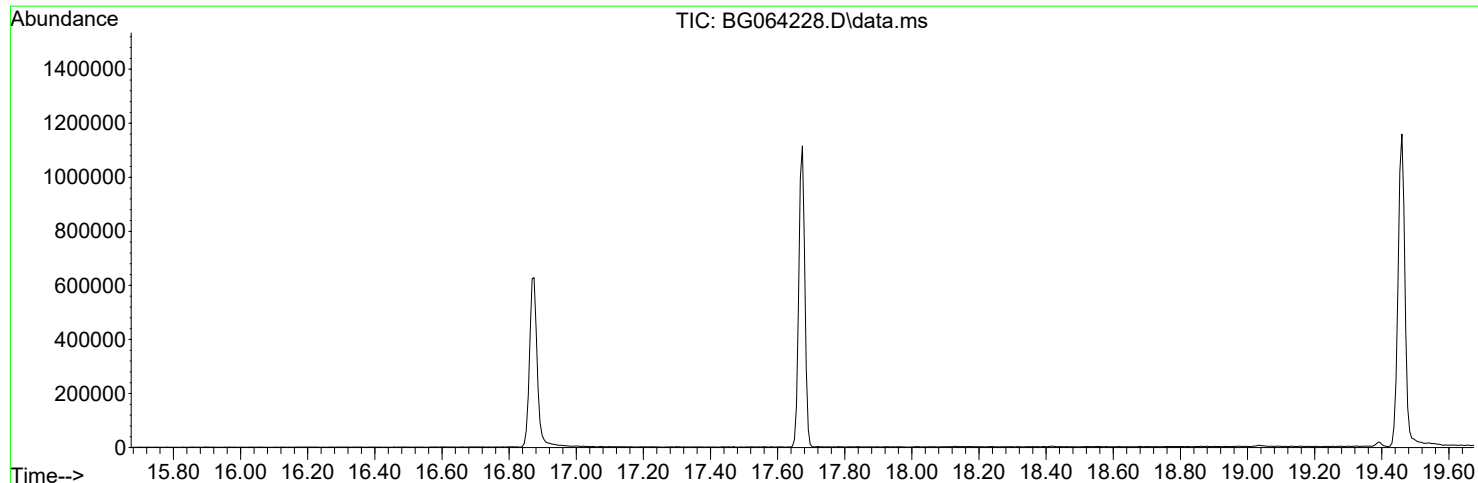

AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2474

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	0.9	283	PASS
69	69	100	100	100.0	33152	PASS
70	69	0.00	2	0.3	105	PASS
197	198	0.00	2	0.4	413	PASS
198	198	100	100	100.0	98995	PASS
199	198	5	9	6.7	6664	PASS
365	198	1	100	5.1	5036	PASS
441	443	0.01	150	84.2	14118	PASS
442	442	100	100	100.0	88395	PASS
443	442	15	24	19.0	16771	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/29/2025	BNA_G	<u>BG064228.D</u>
Compound Name	Response	Retention Time
DDT	334216	20.694
DDD	8270	20.253
DDE	0	19.751
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8270	342486	2.41

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082925\
Data File : BG064228.D
Acq On : 29 Aug 2025 13:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 29 15:18:16 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 28 17:41:58 2025
Response via : Initial Calibration

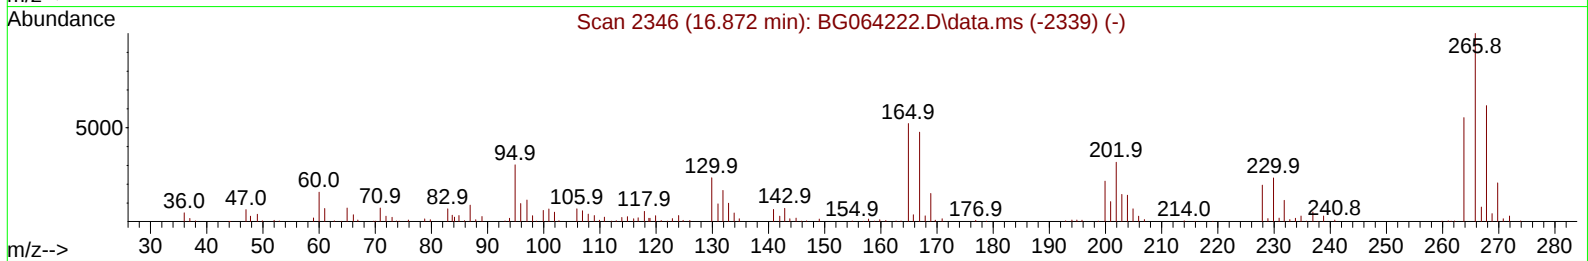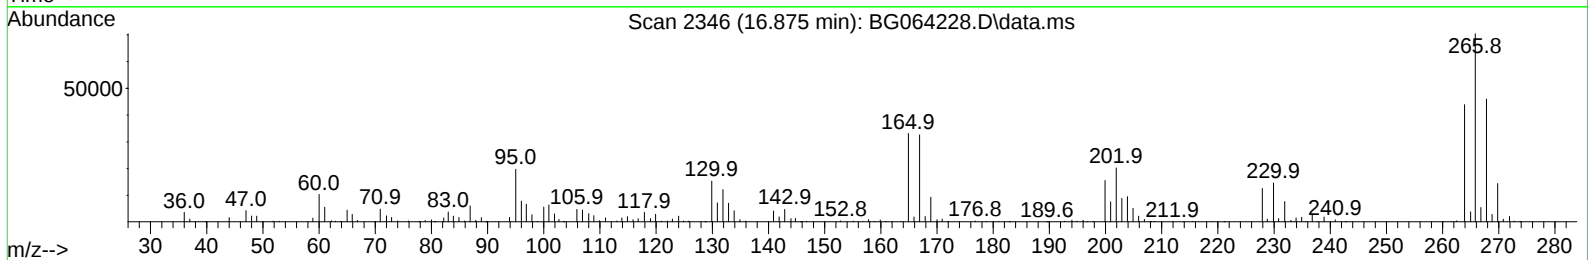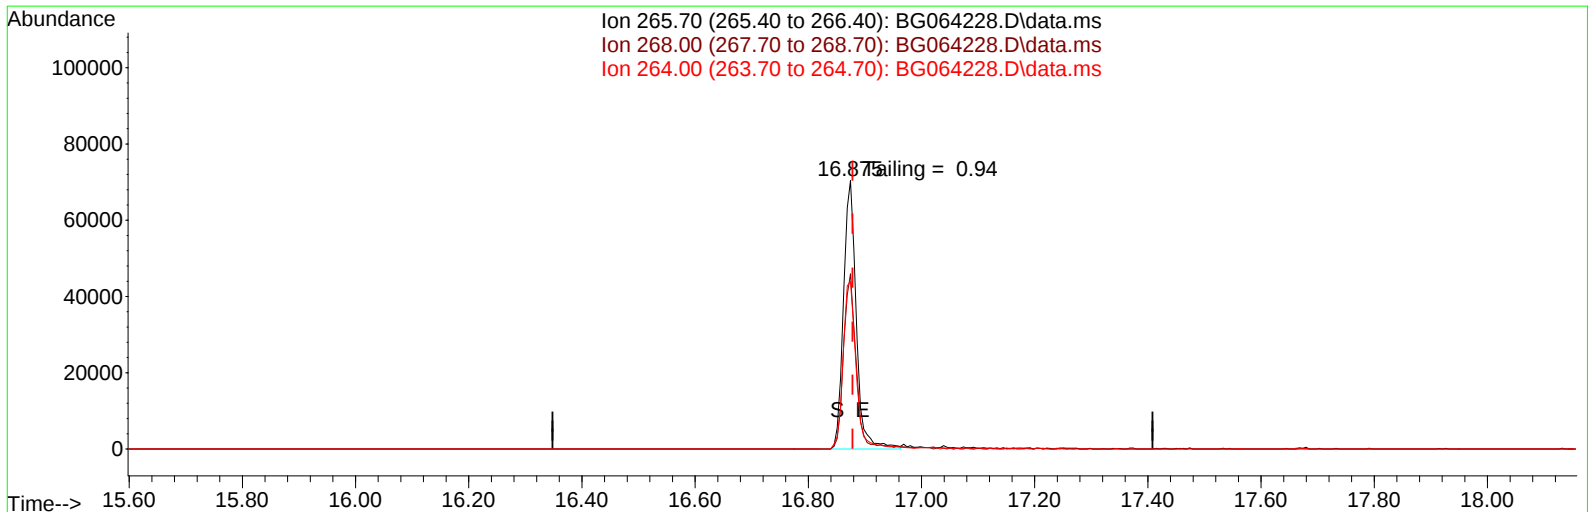

TIC: BG064228.D\data.ms

(70) Pentachlorophenol (C)

16.875min (-0.003) 97482.03 ng




response 110848

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	65.28
264.00	55.40	62.38
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082925\
Data File : BG064228.D
Acq On : 29 Aug 2025 13:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 29 15:18:16 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 28 17:41:58 2025
Response via : Initial Calibration

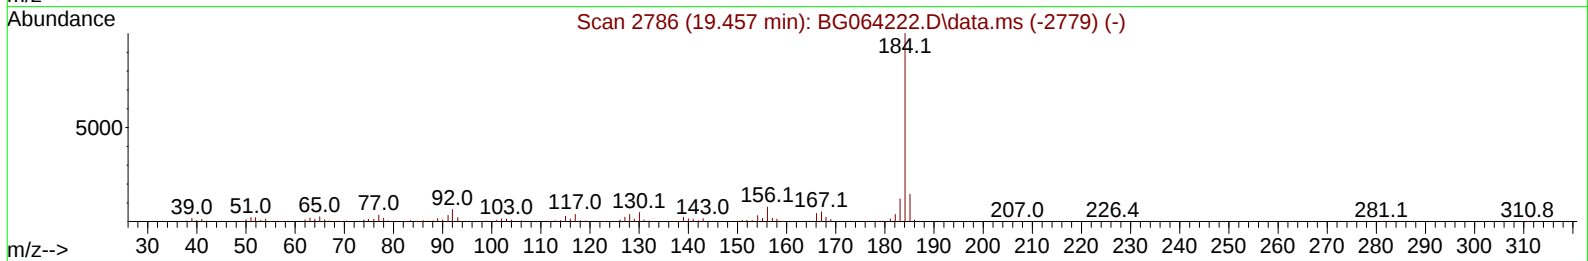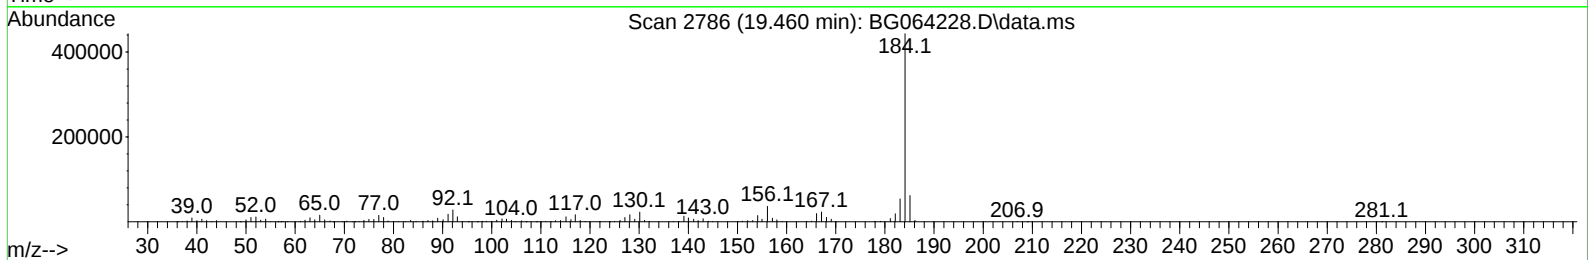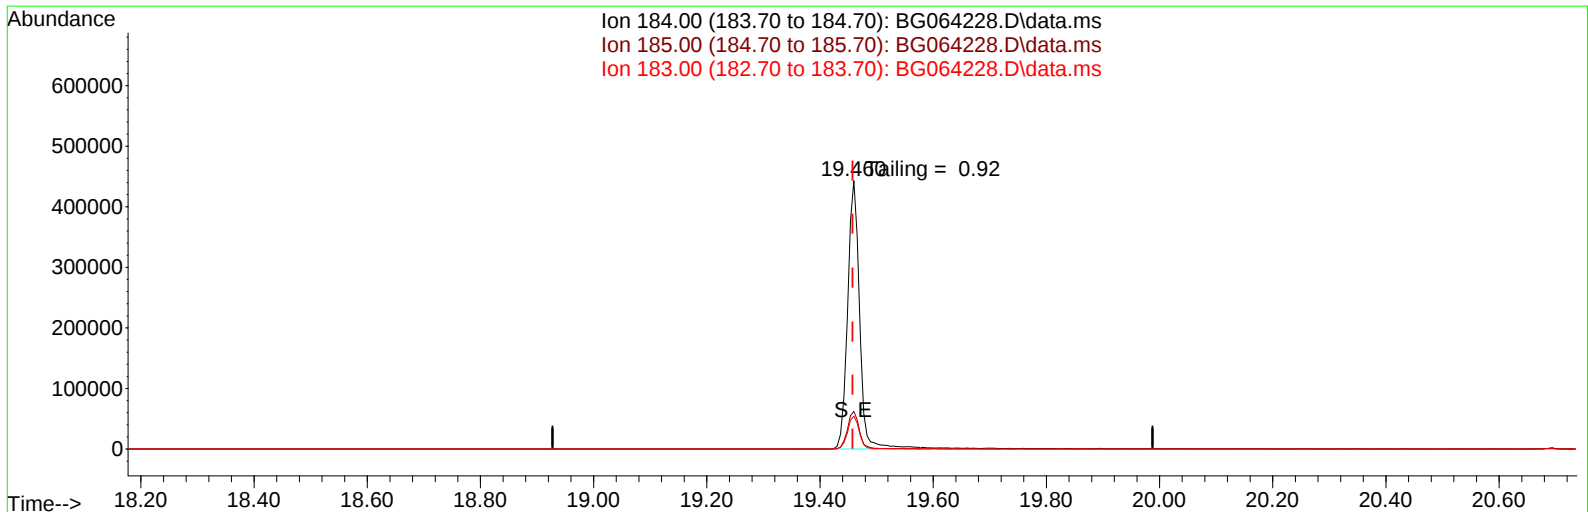

TIC: BG064228.D\data.ms

(77) Benzidine

19.460min (+ 0.002) 517458.75 ng

response 653131

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.03
183.00	12.10	12.21
0.00	0.00	0.00