

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG083019\
 Data File : BG042594.D
 Acq On : 30 Aug 2019 10:56
 Operator : HP/JU
 Sample : PB122666TB
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB122666TB

Quant Time: Aug 30 16:27:49 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082219.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 22 14:29:15 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.00	152	36745	20.00	ng	0.00
21) Naphthalene-d8	10.82	136	140168	20.00	ng	0.00
39) Acenaphthene-d10	14.66	164	101125	20.00	ng	0.00
64) Phenanthrene-d10	17.41	188	238571	20.00	ng	0.00
76) Chrysene-d12	21.68	240	265095	20.00	ng	-0.01
87) Perylene-d12	24.93	264	307872	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.55	112	233572	128.74	ng	0.00
7) Phenol-d6	7.16	99	301130	122.87	ng	0.00
23) Nitrobenzene-d5	9.16	82	171031	84.32	ng	-0.01
42) 2,4,6-Tribromophenol	16.15	330	184725	128.52	ng	0.00
45) 2-Fluorobiphenyl	13.27	172	569052	95.17	ng	0.00
79) Terphenyl-d14	20.02	244	1135316	92.59	ng	0.00


Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG083019\
Data File : BG042594.D
Acq On : 30 Aug 2019 10:56
Operator : HP/JU
Sample : PB122666TB
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB122666TB

Quant Time: Aug 30 16:27:49 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 22 14:29:15 2019
Response via : Initial Calibration

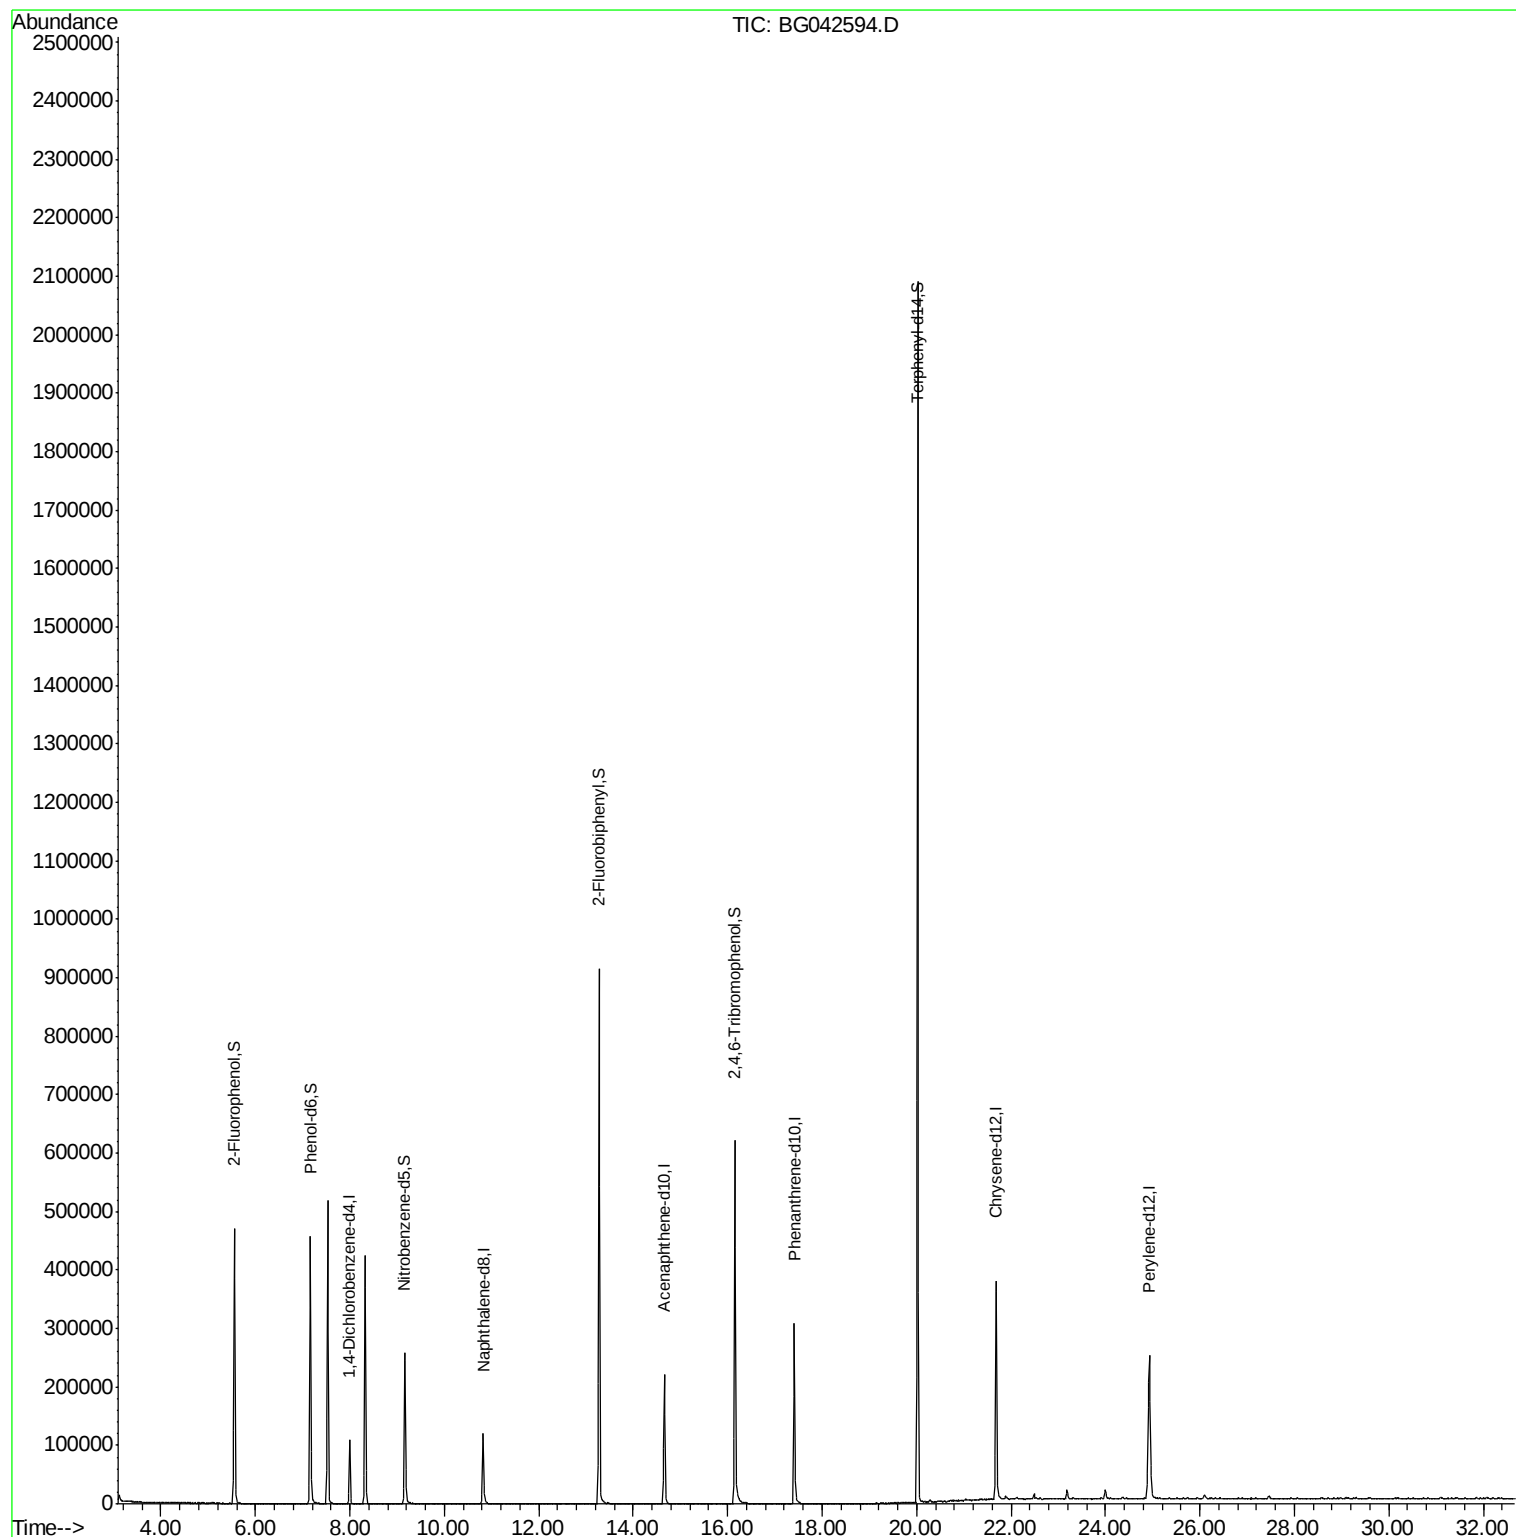




#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.00 min Scan# 836
Delta R.T. -0.01 min
Lab File: BG042594.D
Acq: 30 Aug 2019 10:56

Instrument :
BNA_G
ClientSampleId :
PB122666TB

Tot Ion:152 Resp: 36745
Ion Ratio Lower Upper
152 100
150 154.1 125.4 188.0
115 52.4 38.5 57.7

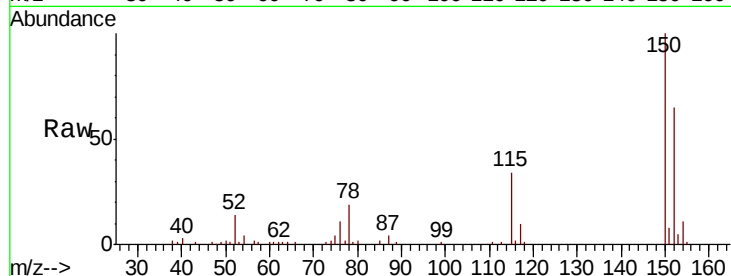


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

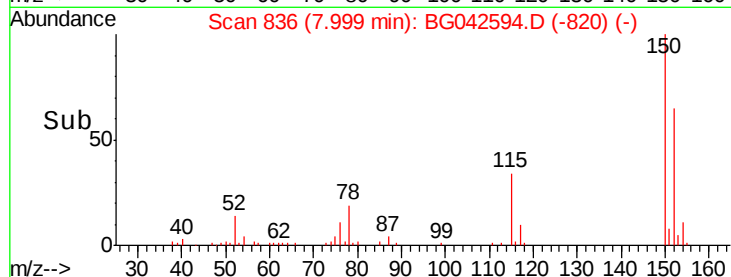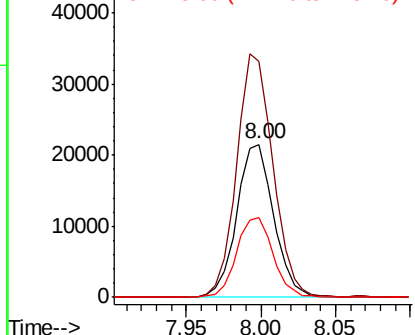



#5

2-Fluorophenol
Concen: 128.739 ng
RT: 5.55 min Scan# 420
Delta R.T. -0.01 min
Lab File: BG042594.D
Acq: 30 Aug 2019 10:56

Tgt Ion:112 Resp: 233572
Ion Ratio Lower Upper
112 100
64 54.8 42.8 64.2
63 28.8 22.7 34.1

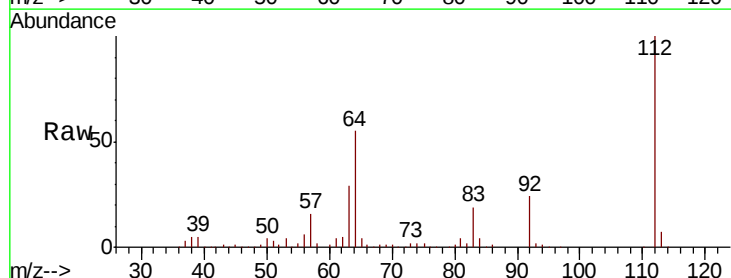

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

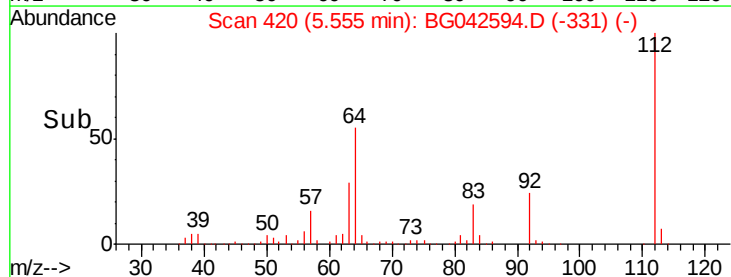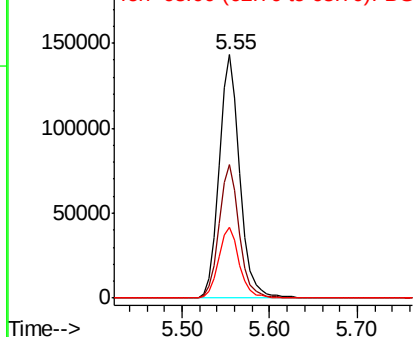



#7

Phenol-d6

Concen: 122.874 ng

RT: 7.16 min Scan# 694

Delta R.T. -0.01 min

Lab File: BG042594.D

Acq: 30 Aug 2019 10:56

Instrument :

BNA_G

ClientSampleId :

PB122666TB


Tot Ion: 99 Resp: 301130

Ion Ratio Lower Upper




99 100

42 14.6 12.0 18.0

71 35.6 26.3 39.5

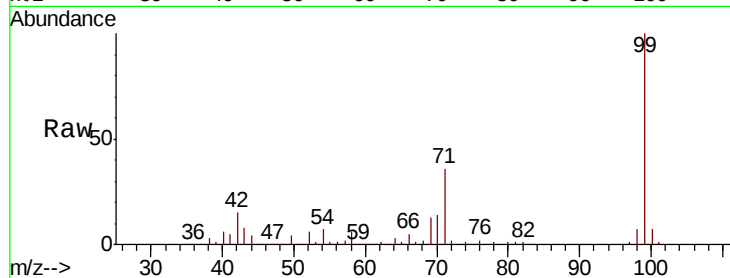

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

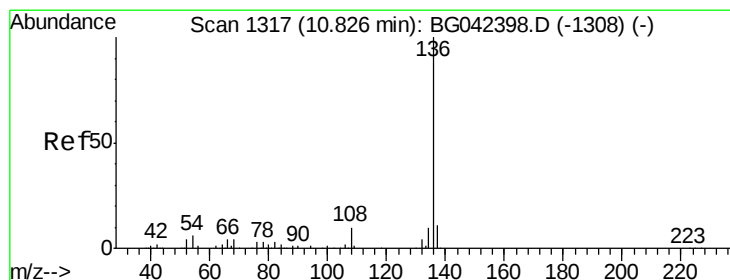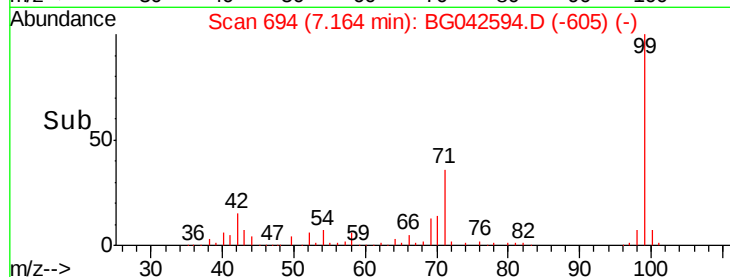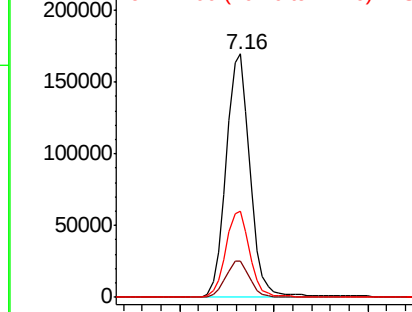

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.82 min Scan# 1316

Delta R.T. -0.01 min

Lab File: BG042594.D

Acq: 30 Aug 2019 10:56

Tgt Ion: 136 Resp: 140168


Ion Ratio Lower Upper

136 100



137 10.6 8.7 13.1

54 5.6 4.9 7.3

68 4.0 3.6 5.4

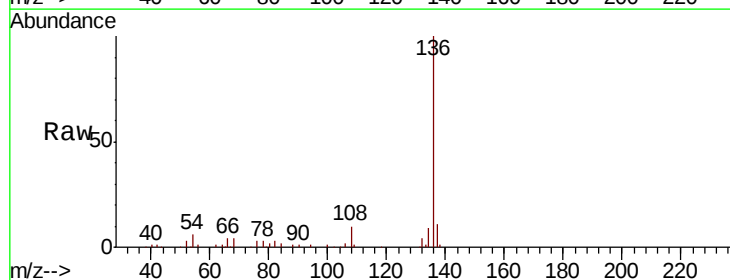

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

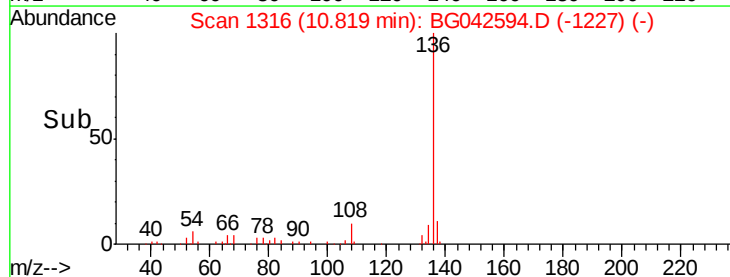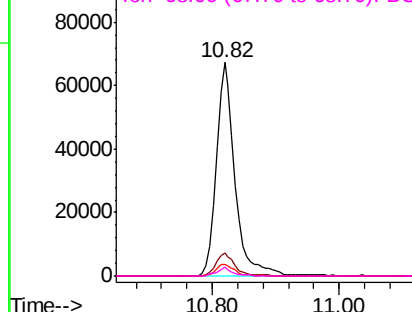






#23
Nitrobenzene-d5
Concen: 84.320 ng
RT: 9.16 min Scan# 1034
Delta R.T. -0.01 min
Lab File: BG042594.D
Acq: 30 Aug 2019 10:56

Instrument :
BNA_G
ClientSampleId :
PB122666TB

Tot Ion	82	Resp	171031
Ion Ratio	100	Lower	Upper
128	52.2	40.7	61.1
54	47.9	36.3	54.5

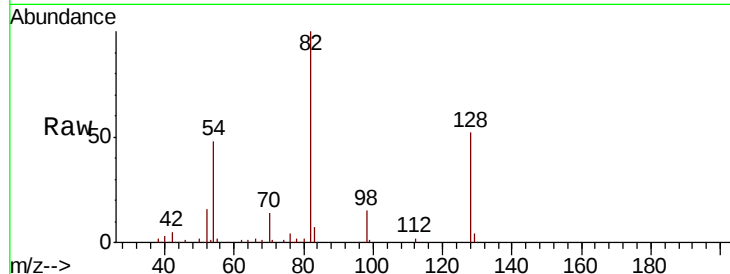


Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): BGC
Ion 54.00 (53.70 to 54.70): BGC

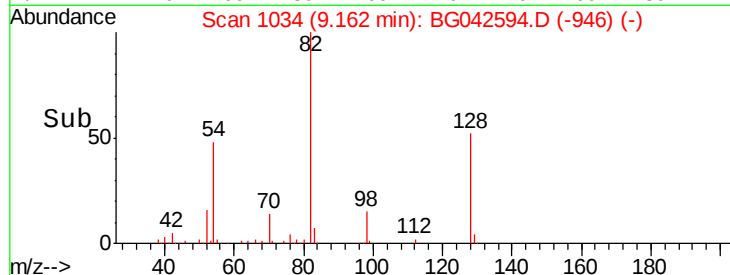
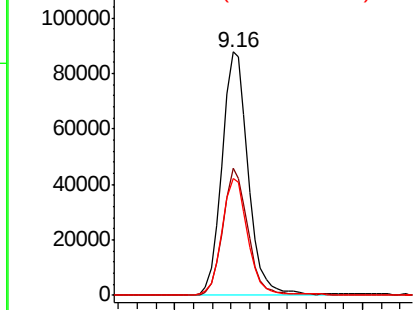



#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.66 min Scan# 1969
Delta R.T. -0.01 min
Lab File: BG042594.D
Acq: 30 Aug 2019 10:56

Tgt Ion	164	Resp	101125
Ion Ratio	100	Lower	Upper
162	98.7	79.9	119.9
160	43.3	34.3	51.5

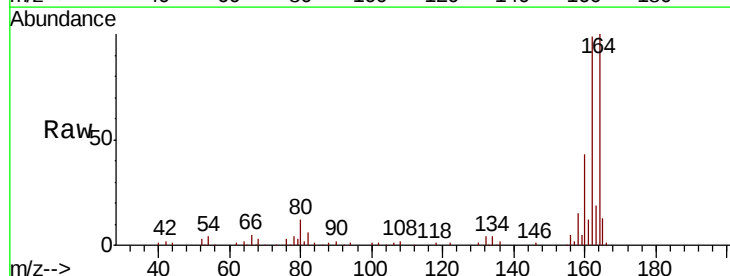

Abundance Ion 164.00 (163.70 to 164.70): BGC
Ion 162.00 (161.70 to 162.70): BGC
Ion 160.00 (159.70 to 160.70): BGC

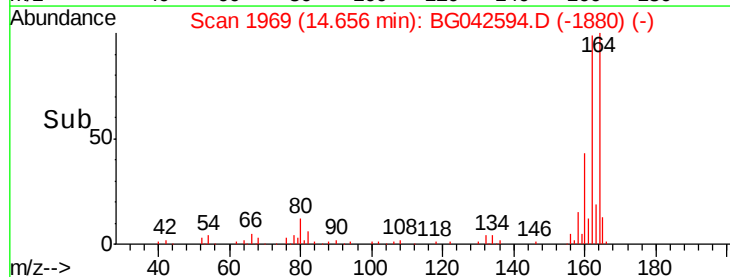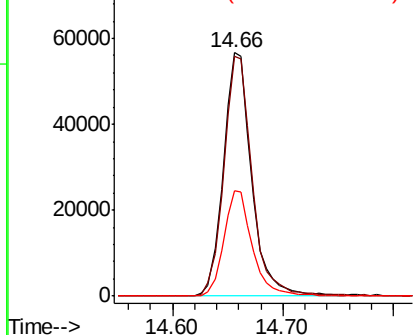

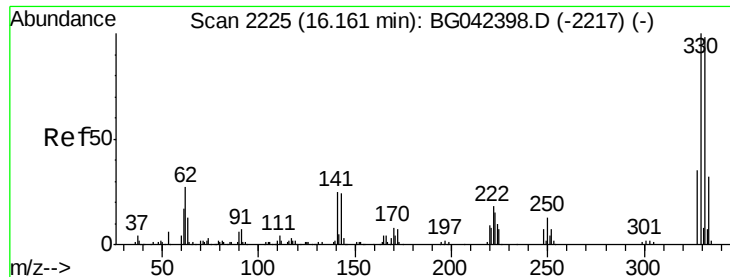

#42

2,4,6-Tribromophenol

Concen: 128.520 ng

RT: 16.15 min Scan# 2224

Delta R.T. -0.01 min

Lab File: BG042594.D

Acq: 30 Aug 2019 10:56

Instrument :

BNA_G

ClientSampleId :

PB122666TB


Tot Ion:330 Resp: 184725

Ion Ratio Lower Upper

330 100

332 97.2 77.4 116.0




141 26.0 21.4 32.0

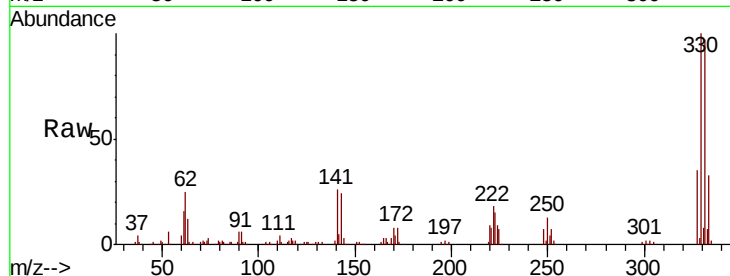

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

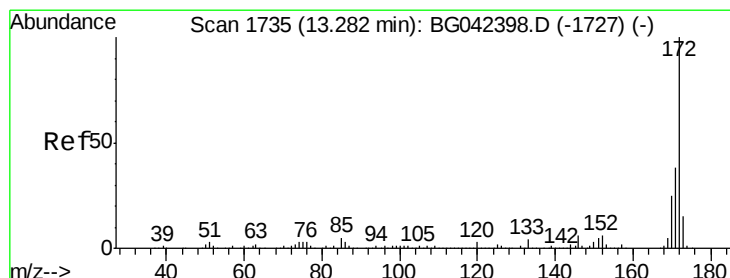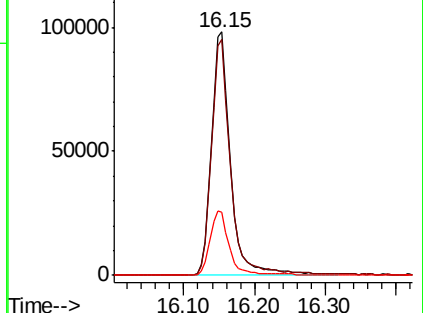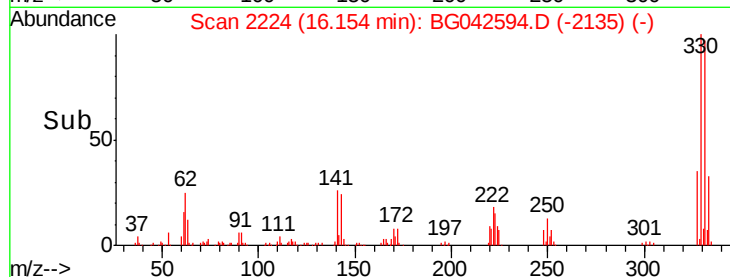

#45

2-Fluorobiphenyl

Concen: 95.172 ng

RT: 13.27 min Scan# 1734

Delta R.T. -0.01 min

Lab File: BG042594.D

Acq: 30 Aug 2019 10:56


Tgt Ion:172 Resp: 569052

Ion Ratio Lower Upper

172 100

171 36.5 30.5 45.7



170 24.0 20.2 30.2

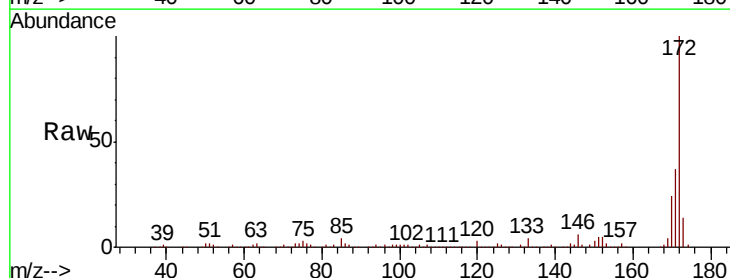


Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

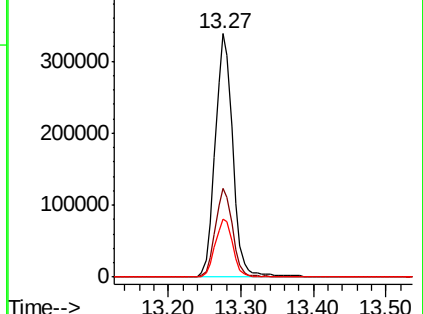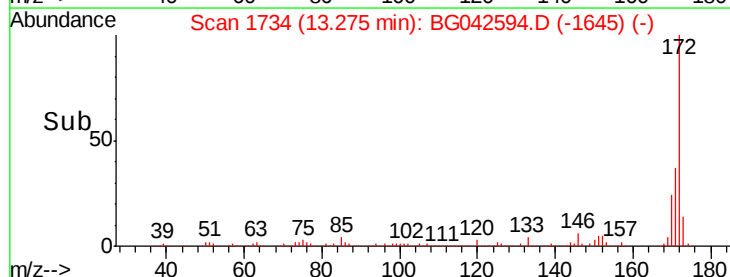


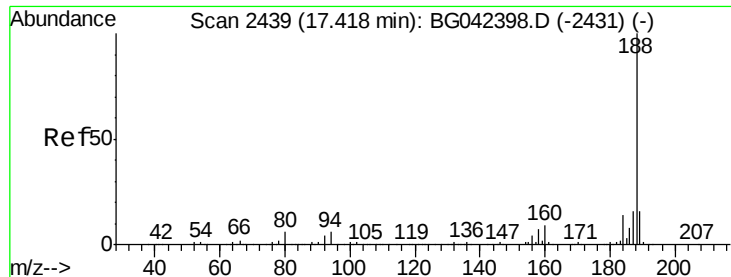




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.41 min Scan# 2438
Delta R.T. -0.01 min
Lab File: BG042594.D
Acq: 30 Aug 2019 10:56

Instrument :
BNA_G
ClientSampleId :
PB122666TB

Tot Ion:188 Resp: 238571
Ion Ratio Lower Upper
188 100
94 4.4 4.5 6.7#
80 5.2 4.9 7.3

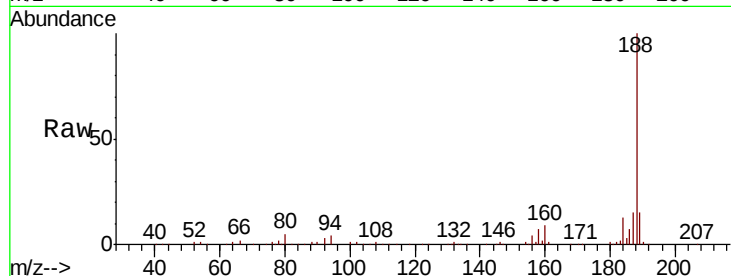


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BG
Ion 80.00 (79.70 to 80.70): BG

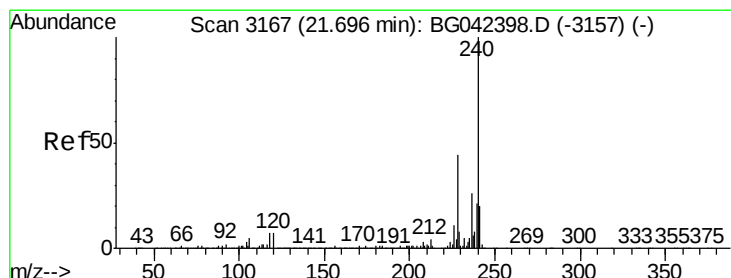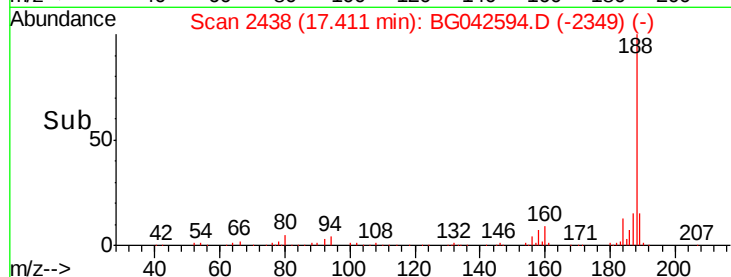
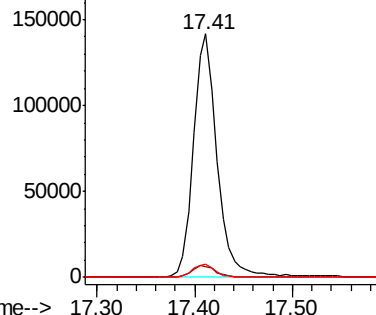


#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.68 min Scan# 3165
Delta R.T. -0.01 min
Lab File: BG042594.D
Acq: 30 Aug 2019 10:56

Tgt Ion:240 Resp: 265095
Ion Ratio Lower Upper
240 100
120 6.0 5.7 8.5
236 25.7 21.0 31.4

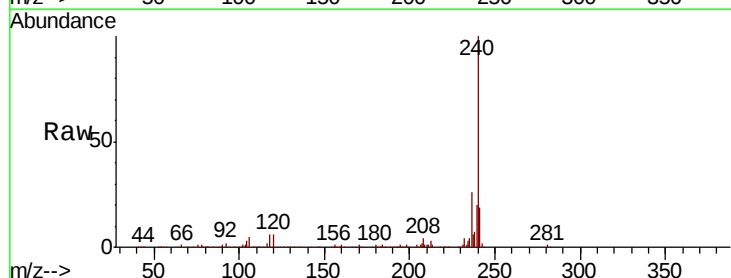

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

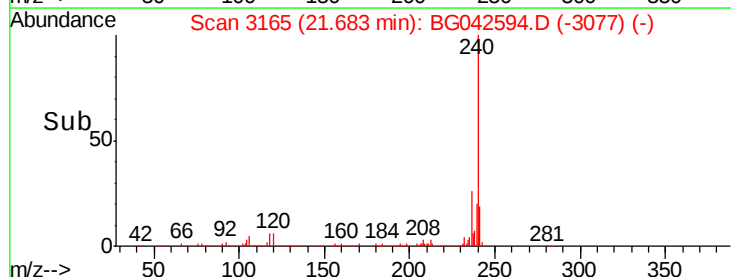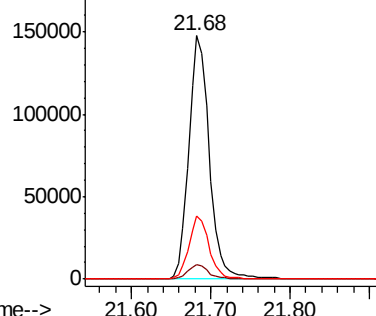



#79

Terphenyl-d14

Concen: 92.588 ng

RT: 20.02 min Scan# 2882

Delta R.T. -0.01 min

Lab File: BG042594.D

Acq: 30 Aug 2019 10:56

Instrument :


BNA_G

ClientSampleId :

PB122666TB

Tot Ion:244 Resp: 1135316

Ion	Ratio	Lower	Upper
244	100		
212	6.9	6.0	9.0
122	7.0	6.7	10.1



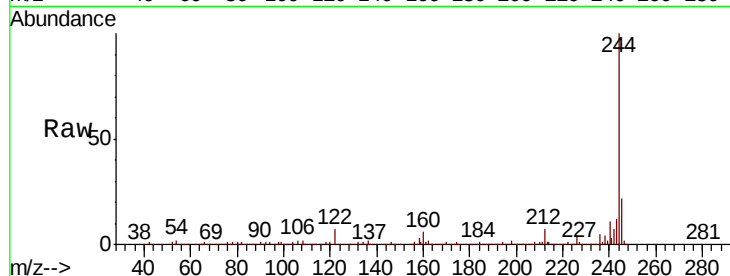


Abundance

Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

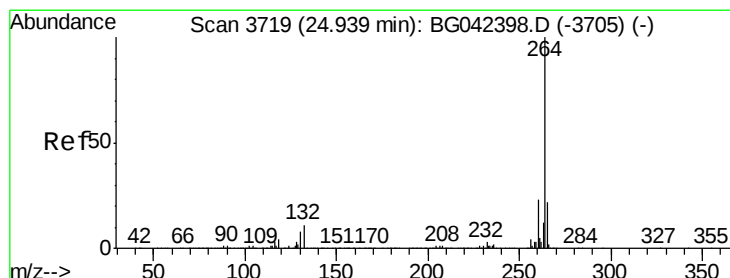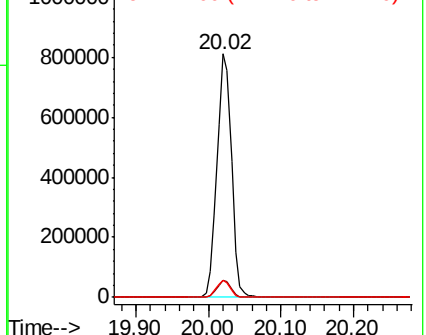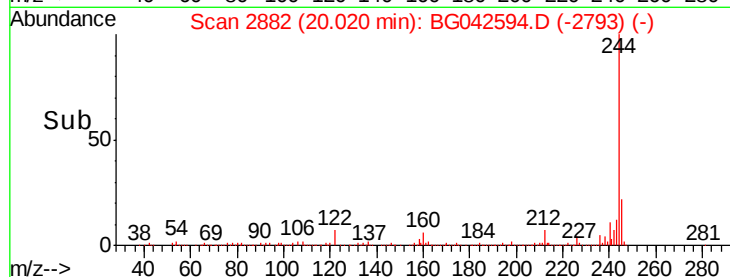

#87

Perylene-d12

Concen: 20.000 ng

RT: 24.93 min Scan# 3717


Delta R.T. -0.01 min

Lab File: BG042594.D

Acq: 30 Aug 2019 10:56

Tgt Ion:264 Resp: 307872

Ion	Ratio	Lower	Upper
264	100		
260	23.1	18.5	27.7
265	22.9	17.6	26.4

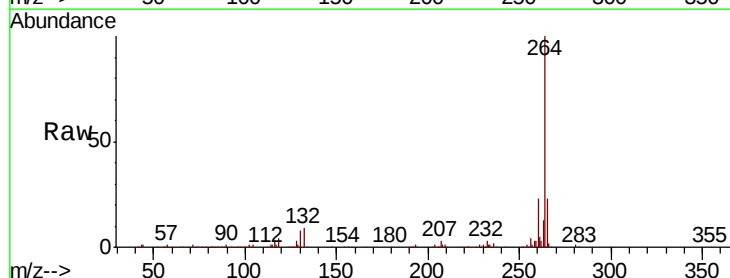

Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

