


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG083019\
Data File : BG042589.D
Acq On : 30 Aug 2019 7:05
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082219.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Aug 22 14:29:15 2019

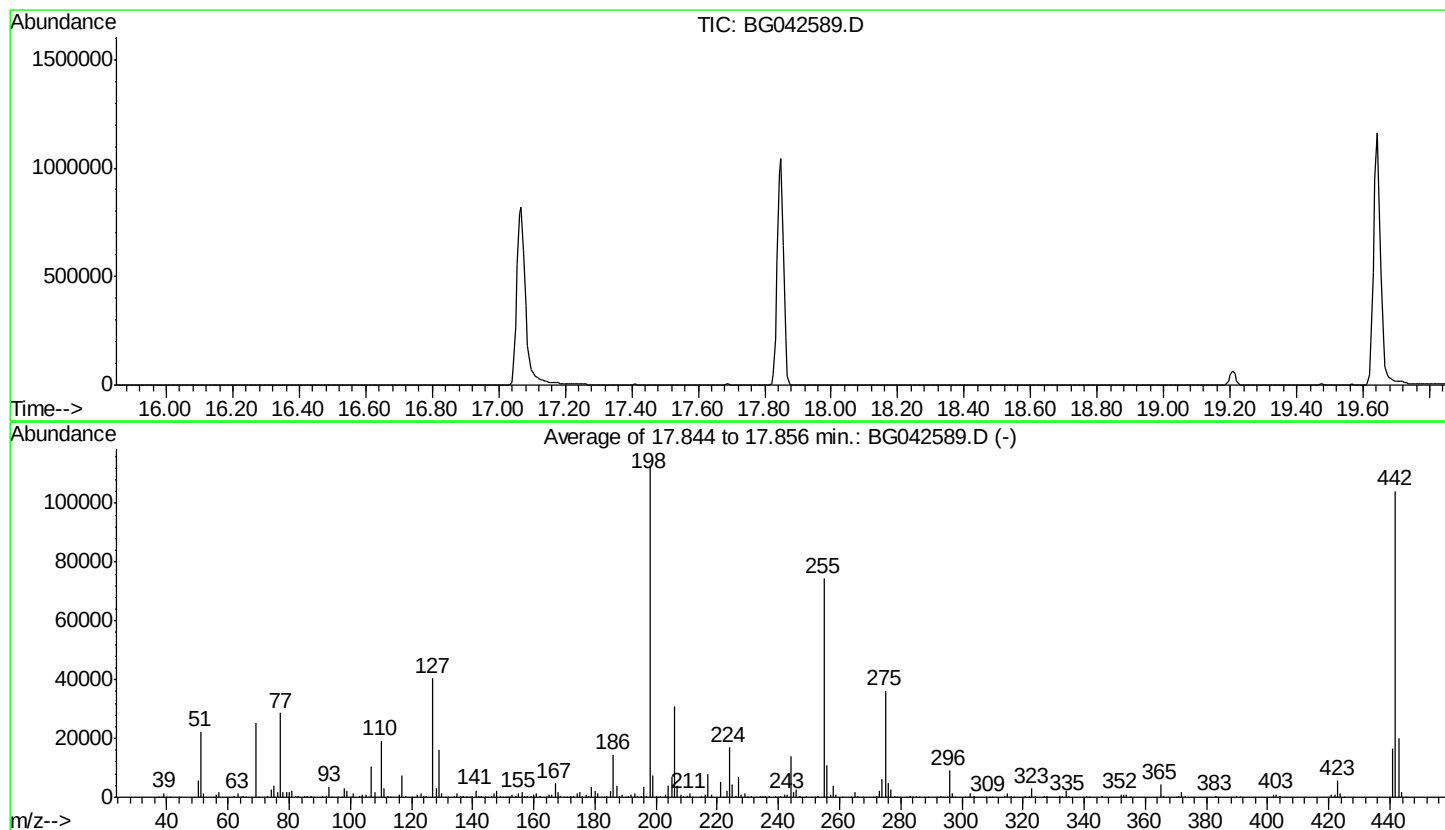

AutoFind: Scans 2511, 2512, 2513; Background Corrected with Scan 2504

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	19.8	22329	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	22.5	25378	PASS
70	69	0.00	2	0.2	63	PASS
127	198	10	80	35.9	40482	PASS
197	198	0.00	2	0.4	400	PASS
198	198	100	100	100.0	112845	PASS
199	198	5	9	6.5	7360	PASS
275	198	10	60	32.1	36173	PASS
365	198	1	100	3.7	4169	PASS
441	198	0.01	100	14.7	16625	PASS
442	198	50	100	92.4	104253	PASS
443	442	15	24	19.4	20264	PASS