


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG083019\
 Data File : BG042603.D
 Acq On : 30 Aug 2019 16:44
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 22 14:29:15 2019

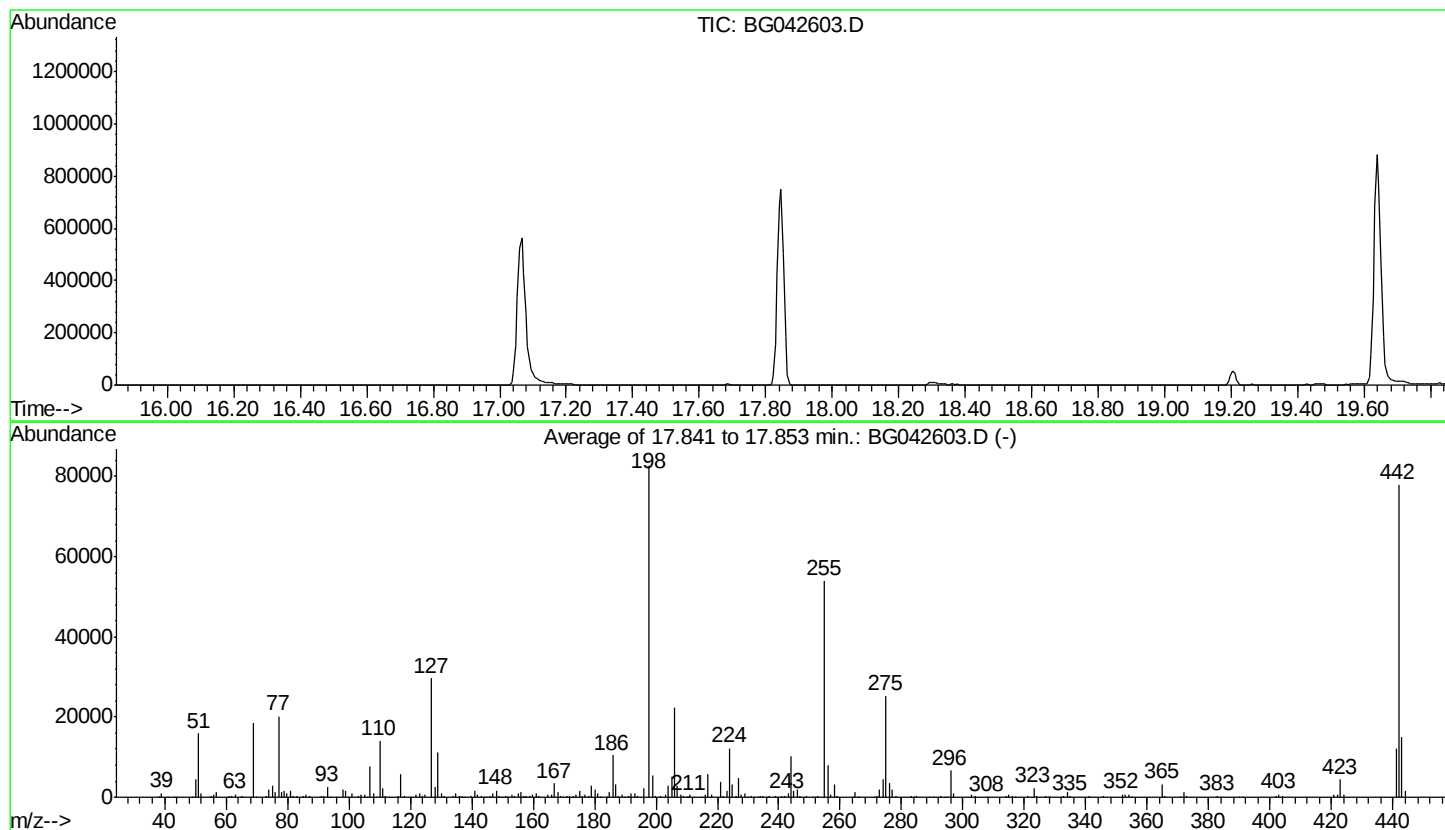

AutoFind: Scans 2511, 2512, 2513; Background Corrected with Scan 2504

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	19.3	15944	PASS
68	69	0.00	2	0.5	90	PASS
69	198	0.00	100	22.3	18453	PASS
70	69	0.00	2	0.6	104	PASS
127	198	10	80	35.8	29578	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	82701	PASS
199	198	5	9	6.8	5597	PASS
275	198	10	60	30.7	25368	PASS
365	198	1	100	3.9	3245	PASS
441	198	0.01	100	14.6	12098	PASS
442	198	50	100	94.3	77960	PASS
443	442	15	24	19.3	15050	PASS