

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083021\
 Data File : BG050037.D
 Acq On : 30 Aug 2021 18:27
 Operator : CG/JU
 Sample : M3458-19
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0B64

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
 Title : SVOA CALIBRATION

Signal : TIC: BG050037.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.502	77	79	82	rBV3	1585	2090	0.50%	0.044%
2	3.772	121	125	129	rBV2	5875	10269	2.45%	0.217%
3	5.176	361	364	365	rBV2	1441	1704	0.41%	0.036%
4	5.599	434	436	438	rBV	1689	1652	0.39%	0.035%
5	5.816	469	473	474	rVB3	1588	1690	0.40%	0.036%
6	5.857	477	480	481	rBV	1320	1406	0.34%	0.030%
7	5.928	490	492	494	rBV2	1332	1206	0.29%	0.026%
8	6.233	542	544	547	rVB	1374	1220	0.29%	0.026%
9	6.286	550	553	555	rBV3	1340	1165	0.28%	0.025%
10	6.539	593	596	598	rBV3	1165	1189	0.28%	0.025%
11	6.891	654	656	659	rBV	960	1157	0.28%	0.024%
12	7.138	691	698	705	rBV	54335	92660	22.12%	1.960%
13	7.285	717	723	732	rVB	40342	71115	16.98%	1.504%
14	7.408	742	744	748	rVB2	1298	1254	0.30%	0.027%
15	7.496	751	759	766	rBV	62864	106344	25.39%	2.250%
16	7.696	791	793	796	rBV	1329	1680	0.40%	0.036%
17	7.831	814	816	821	rBV3	1282	1542	0.37%	0.033%
18	7.961	831	838	848	rVB	100583	167295	39.94%	3.539%
19	8.196	874	878	881	rBV	1249	1717	0.41%	0.036%
20	8.413	912	915	918	rBV2	1363	2099	0.50%	0.044%
21	8.548	936	938	942	rVB	1159	1359	0.32%	0.029%
22	8.595	942	946	949	rBV	1575	2296	0.55%	0.049%
23	8.689	956	962	970	rBV	52243	94910	22.66%	2.008%
24	8.742	970	971	976	rVV	1946	1997	0.48%	0.042%
25	8.801	978	981	983	rVB3	1516	1318	0.31%	0.028%
26	9.135	1030	1038	1045	rBV3	63105	117903	28.15%	2.494%
27	9.265	1057	1060	1062	rBV	1372	1344	0.32%	0.028%
28	9.511	1098	1102	1105	rBV2	1049	1647	0.39%	0.035%
29	9.864	1155	1162	1171	rVB2	59552	109058	26.04%	2.307%
30	10.140	1207	1209	1212	rVB	1423	1143	0.27%	0.024%
31	10.416	1250	1256	1268	rVB2	85235	150961	36.04%	3.194%
32	10.551	1274	1279	1283	rBV4	9284	16455	3.93%	0.348%
33	10.739	1306	1311	1312	rBV3	1187	1720	0.41%	0.036%
34	10.786	1312	1319	1327	rVB	132652	238943	57.05%	5.055%
35	10.921	1332	1342	1350	rBV	57735	111613	26.65%	2.361%
36	11.620	1457	1461	1463	rVV2	1042	1539	0.37%	0.033%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083021\
 Data File : BG050037.D
 Acq On : 30 Aug 2021 18:27
 Operator : CG/JU
 Sample : M3458-19
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0B64

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
 Title : SVOA CALIBRATION

37	11.638	1463	1464	1468	rVB2	1132	1190	0.28%	0.025%
38	11.797	1487	1491	1493	rBV2	1661	2648	0.63%	0.056%
39	11.849	1496	1500	1501	rBV	1002	1417	0.34%	0.030%
40	12.196	1555	1559	1562	rBV2	2098	2178	0.52%	0.046%
41	12.272	1568	1572	1576	rVB2	1304	1816	0.43%	0.038%
42	12.302	1576	1577	1581	rBV	1381	1616	0.39%	0.034%
43	12.449	1598	1602	1607	rBV2	2215	3155	0.75%	0.067%
44	13.142	1718	1720	1723	rVB2	1073	1187	0.28%	0.025%
45	13.206	1730	1731	1735	rVB	1290	1317	0.31%	0.028%
46	13.435	1764	1770	1774	rVB3	3017	4946	1.18%	0.105%
47	13.635	1802	1804	1807	rVB	1359	1150	0.27%	0.024%
48	13.759	1821	1825	1828	rBV2	934	1264	0.30%	0.027%
49	13.941	1854	1856	1860	rVB2	1839	1572	0.38%	0.033%
50	14.023	1863	1870	1876	rBV	163521	236197	56.39%	4.997%
51	14.270	1908	1912	1914	rBV	886	1522	0.36%	0.032%
52	14.317	1914	1920	1932	rVB	171562	273423	65.28%	5.784%
53	14.505	1949	1952	1958	rVB3	3439	4565	1.09%	0.097%
54	14.628	1966	1973	1983	rVB	218915	349608	83.47%	7.396%
55	14.863	2008	2013	2024	rBV4	27853	61953	14.79%	1.311%
56	15.198	2067	2070	2075	rBV	1289	1920	0.46%	0.041%
57	15.398	2103	2104	2109	rVB2	1176	1156	0.28%	0.024%
58	15.456	2111	2114	2119	rVB3	3530	4433	1.06%	0.094%
59	15.621	2136	2142	2151	rVB	224323	337535	80.59%	7.140%
60	15.762	2160	2166	2173	rBV3	32932	51187	12.22%	1.083%
61	15.862	2178	2183	2186	rVV2	2447	3395	0.81%	0.072%
62	15.885	2186	2187	2193	rVB2	1269	1345	0.32%	0.028%
63	15.944	2195	2197	2199	rBV2	2098	1509	0.36%	0.032%
64	16.108	2223	2225	2228	rVB2	2198	1473	0.35%	0.031%
65	16.273	2251	2253	2255	rBV2	1243	1193	0.28%	0.025%
66	16.320	2258	2261	2263	rVV2	5442	6172	1.47%	0.131%
67	16.343	2263	2265	2270	rVB3	3758	5315	1.27%	0.112%
68	16.484	2285	2289	2290	rBV	1102	1431	0.34%	0.030%
69	16.531	2295	2297	2299	rVV2	1481	1261	0.30%	0.027%
70	16.555	2299	2301	2303	rVB2	1603	1503	0.36%	0.032%
71	16.596	2305	2308	2310	rBV2	1299	1431	0.34%	0.030%
72	16.713	2327	2328	2333	rBV	1441	1616	0.39%	0.034%
73	16.784	2337	2340	2342	rVV	1372	1453	0.35%	0.031%
74	16.843	2346	2350	2351	rBV2	1103	1269	0.30%	0.027%
75	16.890	2357	2358	2360	rBV	1818	1361	0.32%	0.029%
76	17.031	2378	2382	2383	rBV2	1291	1217	0.29%	0.026%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083021\
 Data File : BG050037.D
 Acq On : 30 Aug 2021 18:27
 Operator : CG/JU
 Sample : M3458-19
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0B64

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
 Title : SVOA CALIBRATION

77	17.119	2393	2397	2400	rBV3	4360	5998	1.43%	0.127%
78	17.172	2402	2406	2414	rVB4	2872	5258	1.26%	0.111%
79	17.377	2435	2441	2447	rBV	261198	409716	97.82%	8.667%
80	17.477	2452	2458	2466	rVB	220916	338928	80.92%	7.170%
81	17.636	2484	2485	2487	rBV	1377	1245	0.30%	0.026%
82	17.653	2487	2488	2492	rVB2	2779	2096	0.50%	0.044%
83	17.700	2494	2496	2499	rBV2	2457	2586	0.62%	0.055%
84	17.853	2519	2522	2526	rBV3	5947	7101	1.70%	0.150%
85	17.976	2541	2543	2545	rBV2	2247	1790	0.43%	0.038%
86	18.029	2549	2552	2556	rVB2	11253	13135	3.14%	0.278%
87	18.106	2562	2565	2566	rBV3	1785	1405	0.34%	0.030%
88	18.194	2579	2580	2582	rBV2	2415	1362	0.33%	0.029%
89	18.211	2582	2583	2585	rBV2	2291	1365	0.33%	0.029%
90	18.241	2587	2588	2589	rBV2	2524	1497	0.36%	0.032%
91	18.258	2589	2591	2592	rBV2	2445	1563	0.37%	0.033%
92	18.311	2597	2600	2602	rBV4	3108	4484	1.07%	0.095%
93	18.440	2619	2622	2625	rBV5	3783	5022	1.20%	0.106%
94	18.546	2636	2640	2643	rBV4	5740	7667	1.83%	0.162%
95	18.799	2682	2683	2685	rBV2	3430	1813	0.43%	0.038%
96	19.046	2724	2725	2727	rBV2	4214	2637	0.63%	0.056%
97	19.439	2788	2792	2795	rVB2	14384	18998	4.54%	0.402%
98	19.768	2843	2848	2858	rVB2	248377	378795	90.44%	8.013%
99	21.654	3163	3169	3175	rBV2	239960	387219	92.45%	8.191%
100	24.879	3712	3718	3728	rVB	152707	418846	100.00%	8.861%




Sum of corrected areas: 4727085

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083021\
Data File : BG050037.D
Acq On : 30 Aug 2021 18:27
Operator : CG/JU
Sample : M3458-19
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0B64

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

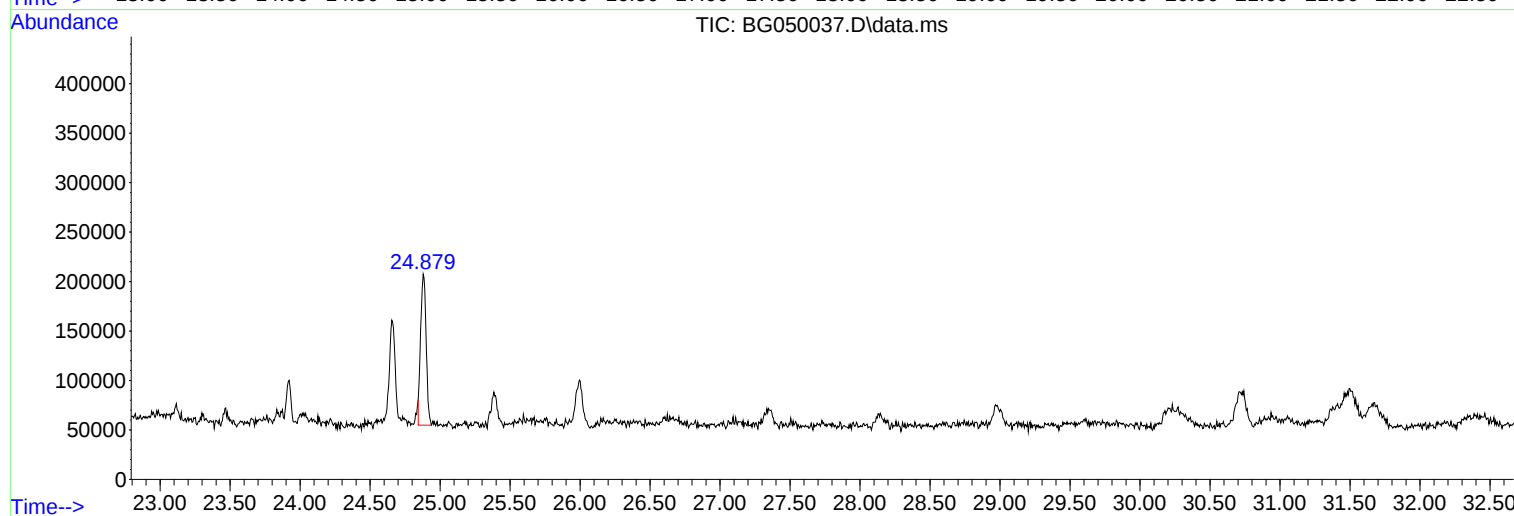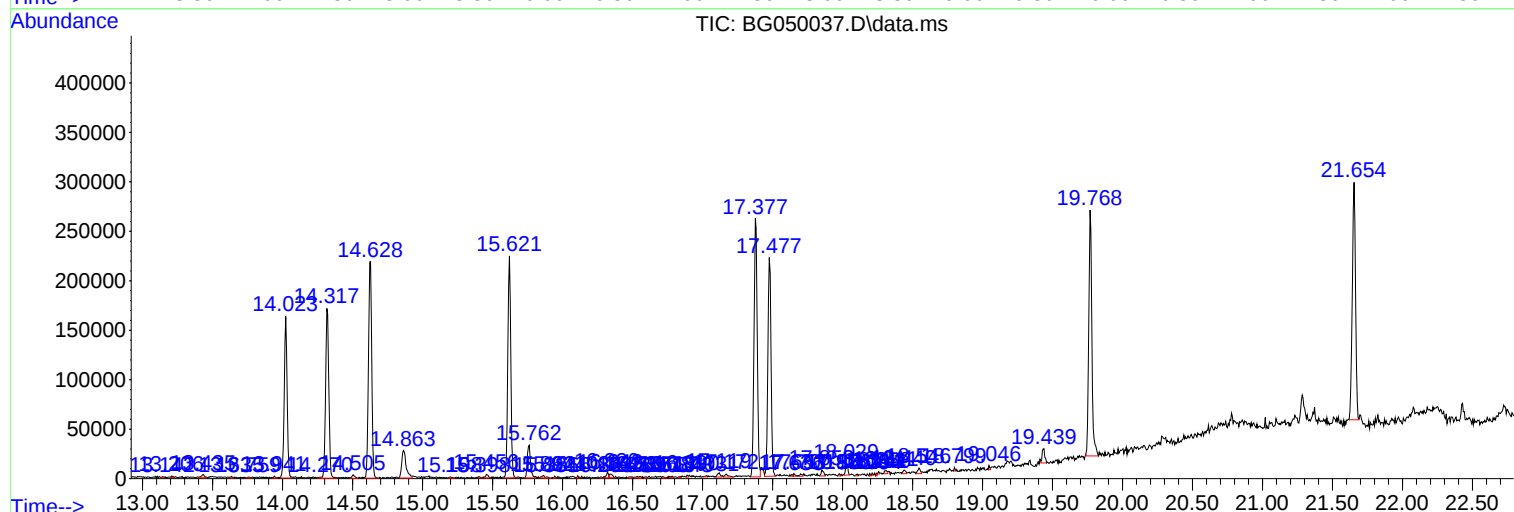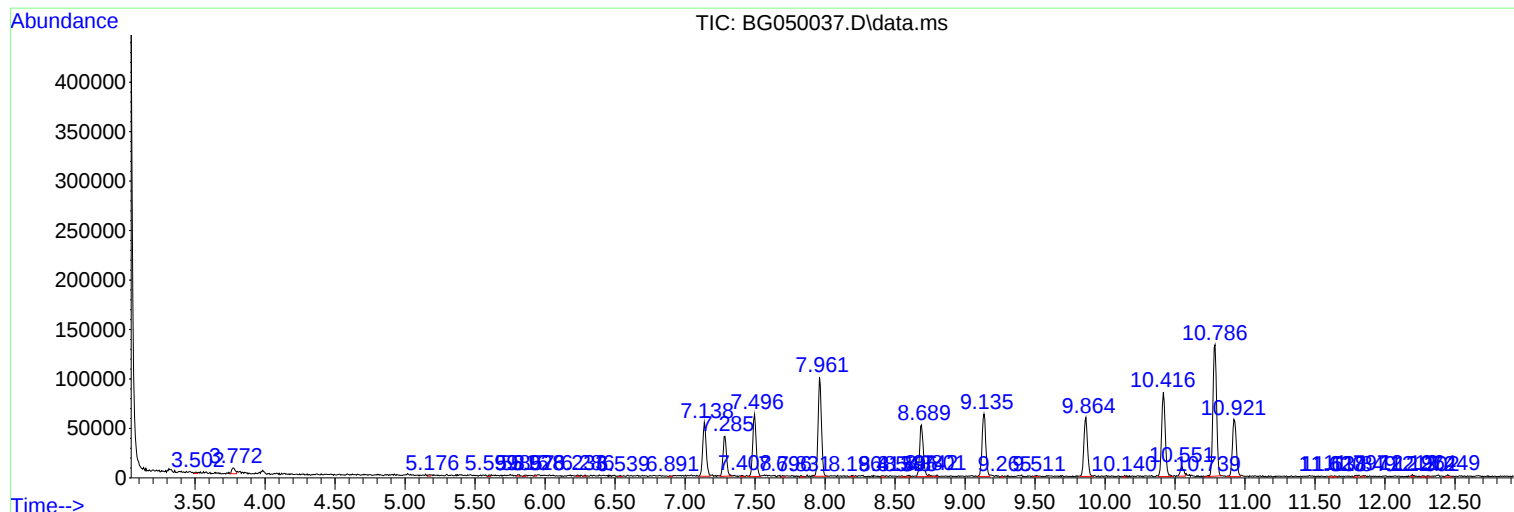

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083021\
Data File : BG050037.D
Acq On : 30 Aug 2021 18:27
Operator : CG/JU
Sample : M3458-19
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0B64

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083021\
Data File : BG050037.D
Acq On : 30 Aug 2021 18:27
Operator : CG/JU
Sample : M3458-19
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0B64

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
