

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083021\
 Data File : BG050041.D
 Acq On : 30 Aug 2021 21:54
 Operator : CG/JU
 Sample : M3472-06
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AX0

Integration Parameters: LSCINT.P

Integrator: RTE

Soothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
 Title : SVOA CALIBRATION

Signal : TIC: BG050041.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.316	45	47	53	rVB5	3687	5389	1.32%	0.134%
2	3.457	69	71	72	rVV2	2186	993	0.24%	0.025%
3	3.762	120	123	130	rBV3	12230	20419	5.01%	0.507%
4	3.980	158	160	166	rVB4	3326	3350	0.82%	0.083%
5	4.356	223	224	226	rBV2	1633	1146	0.28%	0.028%
6	4.878	311	313	315	rBV2	1198	1343	0.33%	0.033%
7	5.019	335	337	341	rVB4	2374	2827	0.69%	0.070%
8	5.548	424	427	429	rBV3	1627	2218	0.54%	0.055%
9	5.648	442	444	447	rVB2	1537	1188	0.29%	0.030%
10	6.564	598	600	603	rBV2	1154	1123	0.28%	0.028%
11	6.717	624	626	629	rVB3	947	1044	0.26%	0.026%
12	6.852	646	649	651	rBV2	1466	1730	0.42%	0.043%
13	7.134	692	697	707	rVB2	41464	74837	18.36%	1.859%
14	7.287	717	723	730	rBV2	25516	45253	11.10%	1.124%
15	7.493	753	758	769	rVB	40917	73529	18.04%	1.827%
16	7.575	769	772	773	rBV2	1937	1903	0.47%	0.047%
17	7.616	776	779	781	rBV2	1095	1015	0.25%	0.025%
18	7.963	830	838	845	rBV	92466	158266	38.83%	3.932%
19	8.262	887	889	892	rBV2	799	999	0.25%	0.025%
20	8.327	898	900	904	rVB2	1261	1818	0.45%	0.045%
21	8.421	914	916	918	rVB	1413	1356	0.33%	0.034%
22	8.450	918	921	925	rBV3	888	1475	0.36%	0.037%
23	8.685	955	961	969	rBV3	50335	89329	21.91%	2.220%
24	8.797	977	980	985	rBV2	2704	3892	0.95%	0.097%
25	9.079	1024	1028	1030	rBV2	777	1087	0.27%	0.027%
26	9.132	1030	1037	1046	rBV2	41805	75584	18.54%	1.878%
27	9.284	1062	1063	1066	rBV2	814	1025	0.25%	0.025%
28	9.437	1087	1089	1092	rVB2	1505	1728	0.42%	0.043%
29	9.766	1144	1145	1149	rVV	1713	1226	0.30%	0.030%
30	9.807	1149	1152	1155	rVV2	792	1270	0.31%	0.032%
31	9.860	1155	1161	1170	rVB2	39365	70035	17.18%	1.740%
32	10.101	1199	1202	1205	rBV2	899	1219	0.30%	0.030%
33	10.171	1211	1214	1216	rBV2	1049	1314	0.32%	0.033%
34	10.224	1220	1223	1225	rVV2	1703	1471	0.36%	0.037%
35	10.330	1238	1241	1243	rBV2	929	1384	0.34%	0.034%
36	10.418	1250	1256	1263	rBV	51738	95227	23.36%	2.366%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083021\
 Data File : BG050041.D
 Acq On : 30 Aug 2021 21:54
 Operator : CG/JU
 Sample : M3472-06
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AX0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
 Title : SVOA CALIBRATION

37	10.483	1266	1267	1271	rVB3	1291	1137	0.28%	0.028%
38	10.782	1311	1318	1330	rVB	121997	228434	56.04%	5.676%
39	10.923	1336	1342	1351	rVV2	44397	86082	21.12%	2.139%
40	11.029	1358	1360	1363	rBV	1070	1067	0.26%	0.027%
41	11.305	1406	1407	1411	rVB	1329	1197	0.29%	0.030%
42	11.857	1499	1501	1505	rBV	1271	1638	0.40%	0.041%
43	11.963	1516	1519	1521	rVB	1258	1421	0.35%	0.035%
44	12.180	1554	1556	1558	rVB2	1074	995	0.24%	0.025%
45	12.374	1586	1589	1592	rBV2	866	1034	0.25%	0.026%
46	13.314	1747	1749	1751	rBV	1367	1391	0.34%	0.035%
47	14.019	1863	1869	1876	rBV	101170	146678	35.98%	3.644%
48	14.319	1914	1920	1928	rBV	114007	173695	42.61%	4.316%
49	14.424	1936	1938	1943	rVB	733	1093	0.27%	0.027%
50	14.483	1945	1948	1949	rBV	1309	1047	0.26%	0.026%
51	14.624	1965	1972	1980	rVB	218555	332711	81.62%	8.267%
52	14.865	2008	2013	2026	rBV4	22076	47029	11.54%	1.169%
53	15.047	2041	2044	2046	rVB	1408	1423	0.35%	0.035%
54	15.200	2065	2070	2072	rVB	1022	1460	0.36%	0.036%
55	15.229	2072	2075	2079	rBV2	1070	1532	0.38%	0.038%
56	15.317	2089	2090	2094	rBV	1210	1245	0.31%	0.031%
57	15.370	2094	2099	2102	rVB3	1223	1970	0.48%	0.049%
58	15.617	2135	2141	2152	rVB	142035	218767	53.67%	5.436%
59	15.758	2162	2165	2173	rVB3	11179	15774	3.87%	0.392%
60	15.852	2180	2181	2185	rBV2	1221	1333	0.33%	0.033%
61	15.905	2187	2190	2192	rVB	1498	1083	0.27%	0.027%
62	16.375	2268	2270	2274	rBV	681	1100	0.27%	0.027%
63	16.833	2345	2348	2350	rBV	828	1277	0.31%	0.032%
64	16.968	2369	2371	2376	rVB3	1295	1895	0.46%	0.047%
65	17.038	2380	2383	2390	rBV3	1441	2949	0.72%	0.073%
66	17.115	2393	2396	2399	rVB	1256	1614	0.40%	0.040%
67	17.379	2433	2441	2447	rBV	277255	407638	100.00%	10.128%
68	17.420	2447	2448	2452	rVV	5035	4259	1.04%	0.106%
69	17.479	2452	2458	2465	rVB	153737	236039	57.90%	5.865%
70	17.561	2470	2472	2475	rBV	1234	1222	0.30%	0.030%
71	17.661	2486	2489	2490	rVB	1385	993	0.24%	0.025%
72	17.755	2503	2505	2508	rVB	2069	1567	0.38%	0.039%
73	17.790	2508	2511	2515	rBV2	1731	2277	0.56%	0.057%
74	17.961	2536	2540	2541	rBV2	962	1005	0.25%	0.025%
75	18.014	2546	2549	2552	rBV	2002	2460	0.60%	0.061%
76	18.037	2552	2553	2555	rVB2	3049	1631	0.40%	0.041%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083021\
 Data File : BG050041.D
 Acq On : 30 Aug 2021 21:54
 Operator : CG/JU
 Sample : M3472-06
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AX0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
 Title : SVOA CALIBRATION

77	18.067	2555	2558	2560	rBV2	1549	1514	0.37%	0.038%
78	18.172	2573	2576	2577	rBV2	1654	1638	0.40%	0.041%
79	18.202	2577	2581	2582	rVV3	1109	1023	0.25%	0.025%
80	18.243	2587	2588	2590	rBV	2116	1161	0.28%	0.029%
81	18.266	2590	2592	2595	rBV	1237	1441	0.35%	0.036%
82	18.331	2595	2603	2604	rBV4	1941	3840	0.94%	0.095%
83	18.360	2606	2608	2612	rVB	1536	1524	0.37%	0.038%
84	18.390	2612	2613	2615	rBV2	1237	1008	0.25%	0.025%
85	18.437	2620	2621	2624	rBV2	1637	1706	0.42%	0.042%
86	18.478	2626	2628	2630	rVB2	2294	1773	0.43%	0.044%
87	18.507	2632	2633	2637	rVB2	1078	1068	0.26%	0.027%
88	18.719	2667	2669	2672	rBV3	1610	1333	0.33%	0.033%
89	18.742	2672	2673	2675	rVV2	2530	1691	0.41%	0.042%
90	18.777	2677	2679	2681	rVV	1437	1293	0.32%	0.032%
91	18.813	2683	2685	2688	rVB2	1845	1882	0.46%	0.047%
92	19.001	2715	2717	2720	rVB2	2067	1867	0.46%	0.046%
93	19.065	2724	2728	2732	rBV4	2168	3719	0.91%	0.092%
94	19.106	2732	2735	2736	rBV3	1670	1786	0.44%	0.044%
95	19.271	2762	2763	2765	rBV2	2425	2082	0.51%	0.052%
96	19.324	2770	2772	2777	rVV6	2404	4034	0.99%	0.100%
97	19.770	2842	2848	2858	rBV	189697	277510	68.08%	6.895%
98	21.650	3162	3168	3174	rBV	235912	377273	92.55%	9.374%
99	24.658	3673	3680	3690	rVB2	97767	254685	62.48%	6.328%
100	24.881	3710	3718	3726	rVB2	143154	389660	95.59%	9.682%




Sum of corrected areas: 4024685

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083021\
Data File : BG050041.D
Acq On : 30 Aug 2021 21:54
Operator : CG/JU
Sample : M3472-06
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AX0

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

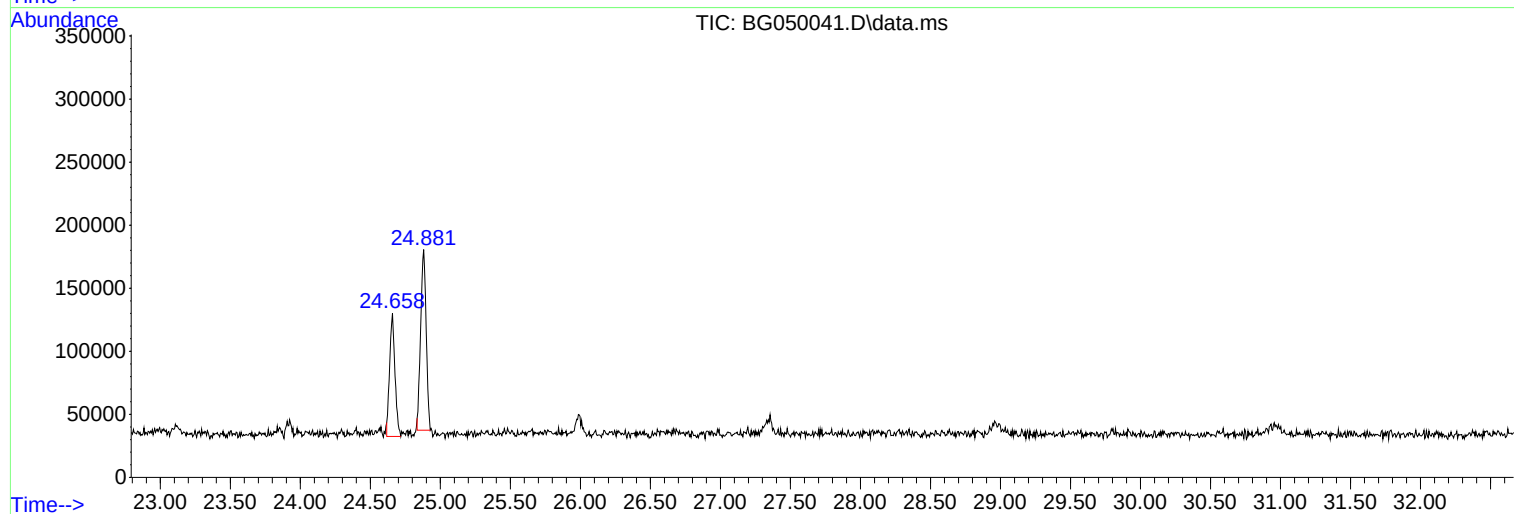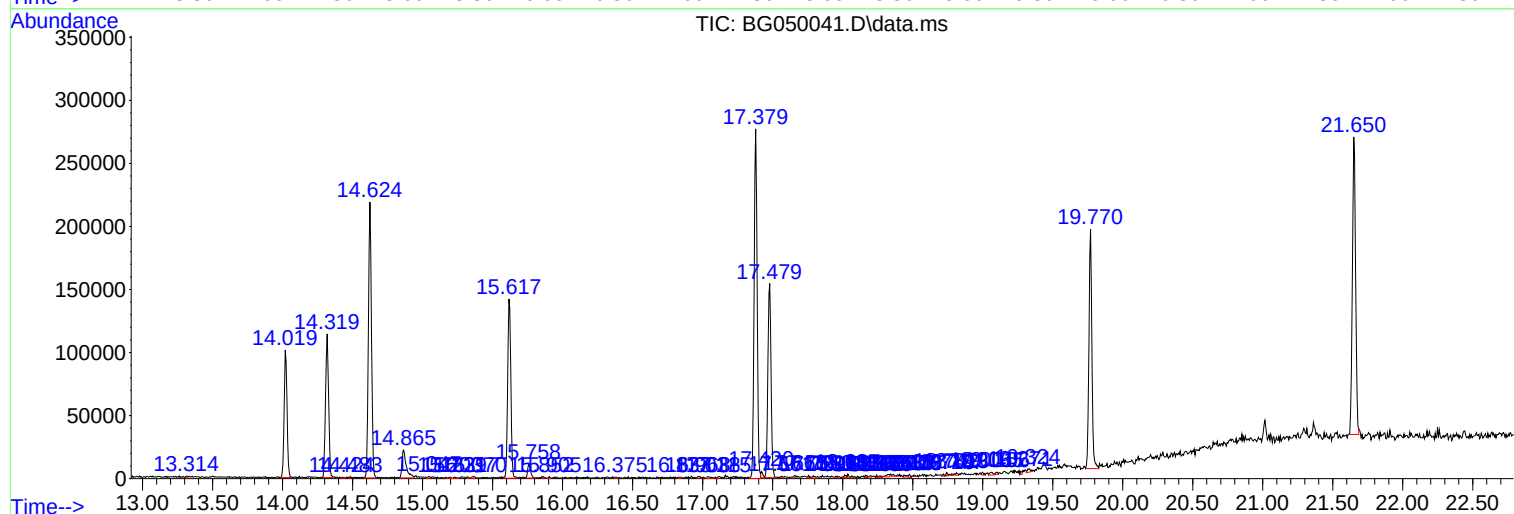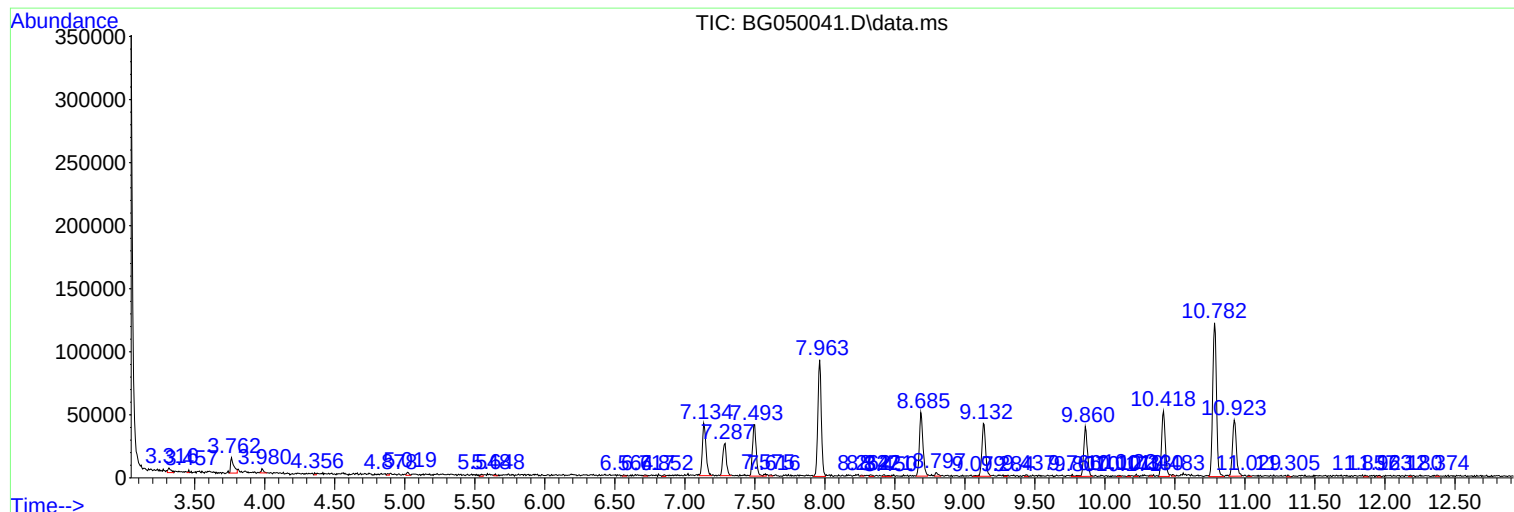

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083021\
Data File : BG050041.D
Acq On : 30 Aug 2021 21:54
Operator : CG/JU
Sample : M3472-06
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AX0

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083021\
Data File : BG050041.D
Acq On : 30 Aug 2021 21:54
Operator : CG/JU
Sample : M3472-06
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AX0

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
