

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083021\
 Data File : BG050048.D
 Acq On : 31 Aug 2021 3:23
 Operator : CG/JU
 Sample : M3472-07
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0B89

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
 Title : SVOA CALIBRATION

Signal : TIC: BG050048.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.314	45	47	52	rVB5	3944	5670	0.72%	0.083%
2	3.619	97	99	104	rVB3	1604	1759	0.22%	0.026%
3	3.754	119	122	135	rBV	26560	57211	7.30%	0.834%
4	3.977	156	160	163	rBV3	6096	7192	0.92%	0.105%
5	4.459	241	242	245	rBV2	1353	1567	0.20%	0.023%
6	4.653	274	275	282	rBV5	1614	2809	0.36%	0.041%
7	4.859	306	310	313	rVB3	1245	1753	0.22%	0.026%
8	4.964	326	328	333	rVB3	1692	2652	0.34%	0.039%
9	5.023	333	338	343	rBV5	2549	6108	0.78%	0.089%
10	5.505	417	420	422	rBV	1846	1416	0.18%	0.021%
11	5.534	423	425	428	rVB3	1635	1573	0.20%	0.023%
12	5.563	428	430	432	rBV	1634	1780	0.23%	0.026%
13	5.751	460	462	464	rBV	1663	1771	0.23%	0.026%
14	7.132	691	697	710	rVB	107091	198990	25.40%	2.901%
15	7.285	717	723	731	rBV	61904	112186	14.32%	1.636%
16	7.355	734	735	740	rVB3	1844	1754	0.22%	0.026%
17	7.496	752	759	767	rVV	103296	181521	23.17%	2.646%
18	7.567	768	771	775	rVV3	2831	3957	0.51%	0.058%
19	7.614	777	779	782	rVV2	1716	1753	0.22%	0.026%
20	7.666	786	788	791	rBV2	1491	1549	0.20%	0.023%
21	7.960	831	838	847	rVV	118573	200757	25.63%	2.927%
22	8.025	847	849	852	rVB2	1458	1342	0.17%	0.020%
23	8.683	955	961	973	rVB	120549	217199	27.73%	3.167%
24	9.135	1031	1038	1045	rBV	100728	186971	23.87%	2.726%
25	9.188	1045	1047	1052	rVB4	4699	5402	0.69%	0.079%
26	9.276	1060	1062	1066	rVV2	1568	1779	0.23%	0.026%
27	9.317	1066	1069	1076	rVB3	1404	2767	0.35%	0.040%
28	9.864	1154	1162	1170	rBV	99718	178084	22.74%	2.596%
29	10.416	1249	1256	1263	rBV	146130	276006	35.24%	4.024%
30	10.545	1273	1278	1285	rBV2	10184	18229	2.33%	0.266%
31	10.627	1289	1292	1295	rVB2	1775	1717	0.22%	0.025%
32	10.780	1306	1318	1332	rBV	153593	295248	37.69%	4.304%
33	10.921	1336	1342	1351	rVV	59844	113316	14.47%	1.652%
34	11.485	1434	1438	1439	rBV	1345	1349	0.17%	0.020%
35	12.190	1552	1558	1563	rBV2	21948	31710	4.05%	0.462%
36	12.378	1585	1590	1594	rBV3	3352	4133	0.53%	0.060%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083021\
 Data File : BG050048.D
 Acq On : 31 Aug 2021 3:23
 Operator : CG/JU
 Sample : M3472-07
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0B89

Integration Parameters: LSCINT.P

Integrator: RTE

Soothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
 Title : SVOA CALIBRATION

37	12.807	1659	1663	1664	rBV	1039	1335	0.17%	0.019%
38	12.889	1675	1677	1680	rVB2	1328	1421	0.18%	0.021%
39	12.924	1680	1683	1685	rBV	925	1343	0.17%	0.020%
40	12.989	1692	1694	1695	rBV	2476	1558	0.20%	0.023%
41	13.006	1695	1697	1700	rVV2	2903	3389	0.43%	0.049%
42	13.036	1700	1702	1705	rVV	1429	1559	0.20%	0.023%
43	13.089	1709	1711	1713	rVB2	1924	1439	0.18%	0.021%
44	13.224	1725	1734	1739	rVB3	1532	3823	0.49%	0.056%
45	13.429	1765	1769	1778	rBV4	7374	13124	1.68%	0.191%
46	13.506	1778	1782	1784	rBV3	1679	1915	0.24%	0.028%
47	13.887	1845	1847	1849	rBV	1404	1421	0.18%	0.021%
48	13.940	1852	1856	1861	rVB4	2126	3127	0.40%	0.046%
49	14.023	1861	1870	1876	rBV	277181	411556	52.54%	6.000%
50	14.128	1886	1888	1892	rVB	1714	2008	0.26%	0.029%
51	14.187	1894	1898	1900	rBV2	1561	2292	0.29%	0.033%
52	14.252	1905	1909	1911	rBV	1444	1715	0.22%	0.025%
53	14.316	1913	1920	1929	rVB	289492	468168	59.77%	6.825%
54	14.504	1948	1952	1957	rBV3	8620	11521	1.47%	0.168%
55	14.622	1963	1972	1980	rVB	252315	401606	51.27%	5.855%
56	14.710	1983	1987	1989	rVB2	1591	1922	0.25%	0.028%
57	14.857	2006	2012	2027	rBV2	90724	182100	23.25%	2.655%
58	14.980	2030	2033	2039	rVB7	7302	10892	1.39%	0.159%
59	15.103	2052	2054	2058	rBV	1689	1742	0.22%	0.025%
60	15.291	2083	2086	2087	rBV3	2093	2091	0.27%	0.030%
61	15.356	2094	2097	2100	rVB3	1584	1334	0.17%	0.019%
62	15.415	2103	2107	2108	rVV4	1454	1691	0.22%	0.025%
63	15.456	2111	2114	2119	rVB2	10112	13748	1.76%	0.200%
64	15.497	2119	2121	2123	rBV2	1835	2160	0.28%	0.031%
65	15.620	2133	2142	2149	rBV	390819	593702	75.80%	8.656%
66	15.756	2160	2165	2175	rVV2	76322	116030	14.81%	1.692%
67	15.855	2179	2182	2186	rBV3	4489	6098	0.78%	0.089%
68	15.967	2196	2201	2203	rBV2	1687	3124	0.40%	0.046%
69	16.079	2217	2220	2223	rVB3	1929	2411	0.31%	0.035%
70	16.319	2256	2261	2264	rBV3	8953	13440	1.72%	0.196%
71	16.402	2273	2275	2279	rVB5	1739	1753	0.22%	0.026%
72	16.460	2282	2285	2286	rBV	1593	1590	0.20%	0.023%
73	16.572	2302	2304	2305	rBV2	1911	1351	0.17%	0.020%
74	16.613	2308	2311	2314	rBV	1769	2404	0.31%	0.035%
75	16.672	2318	2321	2322	rBV	2013	1912	0.24%	0.028%
76	16.713	2327	2328	2329	rBV	2943	1347	0.17%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083021\
 Data File : BG050048.D
 Acq On : 31 Aug 2021 3:23
 Operator : CG/JU
 Sample : M3472-07
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0B89

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
 Title : SVOA CALIBRATION

77	16.778	2338	2339	2342	rVB2	1797	1361	0.17%	0.020%
78	16.831	2342	2348	2351	rBV3	2140	4434	0.57%	0.065%
79	17.001	2376	2377	2381	rBV3	1137	1606	0.21%	0.023%
80	17.118	2391	2397	2400	rBV4	9067	15914	2.03%	0.232%
81	17.265	2420	2422	2425	rBV2	3086	3794	0.48%	0.055%
82	17.377	2435	2441	2447	rBV	286261	435415	55.59%	6.348%
83	17.424	2447	2449	2452	rVV	10503	10627	1.36%	0.155%
84	17.477	2452	2458	2467	rVB	470101	694055	88.61%	10.119%
85	17.600	2477	2479	2481	rVB3	3635	2898	0.37%	0.042%
86	17.718	2498	2499	2502	rBV3	2721	2012	0.26%	0.029%
87	17.759	2502	2506	2507	rBV4	1772	2213	0.28%	0.032%
88	17.859	2519	2523	2527	rBV3	9082	11932	1.52%	0.174%
89	18.029	2550	2552	2554	rVB3	6222	4804	0.61%	0.070%
90	18.111	2565	2566	2569	rBV3	2859	2576	0.33%	0.038%
91	18.141	2569	2571	2574	rVB3	3001	2648	0.34%	0.039%
92	18.299	2596	2598	2600	rBV3	4530	3875	0.49%	0.056%
93	18.481	2628	2629	2630	rBV	5617	2905	0.37%	0.042%
94	18.546	2636	2640	2644	rBV5	9053	14664	1.87%	0.214%
95	18.734	2670	2672	2673	rBV	3471	1453	0.19%	0.021%
96	19.004	2717	2718	2719	rBV	5157	1865	0.24%	0.027%
97	19.180	2743	2748	2750	rBV5	12447	21701	2.77%	0.316%
98	19.433	2789	2791	2796	rVB	23913	30551	3.90%	0.445%
99	19.768	2843	2848	2857	rBV	523304	783293	100.00%	11.420%
100	21.653	3164	3169	3175	rVB	236703	374374	47.79%	5.458%




Sum of corrected areas: 6859112

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083021\
Data File : BG050048.D
Acq On : 31 Aug 2021 3:23
Operator : CG/JU
Sample : M3472-07
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0B89

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

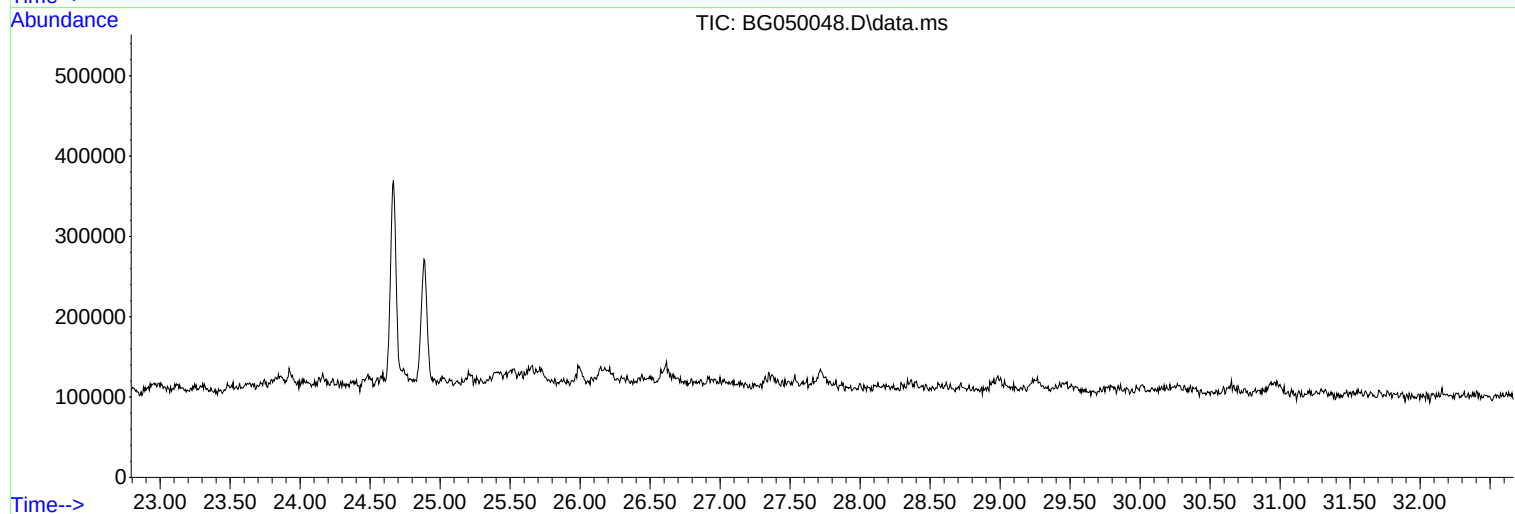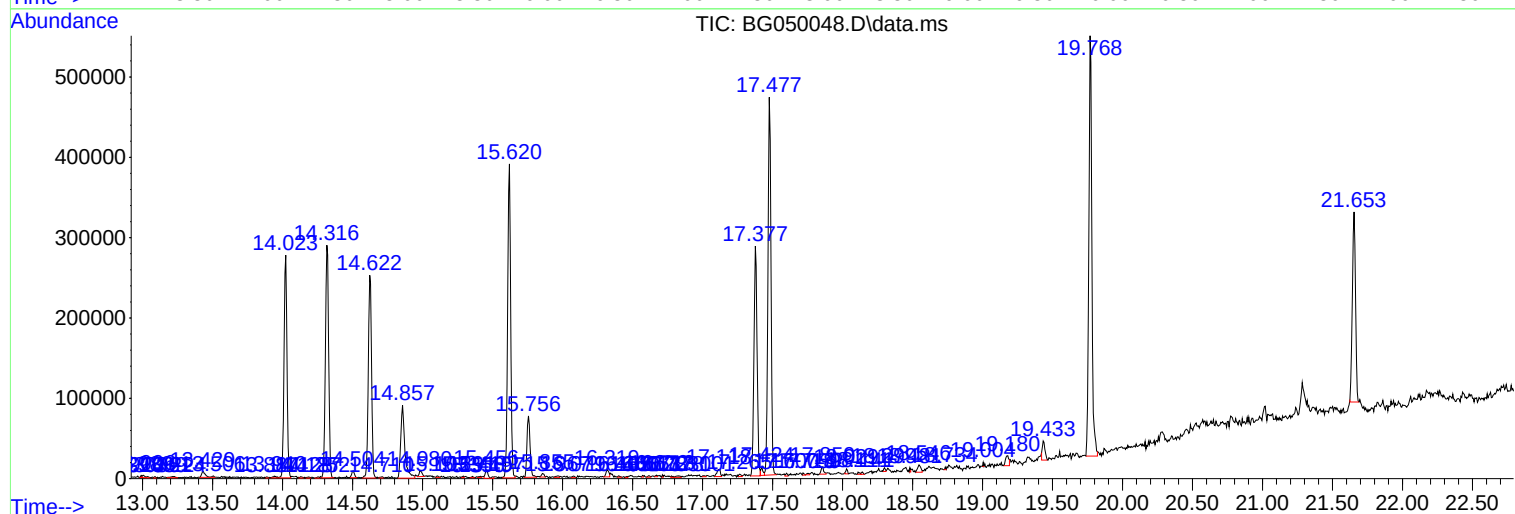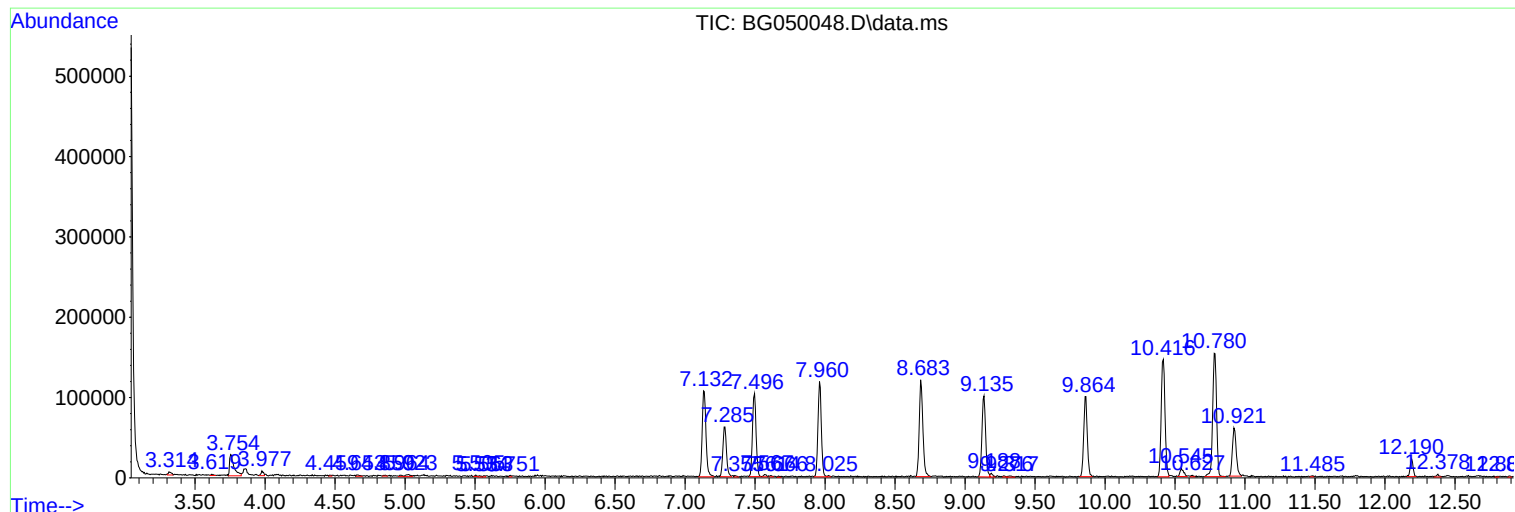

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083021\
Data File : BG050048.D
Acq On : 31 Aug 2021 3:23
Operator : CG/JU
Sample : M3472-07
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0B89










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
12.190	2.15 ng/ul	31710	Naphthalene-d8	10.786

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Dodecane	170	C12H26	000112-40-3	90
2			Carbonic acid, dodecyl vinyl ester	256	C15H28O3	1000382-54-8	83
3			Octadecane, 1-chloro-	288	C18H37Cl	003386-33-2	83
4			Tetradecane	198	C14H30	000629-59-4	78
5			Hexadecane, 1-chloro-	260	C16H33Cl	004860-03-1	72

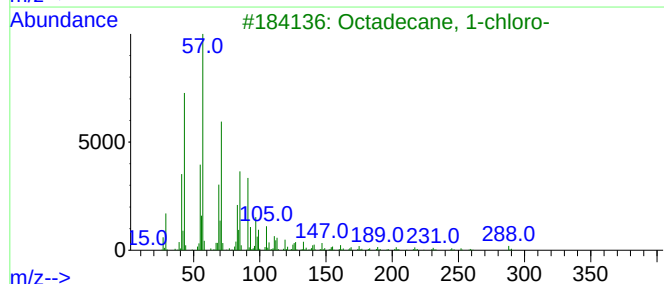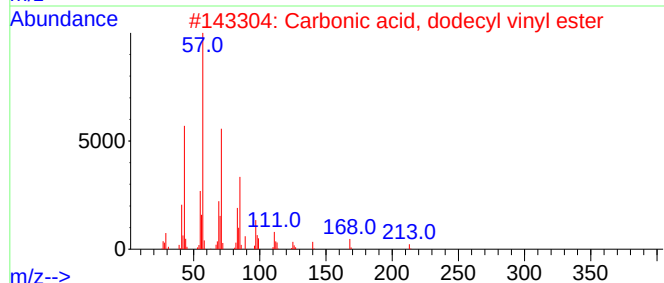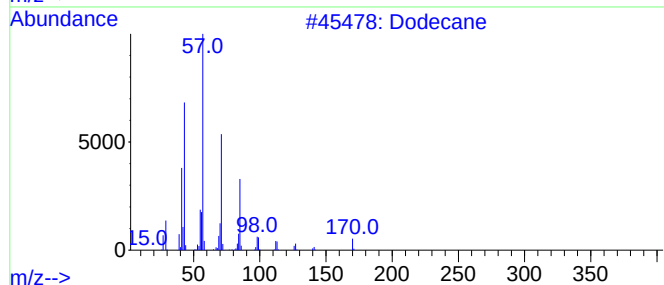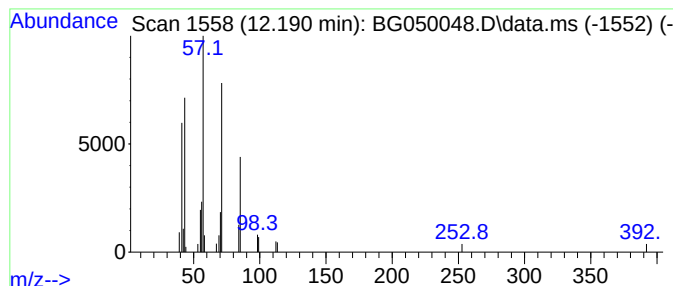

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083021\
Data File : BG050048.D
Acq On : 31 Aug 2021 3:23
Operator : CG/JU
Sample : M3472-07
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0B89

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	12.190	2.1	ng/ul	31710	2	10.786	295248	20.0