

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083021\
 Data File : BG050050.D
 Acq On : 31 Aug 2021 4:45
 Operator : CG/JU
 Sample : M3448-21
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBKG6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
 Title : SVOA CALIBRATION

Signal : TIC: BG050050.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.313	43	47	51	rBV4	5450	8256	1.08%	0.094%
2	3.754	119	122	134	rBV	17842	38525	5.06%	0.438%
3	3.971	157	159	160	rBV2	2831	1743	0.23%	0.020%
4	5.287	381	383	391	rVB3	1435	2489	0.33%	0.028%
5	7.138	693	698	706	rBV2	25862	50882	6.69%	0.578%
6	7.284	716	723	731	rBV	80691	136635	17.95%	1.552%
7	7.496	753	759	769	rBV	100628	174388	22.91%	1.981%
8	7.960	831	838	848	rBV	115488	193985	25.49%	2.204%
9	8.077	855	858	860	rBV2	1571	1743	0.23%	0.020%
10	8.688	956	962	972	rVB	79843	142406	18.71%	1.618%
11	8.818	981	984	987	rBV3	1408	1986	0.26%	0.023%
12	9.135	1029	1038	1045	rBV	127358	236603	31.09%	2.688%
13	9.382	1077	1080	1083	rBV2	1000	1576	0.21%	0.018%
14	9.452	1087	1092	1097	rBV2	2418	4622	0.61%	0.053%
15	9.528	1102	1105	1108	rVB2	1469	1900	0.25%	0.022%
16	9.863	1155	1162	1171	rVB	118696	213331	28.03%	2.423%
17	10.039	1190	1192	1197	rVB	1111	1516	0.20%	0.017%
18	10.098	1197	1202	1205	rBV3	1576	1945	0.26%	0.022%
19	10.180	1212	1216	1224	rBV2	1941	4133	0.54%	0.047%
20	10.415	1249	1256	1265	rBV	154767	275473	36.19%	3.129%
21	10.786	1312	1319	1323	rVV	151387	272646	35.82%	3.097%
22	10.832	1323	1327	1335	rVV	180917	321102	42.19%	3.648%
23	10.926	1336	1343	1356	rVB2	126435	271594	35.68%	3.085%
24	11.144	1376	1380	1385	rVB4	2244	4462	0.59%	0.051%
25	12.342	1578	1584	1588	rBV4	5947	9066	1.19%	0.103%
26	12.377	1588	1590	1597	rVB4	3951	5131	0.67%	0.058%
27	12.665	1630	1639	1646	rVB	61290	107017	14.06%	1.216%
28	13.358	1756	1757	1761	rVB3	1522	1600	0.21%	0.018%
29	13.452	1767	1773	1778	rBV2	16259	26129	3.43%	0.297%
30	13.499	1778	1781	1786	rVB5	4471	6671	0.88%	0.076%
31	13.588	1793	1796	1802	rVB2	1344	1694	0.22%	0.019%
32	13.676	1809	1811	1817	rVB3	2080	2934	0.39%	0.033%
33	13.799	1829	1832	1835	rBV4	1532	1687	0.22%	0.019%
34	13.940	1849	1856	1862	rBV3	12323	22133	2.91%	0.251%
35	14.022	1862	1870	1875	rVV	325296	480650	63.15%	5.460%
36	14.069	1875	1878	1883	rVB	60438	81122	10.66%	0.922%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083021\
 Data File : BG050050.D
 Acq On : 31 Aug 2021 4:45
 Operator : CG/JU
 Sample : M3448-21
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBKG6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
 Title : SVOA CALIBRATION

37	14.181	1893	1897	1899	rBV4	5271	5801	0.76%	0.066%
38	14.322	1913	1921	1933	rBV	326182	540477	71.01%	6.140%
39	14.627	1963	1973	1978	rBV	239976	379096	49.81%	4.307%
40	14.692	1978	1984	1991	rVB	147481	231945	30.48%	2.635%

41	14.762	1991	1996	2002	rBV	12669	17591	2.31%	0.200%
42	14.868	2006	2014	2019	rBV3	18772	37785	4.96%	0.429%
43	15.027	2035	2041	2048	rVB	55614	87601	11.51%	0.995%
44	15.185	2064	2068	2072	rBV4	7687	10997	1.44%	0.125%
45	15.256	2075	2080	2081	rVV2	3063	4490	0.59%	0.051%

46	15.268	2081	2082	2086	rVB	4383	4065	0.53%	0.046%
47	15.362	2093	2098	2102	rBV3	8285	13670	1.80%	0.155%
48	15.409	2102	2106	2112	rVB4	2202	4032	0.53%	0.046%
49	15.620	2135	2142	2148	rBV	444278	674635	88.64%	7.664%
50	15.673	2148	2151	2159	rVB	61438	90155	11.85%	1.024%

51	15.761	2161	2166	2172	rBV2	86551	137371	18.05%	1.561%
52	15.855	2180	2182	2186	rVB3	2488	2365	0.31%	0.027%
53	15.896	2186	2189	2197	rVB3	9608	13868	1.82%	0.158%
54	15.967	2197	2201	2206	rVB3	4403	6848	0.90%	0.078%
55	16.114	2223	2226	2230	rVB3	4417	5301	0.70%	0.060%

56	16.190	2235	2239	2242	rBV	1388	1959	0.26%	0.022%
57	16.243	2245	2248	2250	rVB	1919	1855	0.24%	0.021%
58	16.290	2250	2256	2257	rBV	1661	2502	0.33%	0.028%
59	16.360	2259	2268	2272	rBV4	7581	14919	1.96%	0.169%
60	16.531	2295	2297	2301	rVB3	1319	1772	0.23%	0.020%

61	16.578	2301	2305	2306	rBV	1885	2315	0.30%	0.026%
62	16.648	2314	2317	2321	rBV	2713	4803	0.63%	0.055%
63	16.683	2321	2323	2325	rVB	2122	1530	0.20%	0.017%
64	16.736	2331	2332	2337	rVB3	2436	2899	0.38%	0.033%
65	16.824	2345	2347	2352	rVB2	2316	2264	0.30%	0.026%

66	16.918	2357	2363	2369	rVB	3866	8184	1.08%	0.093%
67	16.965	2369	2371	2372	rBV2	2045	1682	0.22%	0.019%
68	17.001	2375	2377	2378	rBV	2401	1970	0.26%	0.022%
69	17.042	2379	2384	2393	rVV4	37048	65079	8.55%	0.739%
70	17.171	2402	2406	2408	rBV	2696	4169	0.55%	0.047%

71	17.200	2409	2411	2414	rVV3	5876	5695	0.75%	0.065%
72	17.247	2417	2419	2421	rBV	3716	2512	0.33%	0.029%
73	17.330	2430	2433	2434	rBV	1631	1849	0.24%	0.021%
74	17.382	2436	2442	2446	rVV	274572	425199	55.87%	4.830%
75	17.424	2446	2449	2453	rVV	27441	41041	5.39%	0.466%

76	17.482	2453	2459	2468	rVB	501173	744824	97.86%	8.461%
----	--------	------	------	------	-----	--------	--------	--------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083021\
 Data File : BG050050.D
 Acq On : 31 Aug 2021 4:45
 Operator : CG/JU
 Sample : M3448-21
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBKG6

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
 Title : SVOA CALIBRATION

77	17.576	2473	2475	2480	rVB3	1765	2431	0.32%	0.028%
78	17.653	2482	2488	2492	rVB5	4034	6729	0.88%	0.076%
79	17.788	2499	2511	2516	rBV	73321	117775	15.47%	1.338%
80	17.899	2528	2530	2533	rVB2	2809	3135	0.41%	0.036%
81	17.929	2533	2535	2537	rBV3	2344	2027	0.27%	0.023%
82	17.999	2541	2547	2548	rBV5	5870	10010	1.32%	0.114%
83	18.035	2551	2553	2555	rVB3	4051	3821	0.50%	0.043%
84	18.099	2561	2564	2568	rVB4	3928	4774	0.63%	0.054%
85	18.140	2568	2571	2575	rBV3	2531	3985	0.52%	0.045%
86	18.181	2575	2578	2579	rVB3	4098	3787	0.50%	0.043%
87	18.199	2579	2581	2582	rBV2	1861	1723	0.23%	0.020%
88	18.305	2596	2599	2603	rBV2	8624	10201	1.34%	0.116%
89	18.340	2603	2605	2608	rVB3	3597	3694	0.49%	0.042%
90	18.369	2608	2610	2614	rVB5	3011	2310	0.30%	0.026%
91	18.557	2635	2642	2645	rBV6	5963	13449	1.77%	0.153%
92	18.610	2648	2651	2654	rVV3	6479	8108	1.07%	0.092%
93	18.640	2654	2656	2659	rVV4	2737	3097	0.41%	0.035%
94	18.798	2680	2683	2689	rBV8	5202	11560	1.52%	0.131%
95	18.916	2701	2703	2704	rBV2	4119	2705	0.36%	0.031%
96	19.204	2750	2752	2754	rBV2	5043	5598	0.74%	0.064%
97	19.327	2771	2773	2774	rBV2	8799	5523	0.73%	0.063%
98	19.773	2843	2849	2858	rVB	528687	761094	100.00%	8.646%
99	21.653	3164	3169	3181	rVB	230338	403589	53.03%	4.585%
100	24.667	3676	3682	3697	rVB2	252524	694858	91.30%	7.894%




Sum of corrected areas: 8802873

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083021\
Data File : BG050050.D
Acq On : 31 Aug 2021 4:45
Operator : CG/JU
Sample : M3448-21
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBKG6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

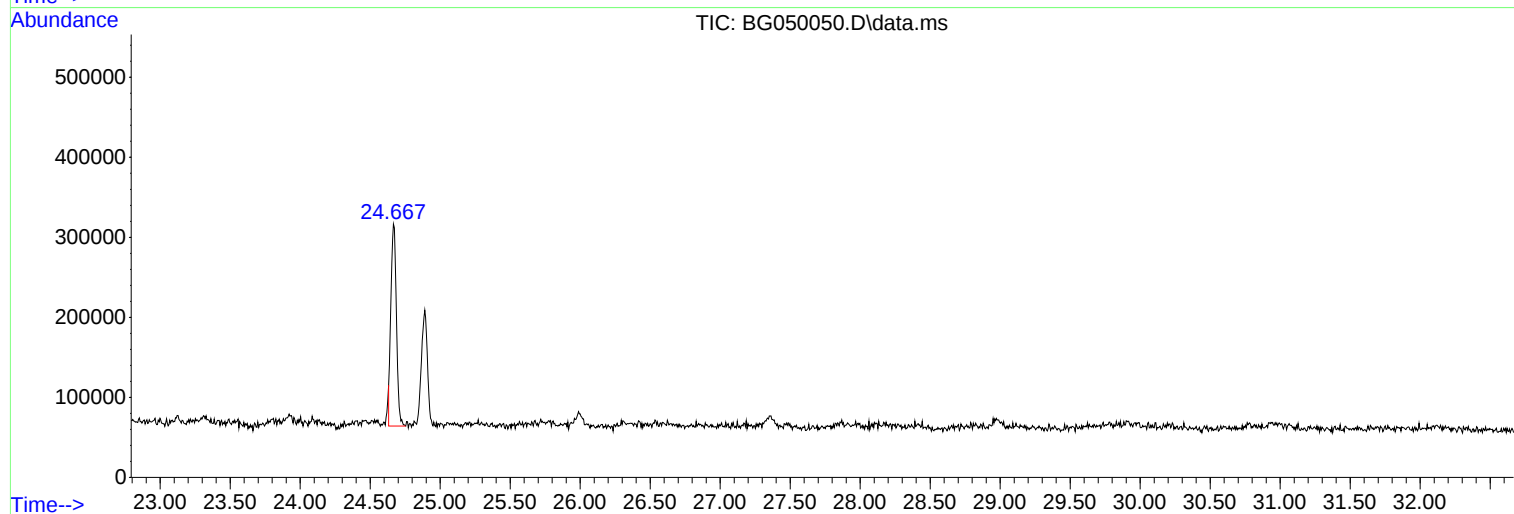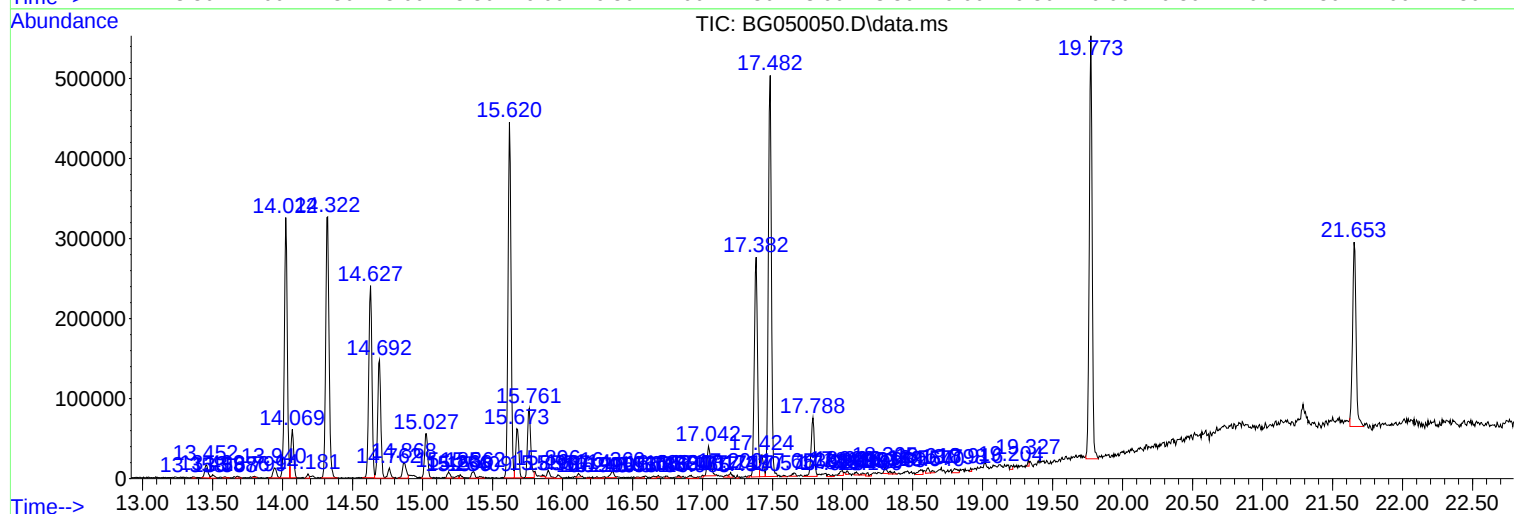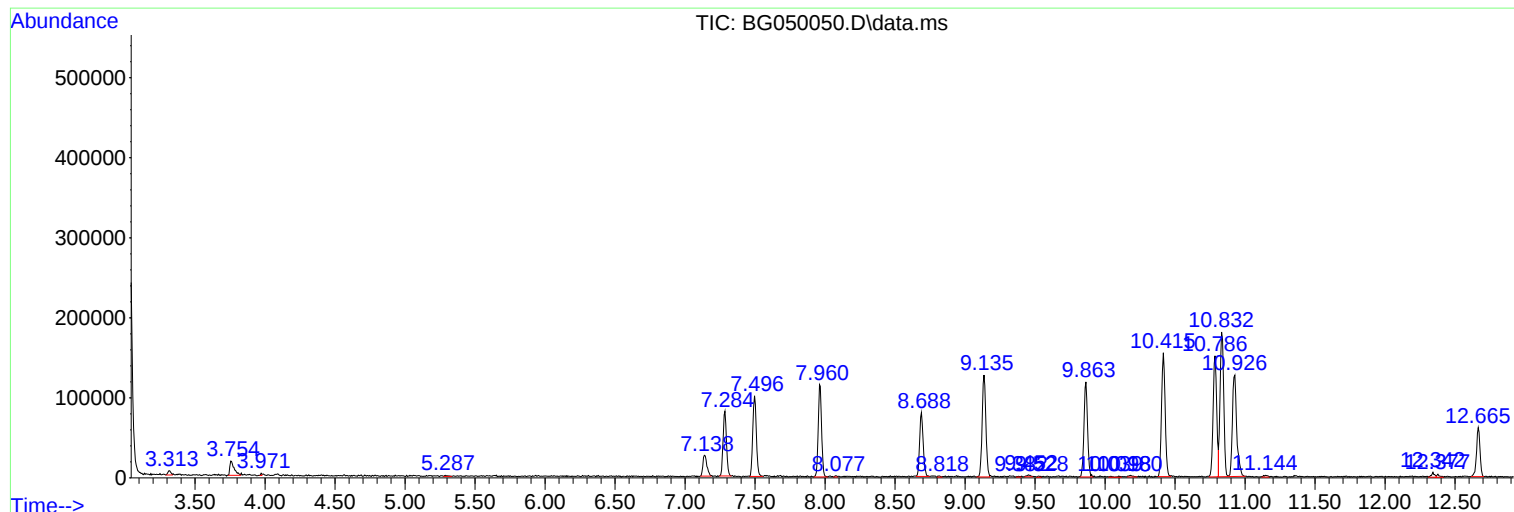

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083021\
Data File : BG050050.D
Acq On : 31 Aug 2021 4:45
Operator : CG/JU
Sample : M3448-21
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBKG6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083021\
Data File : BG050050.D
Acq On : 31 Aug 2021 4:45
Operator : CG/JU
Sample : M3448-21
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBKG6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
