

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083021\
 Data File : BG050053.D
 Acq On : 31 Aug 2021 6:49
 Operator : CG/JU
 Sample : M3464-02
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBKF5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
 Title : SVOA CALIBRATION

Signal : TIC: BG050053.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.191	24	26	29	rVB3	2592	1590	0.19%	0.019%
2	3.314	43	47	51	rBV4	5280	8217	0.98%	0.097%
3	3.391	57	60	61	rBV	2736	1908	0.23%	0.023%
4	3.749	118	121	131	rBV3	24825	52572	6.27%	0.621%
5	3.896	145	146	150	rVB3	1957	1357	0.16%	0.016%
6	4.025	166	168	170	rBV	1233	1361	0.16%	0.016%
7	4.084	175	178	180	rVB2	1771	1868	0.22%	0.022%
8	4.360	222	225	229	rBV3	1372	1944	0.23%	0.023%
9	4.536	252	255	257	rBV3	1140	1446	0.17%	0.017%
10	4.742	288	290	292	rBV2	1347	1435	0.17%	0.017%
11	5.394	397	401	403	rBV3	1112	1703	0.20%	0.020%
12	5.494	416	418	421	rVB4	1157	1325	0.16%	0.016%
13	5.541	423	426	428	rBV3	1019	1360	0.16%	0.016%
14	5.635	438	442	446	rBV2	1053	1537	0.18%	0.018%
15	5.764	460	464	465	rBV2	1629	1758	0.21%	0.021%
16	6.105	520	522	525	rVB3	1535	1380	0.16%	0.016%
17	6.651	614	615	618	rBV2	1320	1402	0.17%	0.017%
18	6.751	629	632	635	rBV	1106	1497	0.18%	0.018%
19	6.997	670	674	676	rBV	1089	1674	0.20%	0.020%
20	7.138	692	698	706	rVB2	30651	55803	6.66%	0.660%
21	7.279	716	722	732	rBV	97908	165061	19.69%	1.951%
22	7.409	741	744	746	rBV3	1269	1715	0.20%	0.020%
23	7.497	752	759	767	rBV	109133	194917	23.25%	2.304%
24	7.961	830	838	846	rVB2	111474	191342	22.83%	2.262%
25	8.031	846	850	853	rBV	735	1356	0.16%	0.016%
26	8.413	909	915	916	rVB	1215	1648	0.20%	0.019%
27	8.625	949	951	954	rBV2	1302	1563	0.19%	0.018%
28	8.683	955	961	970	rVV	90969	163359	19.49%	1.931%
29	9.136	1031	1038	1047	rBV	144312	265508	31.67%	3.138%
30	9.288	1063	1064	1068	rBV	1314	1589	0.19%	0.019%
31	9.529	1102	1105	1110	rVB3	1375	1774	0.21%	0.021%
32	9.864	1154	1162	1171	rVB	129850	233730	27.88%	2.763%
33	10.416	1247	1256	1266	rBV	169790	322124	38.43%	3.808%
34	10.551	1275	1279	1284	rBV5	5164	8477	1.01%	0.100%
35	10.781	1311	1318	1327	rVB	154581	277510	33.11%	3.280%
36	10.922	1335	1342	1352	rBV	127715	240591	28.70%	2.844%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083021\
 Data File : BG050053.D
 Acq On : 31 Aug 2021 6:49
 Operator : CG/JU
 Sample : M3464-02
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBKF5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
 Title : SVOA CALIBRATION

37	11.444	1425	1431	1434	rVB	943	1624	0.19%	0.019%
38	12.373	1585	1589	1595	rVB2	2597	3959	0.47%	0.047%
39	12.619	1629	1631	1636	rBV2	850	1682	0.20%	0.020%
40	13.436	1766	1770	1774	rVB2	1058	1549	0.18%	0.018%
41	14.023	1860	1870	1877	rBV	365662	527990	62.99%	6.241%
42	14.135	1884	1889	1893	rVB2	1388	2273	0.27%	0.027%
43	14.317	1912	1920	1927	rBV	390240	611745	72.98%	7.231%
44	14.517	1948	1954	1956	rBV2	1740	2578	0.31%	0.030%
45	14.570	1958	1963	1965	rBV2	1218	1417	0.17%	0.017%
46	14.622	1966	1972	1980	rVV	253058	384235	45.84%	4.542%
47	14.816	2002	2005	2008	rBV2	1171	1369	0.16%	0.016%
48	14.869	2008	2014	2020	rBV4	20669	39408	4.70%	0.466%
49	15.245	2071	2078	2080	rBV	1505	2805	0.33%	0.033%
50	15.404	2102	2105	2107	rVB2	1597	1352	0.16%	0.016%
51	15.621	2135	2142	2150	rVB	493068	755656	90.15%	8.932%
52	15.756	2160	2165	2173	rBV	104844	154920	18.48%	1.831%
53	15.856	2178	2182	2186	rBV3	4077	5354	0.64%	0.063%
54	16.056	2213	2216	2217	rBV	2492	3048	0.36%	0.036%
55	16.073	2217	2219	2221	rVB	1593	1441	0.17%	0.017%
56	16.320	2257	2261	2263	rBV	1682	2157	0.26%	0.025%
57	16.385	2266	2272	2276	rVV3	2987	5256	0.63%	0.062%
58	16.455	2280	2284	2288	rBV	2000	2495	0.30%	0.029%
59	16.520	2294	2295	2298	rVB	1908	1678	0.20%	0.020%
60	16.555	2298	2301	2303	rBV2	1533	1956	0.23%	0.023%
61	16.608	2306	2310	2313	rBV2	1294	2069	0.25%	0.024%
62	16.690	2322	2324	2325	rBV	1891	1387	0.17%	0.016%
63	16.743	2330	2333	2334	rBV	1383	1548	0.18%	0.018%
64	16.808	2342	2344	2347	rBV	1332	1543	0.18%	0.018%
65	16.960	2366	2370	2372	rBV2	1031	1476	0.18%	0.017%
66	16.984	2372	2374	2377	rVB2	2294	1781	0.21%	0.021%
67	17.049	2382	2385	2386	rBV	1562	1925	0.23%	0.023%
68	17.107	2392	2395	2398	rVB3	2320	2422	0.29%	0.029%
69	17.225	2411	2415	2417	rBV2	2241	2184	0.26%	0.026%
70	17.313	2427	2430	2432	rVB2	1799	1606	0.19%	0.019%
71	17.377	2435	2441	2448	rVB	286850	435513	51.96%	5.148%
72	17.430	2448	2450	2452	rBV2	1770	1732	0.21%	0.020%
73	17.477	2452	2458	2466	rVB	524692	793053	94.61%	9.374%
74	17.671	2489	2491	2493	rBV2	1628	1732	0.21%	0.020%
75	17.859	2521	2523	2526	rVB2	2687	2534	0.30%	0.030%
76	17.889	2526	2528	2529	rBV2	1691	1369	0.16%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083021\
 Data File : BG050053.D
 Acq On : 31 Aug 2021 6:49
 Operator : CG/JU
 Sample : M3464-02
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBKF5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
 Title : SVOA CALIBRATION

77	17.953	2536	2539	2540	rBV3	2756	1999	0.24%	0.024%
78	18.035	2550	2553	2557	rVV4	3789	4015	0.48%	0.047%
79	18.218	2583	2584	2586	rBV	3330	2438	0.29%	0.029%
80	18.276	2589	2594	2595	rBV5	2437	4509	0.54%	0.053%
81	18.347	2605	2606	2608	rBV2	1965	1733	0.21%	0.020%
82	18.435	2619	2621	2622	rBV2	2114	1879	0.22%	0.022%
83	18.453	2622	2624	2625	rVB2	3037	1976	0.24%	0.023%
84	18.470	2625	2627	2631	rBV4	2986	4795	0.57%	0.057%
85	18.529	2635	2637	2638	rVV	2693	1571	0.19%	0.019%
86	18.558	2641	2642	2644	rVV2	3120	1963	0.23%	0.023%
87	18.593	2644	2648	2649	rVV4	2822	2591	0.31%	0.031%
88	18.729	2669	2671	2676	rBV5	3363	4704	0.56%	0.056%
89	18.764	2676	2677	2678	rBV	2684	1737	0.21%	0.021%
90	18.852	2689	2692	2693	rBV3	3971	3322	0.40%	0.039%
91	18.870	2693	2695	2696	rBV2	2728	1607	0.19%	0.019%
92	18.964	2710	2711	2713	rBV2	2667	1614	0.19%	0.019%
93	19.058	2726	2727	2728	rVB	3888	1371	0.16%	0.016%
94	19.087	2730	2732	2734	rVB3	3495	2298	0.27%	0.027%
95	19.328	2771	2773	2777	rVB5	8271	9812	1.17%	0.116%
96	19.404	2783	2786	2791	rVB4	7281	11352	1.35%	0.134%
97	19.774	2842	2849	2856	rBV	575446	838246	100.00%	9.908%
98	21.654	3164	3169	3175	rVB	242860	385449	45.98%	4.556%
99	24.668	3673	3682	3692	rVB2	272098	759557	90.61%	8.978%
100	24.891	3713	3720	3730	rVB2	146717	422386	50.39%	4.993%


Sum of corrected areas: 8460146

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083021\
Data File : BG050053.D
Acq On : 31 Aug 2021 6:49
Operator : CG/JU
Sample : M3464-02
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBKF5

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

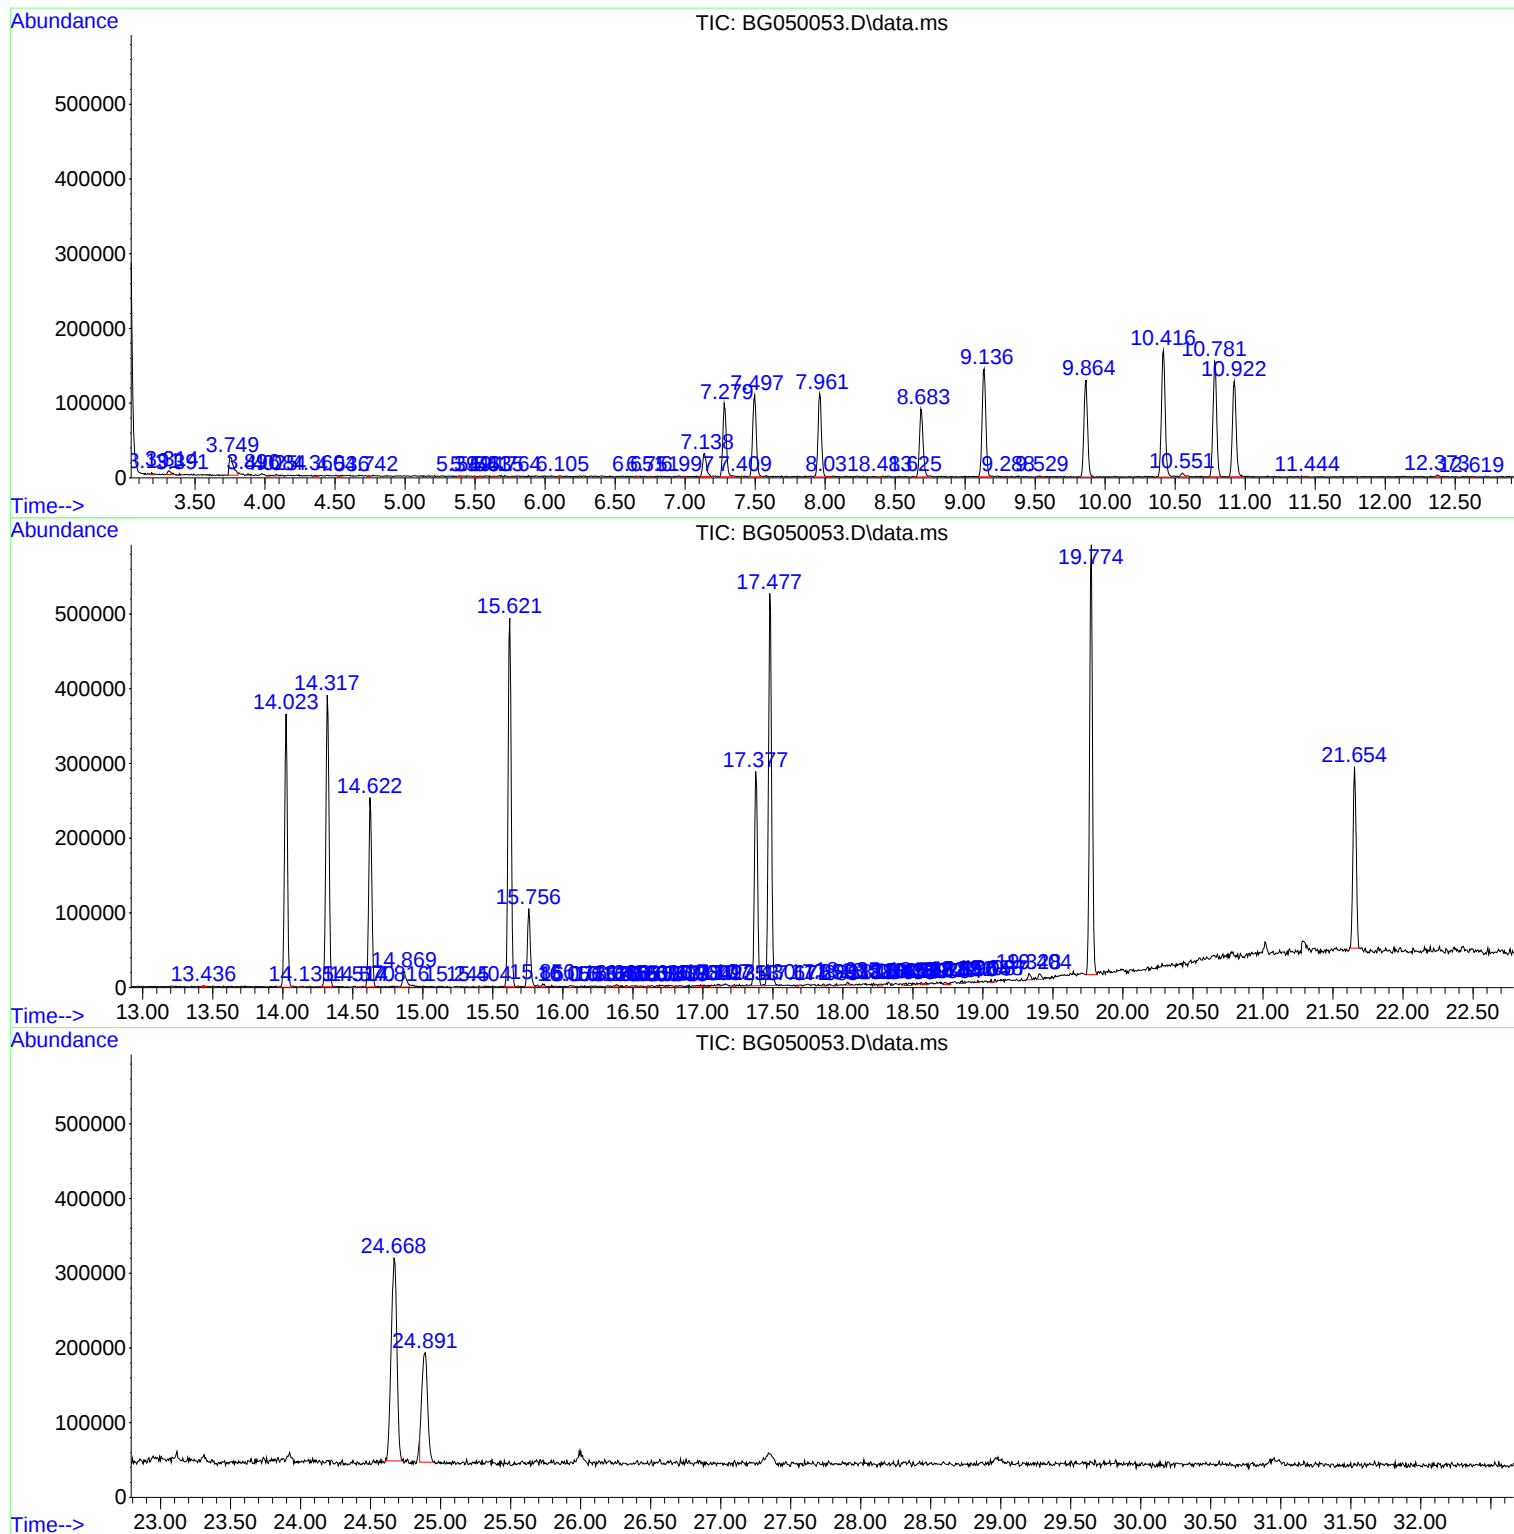

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083021\
Data File : BG050053.D
Acq On : 31 Aug 2021 6:49
Operator : CG/JU
Sample : M3464-02
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBKF5

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083021\
Data File : BG050053.D
Acq On : 31 Aug 2021 6:49
Operator : CG/JU
Sample : M3464-02
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBKF5

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
