

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083021\
 Data File : BG050055.D
 Acq On : 31 Aug 2021 8:11
 Operator : CG/JU
 Sample : M3464-03
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBKF6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
 Title : SVOA CALIBRATION

Signal : TIC: BG050055.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.308	43	46	52	rBV4	4101	7115	0.86%	0.089%
2	3.766	121	124	131	rBV4	4727	8243	1.00%	0.103%
3	4.336	219	221	225	rVB4	1489	1433	0.17%	0.018%
4	4.365	225	226	229	rVB	2026	1279	0.15%	0.016%
5	4.401	229	232	234	rBV2	1656	1910	0.23%	0.024%
6	4.630	269	271	273	rVB2	1282	1126	0.14%	0.014%
7	5.047	339	342	345	rVB3	1211	1742	0.21%	0.022%
8	5.247	373	376	377	rVB2	1370	1341	0.16%	0.017%
9	5.352	393	394	397	rBV2	1046	1099	0.13%	0.014%
10	5.394	397	401	404	rVB2	1110	1520	0.18%	0.019%
11	5.423	404	406	408	rBV3	1437	1329	0.16%	0.017%
12	5.611	435	438	441	rBV2	1063	1319	0.16%	0.017%
13	5.963	494	498	500	rBV4	978	1163	0.14%	0.015%
14	6.363	562	566	569	rBV4	1019	1767	0.21%	0.022%
15	6.668	616	618	623	rVB3	1927	2502	0.30%	0.031%
16	6.721	625	627	634	rVB2	1425	2522	0.30%	0.032%
17	6.909	657	659	662	rBV3	1500	1512	0.18%	0.019%
18	6.956	665	667	671	rVB	1255	1595	0.19%	0.020%
19	7.138	692	698	707	rBV2	27680	48647	5.88%	0.609%
20	7.279	716	722	732	rVB	81466	136868	16.55%	1.713%
21	7.497	752	759	768	rBV	94462	170820	20.66%	2.138%
22	7.961	831	838	845	rBV	108968	180276	21.80%	2.256%
23	8.384	907	910	911	rBV	1282	1236	0.15%	0.015%
24	8.577	939	943	945	rVB2	1625	1635	0.20%	0.020%
25	8.689	954	962	971	rBV	75587	141384	17.10%	1.770%
26	8.812	982	983	988	rBV	1310	1355	0.16%	0.017%
27	8.983	1011	1012	1016	rBV	1069	1436	0.17%	0.018%
28	9.018	1016	1018	1022	rVB	1095	1116	0.13%	0.014%
29	9.071	1025	1027	1030	rVB	1068	1164	0.14%	0.015%
30	9.135	1030	1038	1046	rBV	126476	227905	27.56%	2.852%
31	9.370	1075	1078	1080	rBV	1560	1476	0.18%	0.018%
32	9.746	1138	1142	1145	rVB2	970	1251	0.15%	0.016%
33	9.864	1154	1162	1170	rVB2	112419	205029	24.79%	2.566%
34	10.416	1249	1256	1265	rBV	146423	276317	33.41%	3.458%
35	10.551	1274	1279	1282	rBV4	3245	5141	0.62%	0.064%
36	10.581	1282	1284	1286	rVB2	1908	1426	0.17%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083021\
 Data File : BG050055.D
 Acq On : 31 Aug 2021 8:11
 Operator : CG/JU
 Sample : M3464-03
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBKF6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
 Title : SVOA CALIBRATION

37	10.686	1299	1302	1305	rVB	1162	1630	0.20%	0.020%
38	10.786	1310	1319	1326	rVV	146969	266692	32.25%	3.338%
39	10.921	1333	1342	1351	rBV2	104228	195550	23.65%	2.447%
40	11.661	1466	1468	1471	rVB2	1499	1156	0.14%	0.014%
41	12.378	1584	1590	1593	rBV4	2818	4248	0.51%	0.053%
42	12.425	1596	1598	1602	rVB	1231	1138	0.14%	0.014%
43	12.466	1602	1605	1607	rBV	1094	1429	0.17%	0.018%
44	12.613	1625	1630	1632	rBV2	849	1101	0.13%	0.014%
45	12.678	1637	1641	1642	rBV	1129	1242	0.15%	0.016%
46	12.748	1651	1653	1659	rVB	669	1170	0.14%	0.015%
47	13.224	1730	1734	1736	rVB	1330	1417	0.17%	0.018%
48	13.424	1766	1768	1773	rVB2	1039	1263	0.15%	0.016%
49	13.535	1785	1787	1790	rBV	1101	1183	0.14%	0.015%
50	14.023	1864	1870	1876	rBV	327586	467891	56.58%	5.856%
51	14.070	1876	1878	1883	rVB2	1144	1411	0.17%	0.018%
52	14.317	1913	1920	1927	rBV	336536	533086	64.46%	6.672%
53	14.628	1966	1973	1979	rVB	237946	381953	46.19%	4.780%
54	14.863	2009	2013	2022	rBV2	18756	37327	4.51%	0.467%
55	15.116	2051	2056	2059	rBV	1113	1638	0.20%	0.021%
56	15.556	2129	2131	2135	rVB	931	1282	0.16%	0.016%
57	15.621	2135	2142	2149	rBV	455863	688456	83.25%	8.616%
58	15.756	2160	2165	2172	rBV	103056	159666	19.31%	1.998%
59	15.862	2177	2183	2187	rVB2	2175	3849	0.47%	0.048%
60	16.731	2328	2331	2333	rBV	1619	1306	0.16%	0.016%
61	16.772	2333	2338	2340	rBV2	1019	1258	0.15%	0.016%
62	16.990	2373	2375	2377	rVB2	1227	1131	0.14%	0.014%
63	17.166	2401	2405	2409	rVB2	1766	3033	0.37%	0.038%
64	17.207	2409	2412	2415	rBV2	1159	1453	0.18%	0.018%
65	17.283	2422	2425	2427	rBV2	1329	1373	0.17%	0.017%
66	17.377	2435	2441	2448	rVB	291360	446678	54.01%	5.590%
67	17.477	2451	2458	2465	rBV	531930	793525	95.96%	9.931%
68	17.647	2484	2487	2493	rBV5	3612	6909	0.84%	0.086%
69	17.853	2519	2522	2523	rBV	1617	1821	0.22%	0.023%
70	17.906	2529	2531	2534	rVB2	2267	1915	0.23%	0.024%
71	18.006	2546	2548	2549	rBV	1842	1461	0.18%	0.018%
72	18.029	2549	2552	2555	rVB3	4439	5411	0.65%	0.068%
73	18.153	2571	2573	2575	rBV	1674	1098	0.13%	0.014%
74	18.294	2595	2597	2599	rBV2	1277	1322	0.16%	0.017%
75	18.335	2601	2604	2606	rVV	2202	2263	0.27%	0.028%
76	18.364	2608	2609	2612	rVB2	2243	1323	0.16%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083021\
 Data File : BG050055.D
 Acq On : 31 Aug 2021 8:11
 Operator : CG/JU
 Sample : M3464-03
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBKF6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
 Title : SVOA CALIBRATION

77	18.423	2616	2619	2622	rBV2	889	1513	0.18%	0.019%
78	18.488	2627	2630	2631	rVB2	1648	1594	0.19%	0.020%
79	18.517	2633	2635	2637	rBV	2535	1535	0.19%	0.019%
80	18.546	2637	2640	2643	rBV3	1842	2551	0.31%	0.032%
81	18.582	2645	2646	2647	rBV3	2840	1405	0.17%	0.018%
82	18.711	2667	2668	2670	rBV2	2039	1338	0.16%	0.017%
83	18.752	2673	2675	2678	rVB3	1977	1669	0.20%	0.021%
84	18.781	2678	2680	2684	rVB3	2795	3493	0.42%	0.044%
85	18.811	2684	2685	2686	rBV	3103	1864	0.23%	0.023%
86	18.963	2709	2711	2712	rBV	1509	1130	0.14%	0.014%
87	19.063	2726	2728	2729	rBV	1491	1190	0.14%	0.015%
88	19.163	2743	2745	2748	rBV4	1616	1948	0.24%	0.024%
89	19.187	2748	2749	2754	rVB4	3081	4159	0.50%	0.052%
90	19.245	2757	2759	2763	rBV4	2487	2310	0.28%	0.029%
91	19.333	2769	2774	2778	rBV4	6690	10307	1.25%	0.129%
92	19.369	2778	2780	2783	rBV3	2767	2906	0.35%	0.036%
93	19.404	2783	2786	2791	rVV2	6591	10674	1.29%	0.134%
94	19.463	2794	2796	2799	rVV4	2654	2269	0.27%	0.028%
95	19.774	2842	2849	2856	rBV	562565	826961	100.00%	10.350%
96	19.986	2883	2885	2888	rBV4	4253	5642	0.68%	0.071%
97	20.109	2904	2906	2909	rBV4	5052	3625	0.44%	0.045%
98	21.654	3164	3169	3178	rVB2	249916	407047	49.22%	5.094%
99	24.667	3672	3682	3693	rVB2	268466	762832	92.25%	9.547%
100	24.885	3712	3719	3730	rVB2	161788	455971	55.14%	5.707%




Sum of corrected areas: 7989990

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083021\
Data File : BG050055.D
Acq On : 31 Aug 2021 8:11
Operator : CG/JU
Sample : M3464-03
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBKF6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

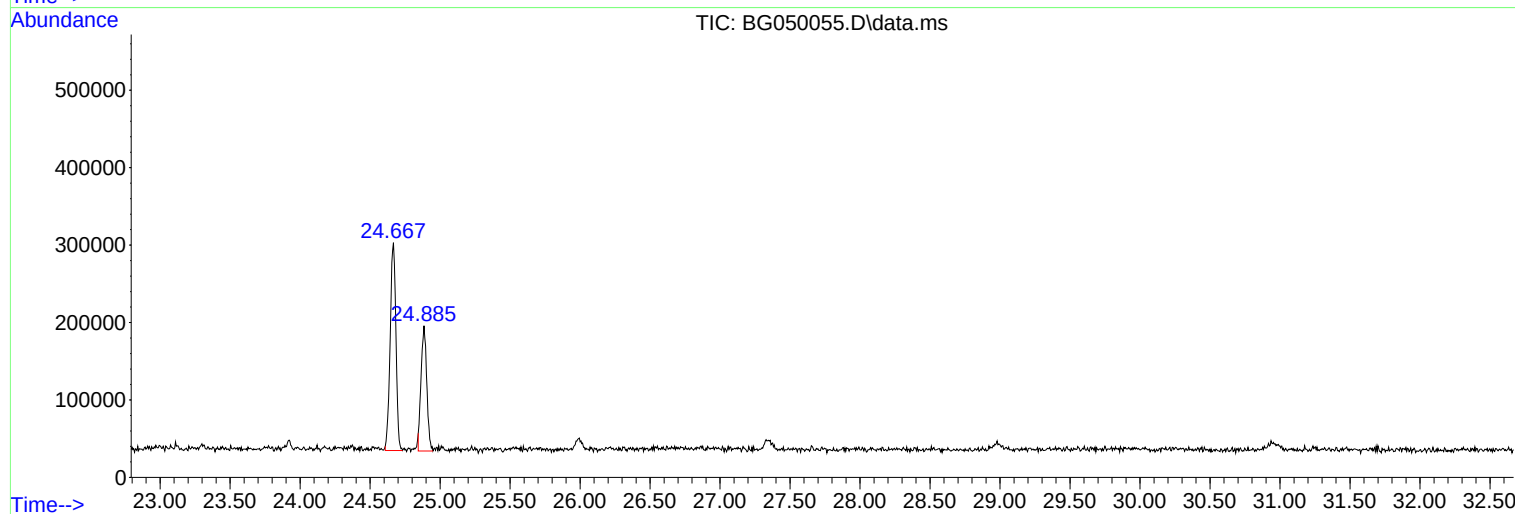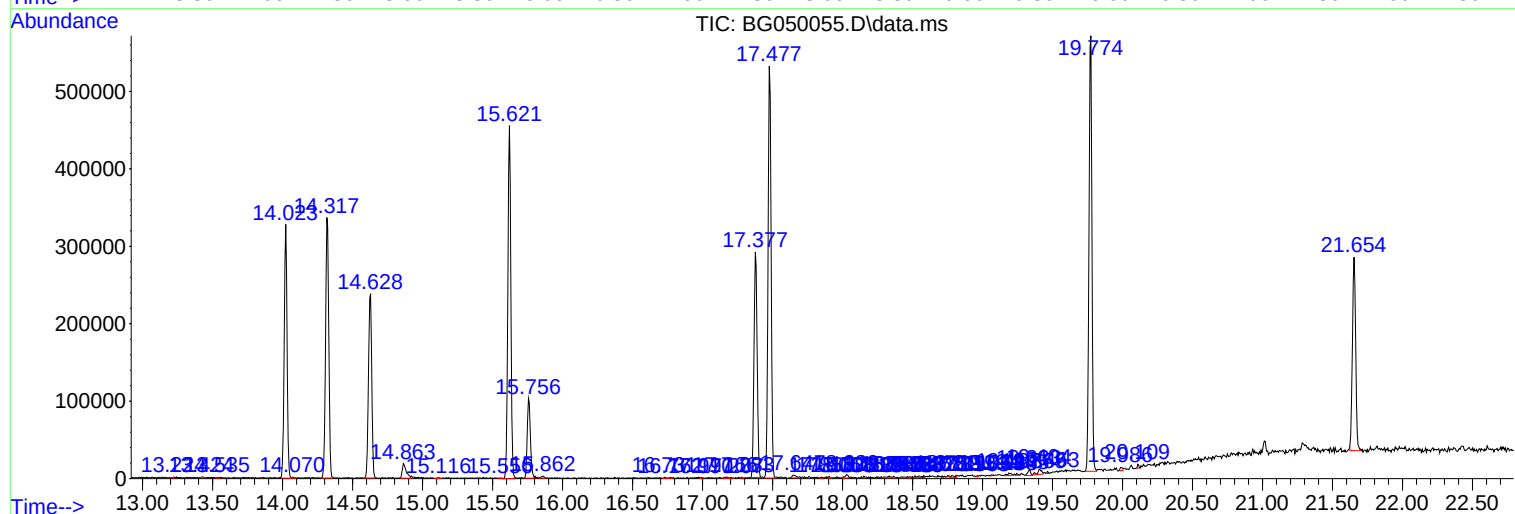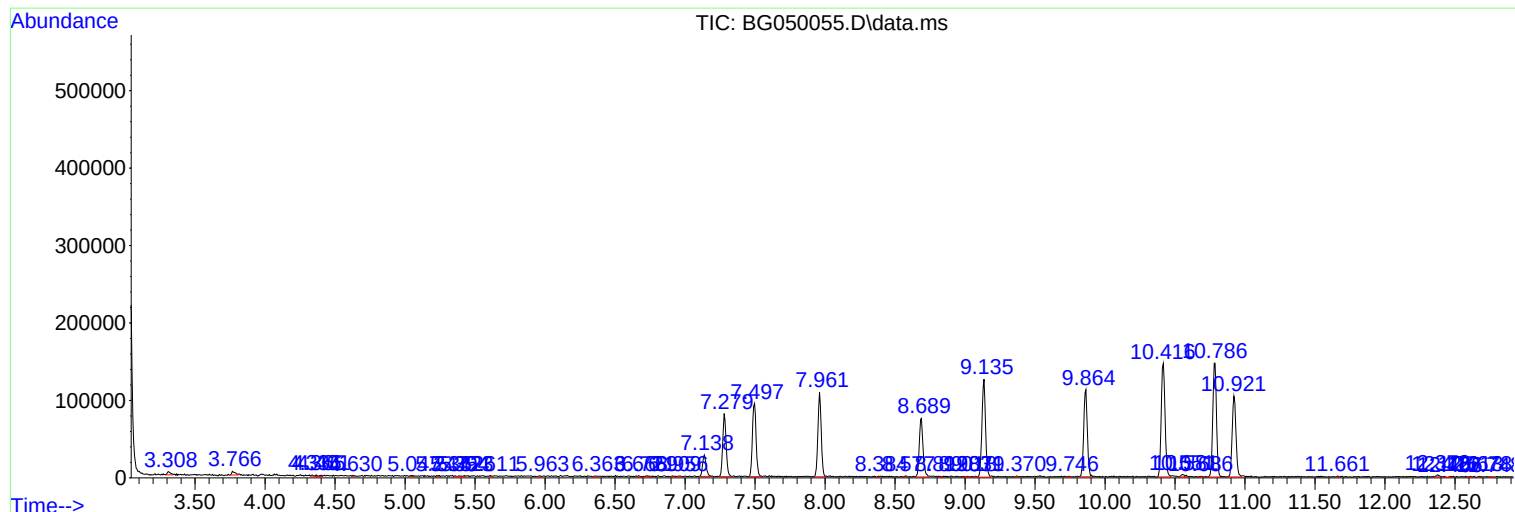

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083021\
Data File : BG050055.D
Acq On : 31 Aug 2021 8:11
Operator : CG/JU
Sample : M3464-03
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBKF6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083021\
Data File : BG050055.D
Acq On : 31 Aug 2021 8:11
Operator : CG/JU
Sample : M3464-03
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBKF6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
