

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083021\
 Data File : BG050057.D
 Acq On : 31 Aug 2021 9:33
 Operator : CG/JU
 Sample : M3464-04
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBKF7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
 Title : SVOA CALIBRATION

Signal : TIC: BG050057.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.314	44	47	50	rBV3	4360	4724	0.51%	0.056%
2	3.543	84	86	88	rBV3	1162	1397	0.15%	0.017%
3	3.766	121	124	134	rBV2	7021	13783	1.50%	0.164%
4	3.978	157	160	165	rVB4	1989	3125	0.34%	0.037%
5	5.776	463	466	469	rBV2	1235	1346	0.15%	0.016%
6	6.198	536	538	540	rBV2	1319	1371	0.15%	0.016%
7	6.445	578	580	583	rBV	1381	1214	0.13%	0.014%
8	6.698	620	623	624	rBV	1270	1318	0.14%	0.016%
9	7.133	691	697	703	rBV2	29638	53651	5.83%	0.639%
10	7.279	716	722	732	rVB	87513	151092	16.41%	1.801%
11	7.403	740	743	745	rBV	1814	1600	0.17%	0.019%
12	7.497	753	759	766	rBV	103525	184723	20.07%	2.202%
13	7.961	831	838	845	rVV2	103858	175734	19.09%	2.095%
14	8.025	847	849	851	rVB	1396	1417	0.15%	0.017%
15	8.560	937	940	945	rBV	1165	2114	0.23%	0.025%
16	8.683	955	961	972	rBV2	84524	150138	16.31%	1.790%
17	9.136	1030	1038	1045	rBV	131368	239179	25.98%	2.851%
18	9.864	1154	1162	1170	rBV	118027	218212	23.70%	2.601%
19	10.416	1249	1256	1271	rBV	155732	290564	31.56%	3.463%
20	10.563	1276	1281	1283	rBV3	2119	3101	0.34%	0.037%
21	10.781	1311	1318	1325	rBV	146212	256243	27.83%	3.054%
22	10.922	1334	1342	1351	rBV	122242	230724	25.06%	2.750%
23	12.378	1586	1590	1594	rBV	2727	4109	0.45%	0.049%
24	14.023	1863	1870	1879	rBV	344937	485709	52.76%	5.789%
25	14.317	1913	1920	1929	rBV	358830	566809	61.57%	6.756%
26	14.622	1966	1972	1981	rVB	229820	362494	39.38%	4.321%
27	14.869	2005	2014	2029	rBV4	19746	45619	4.96%	0.544%
28	15.621	2135	2142	2151	rBV	486216	728234	79.11%	8.680%
29	15.756	2160	2165	2174	rBV	118117	182941	19.87%	2.181%
30	15.856	2179	2182	2190	rVB3	3443	6283	0.68%	0.075%
31	16.320	2258	2261	2265	rVB	1669	1577	0.17%	0.019%
32	16.708	2324	2327	2330	rVB	1505	1441	0.16%	0.017%
33	16.908	2359	2361	2365	rBV	969	1638	0.18%	0.020%
34	17.119	2393	2397	2400	rBV	1640	1739	0.19%	0.021%
35	17.172	2403	2406	2407	rBV	1358	1229	0.13%	0.015%
36	17.231	2413	2416	2419	rBV	1067	1310	0.14%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083021\
 Data File : BG050057.D
 Acq On : 31 Aug 2021 9:33
 Operator : CG/JU
 Sample : M3464-04
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBKF7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
 Title : SVOA CALIBRATION

37	17.377	2434	2441	2449	rBV2	291626	440962	47.90%	5.256%
38	17.477	2452	2458	2470	rVB	561563	862309	93.67%	10.278%
39	17.648	2483	2487	2489	rBV4	4226	5852	0.64%	0.070%
40	17.759	2503	2506	2509	rBV2	1193	1652	0.18%	0.020%
41	17.853	2519	2522	2525	rBV2	1192	1944	0.21%	0.023%
42	17.912	2530	2532	2536	rBV	1108	1522	0.17%	0.018%
43	17.994	2543	2546	2547	rBV2	1417	1291	0.14%	0.015%
44	18.030	2549	2552	2556	rVB4	4005	5491	0.60%	0.065%
45	18.147	2571	2572	2574	rVB	2178	1409	0.15%	0.017%
46	18.182	2574	2578	2579	rVB	2223	2132	0.23%	0.025%
47	18.206	2579	2582	2583	rBV	1552	1526	0.17%	0.018%
48	18.329	2600	2603	2604	rBV2	1795	1864	0.20%	0.022%
49	18.517	2634	2635	2638	rVB	1747	1654	0.18%	0.020%
50	18.546	2638	2640	2641	rBV	1819	1364	0.15%	0.016%
51	18.693	2663	2665	2668	rBV2	1574	1445	0.16%	0.017%
52	18.787	2677	2681	2686	rBV5	1778	3633	0.39%	0.043%
53	18.852	2689	2692	2693	rBV	2914	2371	0.26%	0.028%
54	18.964	2710	2711	2713	rVB	2635	1450	0.16%	0.017%
55	19.134	2739	2740	2743	rBV3	2020	2499	0.27%	0.030%
56	19.293	2766	2767	2768	rBV3	2061	1217	0.13%	0.015%
57	19.328	2770	2773	2779	rVV3	8495	13017	1.41%	0.155%
58	19.404	2781	2786	2792	rVV3	7538	13619	1.48%	0.162%
59	19.774	2842	2849	2855	rBV	626983	920579	100.00%	10.973%
60	19.997	2883	2887	2888	rBV4	3431	4337	0.47%	0.052%
61	20.162	2914	2915	2917	rBV2	4497	3479	0.38%	0.041%
62	21.014	3057	3060	3063	rBV2	31067	33797	3.67%	0.403%
63	21.654	3163	3169	3178	rVB	257616	415613	45.15%	4.954%
64	24.668	3672	3682	3692	rVB2	292018	825924	89.72%	9.844%
65	24.885	3712	3719	3731	rVB	162894	437968	47.58%	5.220%




Sum of corrected areas: 8389822

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083021\
Data File : BG050057.D
Acq On : 31 Aug 2021 9:33
Operator : CG/JU
Sample : M3464-04
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBKF7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

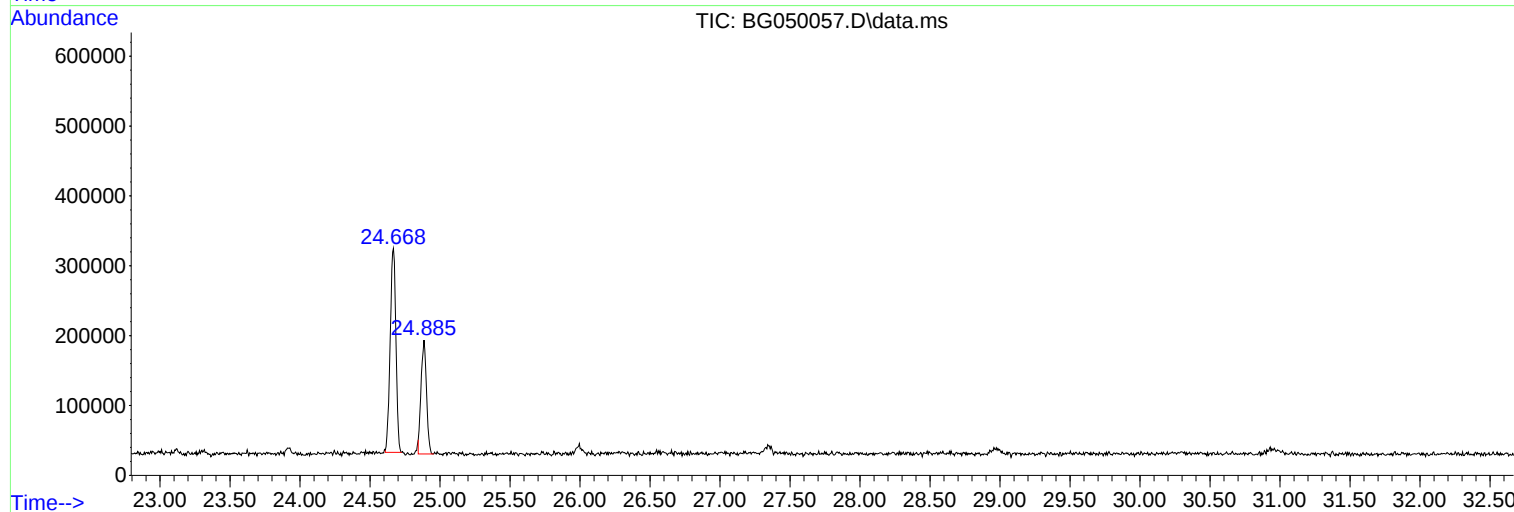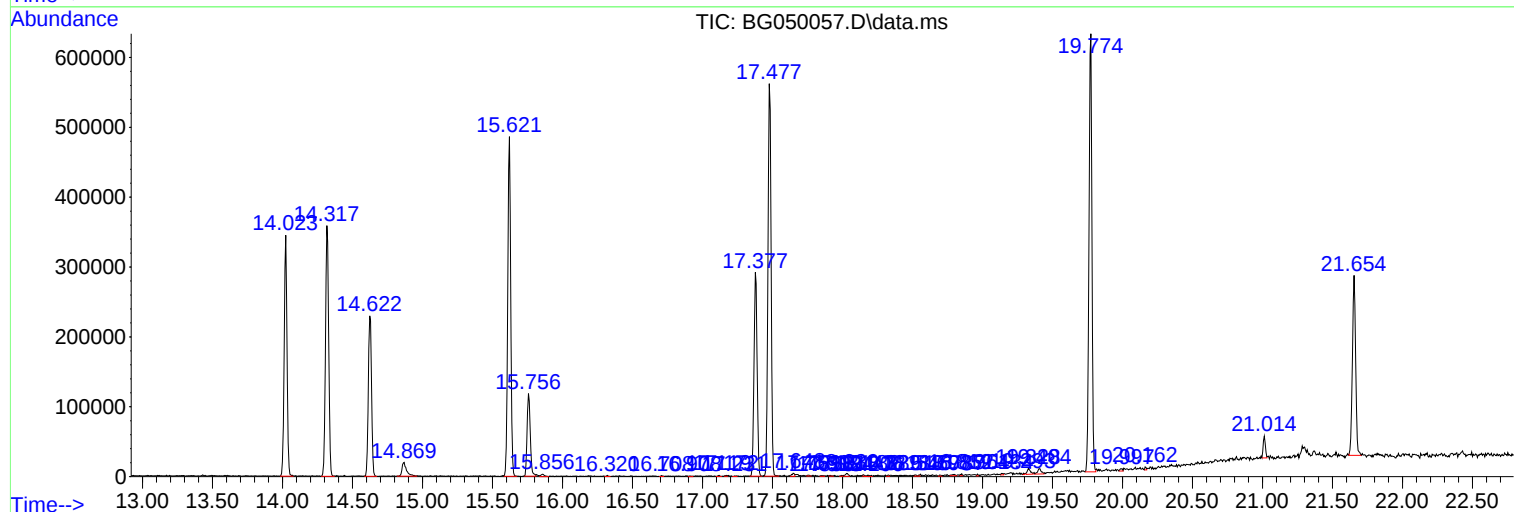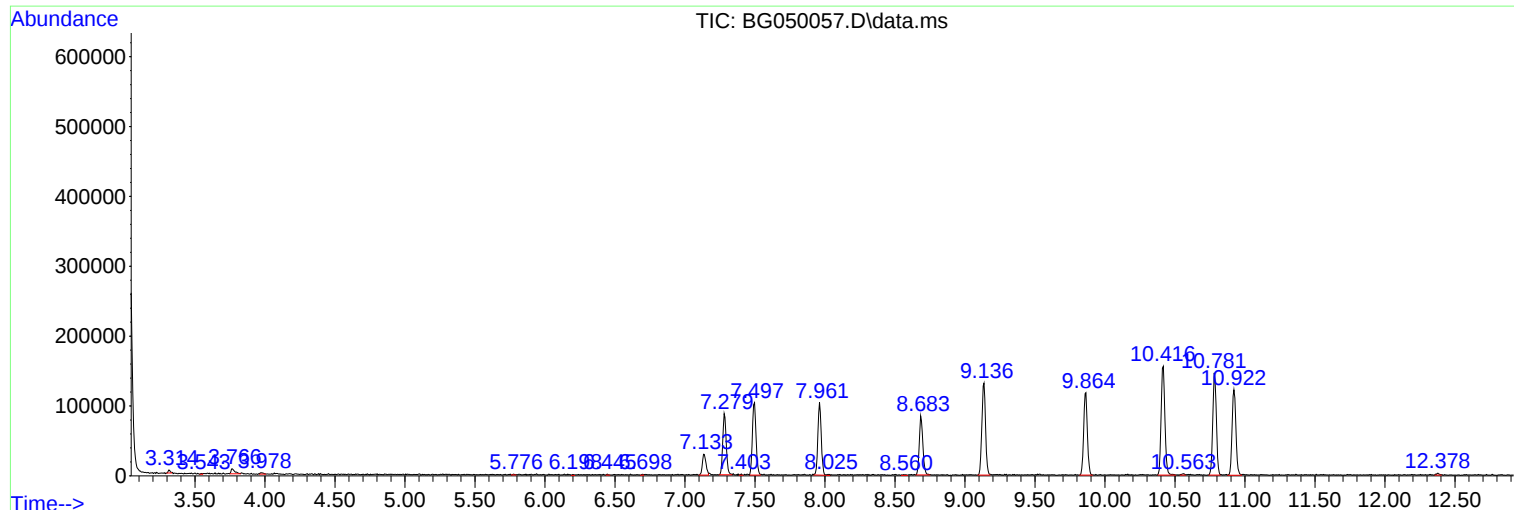

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083021\
Data File : BG050057.D
Acq On : 31 Aug 2021 9:33
Operator : CG/JU
Sample : M3464-04
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBKF7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083021\
Data File : BG050057.D
Acq On : 31 Aug 2021 9:33
Operator : CG/JU
Sample : M3464-04
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBKF7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
