

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083021\
 Data File : BG050059.D
 Acq On : 31 Aug 2021 10:56
 Operator : CG/JU
 Sample : PB138722BL
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK722

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
 Title : SVOA CALIBRATION

Signal : TIC: BG050059.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.309	43	46	52	rBV5	4748	7499	1.12%	0.103%
2	3.521	80	82	84	rBV2	1463	1264	0.19%	0.017%
3	3.609	95	97	100	rBV3	1366	1379	0.21%	0.019%
4	3.697	109	112	114	rBV3	1616	1675	0.25%	0.023%
5	3.744	116	120	134	rBV	57847	120366	17.94%	1.660%
6	4.073	174	176	183	rBV3	2654	4833	0.72%	0.067%
7	4.238	202	204	207	rVB2	1417	983	0.15%	0.014%
8	4.373	225	227	229	rBV2	1597	1471	0.22%	0.020%
9	4.514	249	251	254	rVB2	1111	1019	0.15%	0.014%
10	4.649	273	274	277	rBV2	880	1034	0.15%	0.014%
11	4.760	291	293	295	rBV	987	1208	0.18%	0.017%
12	5.183	362	365	367	rBV2	1298	1269	0.19%	0.018%
13	5.330	385	390	391	rVB3	1282	1806	0.27%	0.025%
14	5.483	413	416	420	rBV3	1074	1435	0.21%	0.020%
15	5.571	425	431	433	rBV3	1390	2257	0.34%	0.031%
16	6.300	552	555	557	rBV2	1240	1242	0.19%	0.017%
17	6.382	567	569	572	rVB	1451	1013	0.15%	0.014%
18	6.558	598	599	602	rBV	1091	1053	0.16%	0.015%
19	6.752	628	632	636	rVV2	1016	1356	0.20%	0.019%
20	6.799	638	640	645	rBV3	855	1546	0.23%	0.021%
21	7.010	671	676	677	rBV2	1076	1142	0.17%	0.016%
22	7.134	691	697	710	rBV2	109690	193273	28.80%	2.666%
23	7.281	716	722	732	rVB	69686	120474	17.95%	1.662%
24	7.492	752	758	767	rVB	107304	191040	28.47%	2.635%
25	7.657	784	786	788	rVB2	1156	1023	0.15%	0.014%
26	7.962	832	838	847	rVB	86357	149498	22.28%	2.062%
27	8.685	955	961	974	rBV	136066	242152	36.09%	3.341%
28	8.949	1003	1006	1007	rBV	956	1058	0.16%	0.015%
29	9.131	1031	1037	1047	rBV	108253	193312	28.81%	2.667%
30	9.660	1126	1127	1130	rVB	1061	931	0.14%	0.013%
31	9.742	1140	1141	1144	rVB2	1119	945	0.14%	0.013%
32	9.859	1154	1161	1171	rVB2	97360	182605	27.21%	2.519%
33	10.341	1241	1243	1246	rBV2	1230	936	0.14%	0.013%
34	10.412	1249	1255	1268	rVV	140700	254545	37.93%	3.511%
35	10.782	1308	1318	1326	rBV	122487	216780	32.31%	2.991%
36	10.923	1335	1342	1354	rVB	126976	238753	35.58%	3.294%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083021\
 Data File : BG050059.D
 Acq On : 31 Aug 2021 10:56
 Operator : CG/JU
 Sample : PB138722BL
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK722

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
 Title : SVOA CALIBRATION

37	11.316	1407	1409	1412	rVB2	1146	990	0.15%	0.014%
38	11.357	1412	1416	1417	rBV	937	1146	0.17%	0.016%
39	11.727	1476	1479	1481	rBV	760	968	0.14%	0.013%
40	11.863	1500	1502	1505	rBV	728	941	0.14%	0.013%
41	11.939	1511	1515	1516	rVB	942	1066	0.16%	0.015%
42	12.380	1585	1590	1591	rBV	1831	1953	0.29%	0.027%
43	12.820	1663	1665	1668	rVB2	1111	1058	0.16%	0.015%
44	12.873	1671	1674	1677	rVV	1238	1194	0.18%	0.016%
45	13.754	1820	1824	1826	rBV2	1084	1055	0.16%	0.015%
46	13.789	1829	1830	1835	rBV	811	1322	0.20%	0.018%
47	14.024	1864	1870	1878	rVB	256053	378768	56.45%	5.225%
48	14.318	1913	1920	1928	rVV	287682	453067	67.52%	6.250%
49	14.394	1930	1933	1936	rBV2	1173	1308	0.19%	0.018%
50	14.624	1966	1972	1981	rVB	214675	318896	47.52%	4.399%
51	14.853	2006	2011	2023	rBV	79536	162066	24.15%	2.236%
52	15.422	2107	2108	2113	rBV	642	957	0.14%	0.013%
53	15.622	2135	2142	2150	rBV2	377785	568415	84.71%	7.841%
54	15.757	2160	2165	2175	rBV	80216	121782	18.15%	1.680%
55	15.857	2179	2182	2187	rVB	3414	5038	0.75%	0.069%
56	16.010	2205	2208	2211	rVB	1086	1163	0.17%	0.016%
57	16.398	2272	2274	2276	rBV	1563	1127	0.17%	0.016%
58	17.167	2402	2405	2407	rVB	988	1001	0.15%	0.014%
59	17.379	2434	2441	2448	rBV	262516	386909	57.66%	5.337%
60	17.479	2451	2458	2465	rVV2	428147	631377	94.09%	8.710%
61	17.555	2468	2471	2473	rBV2	1301	1358	0.20%	0.019%
62	17.725	2498	2500	2503	rVB	1372	909	0.14%	0.013%
63	17.901	2526	2530	2531	rVB	884	1058	0.16%	0.015%
64	17.954	2533	2539	2540	rBV2	1189	991	0.15%	0.014%
65	18.007	2545	2548	2550	rBV2	1051	1107	0.16%	0.015%
66	18.084	2559	2561	2563	rVB	1292	1068	0.16%	0.015%
67	18.136	2569	2570	2572	rBV	1191	968	0.14%	0.013%
68	18.201	2577	2581	2584	rBV2	1208	1699	0.25%	0.023%
69	18.301	2597	2598	2601	rBV2	1245	1278	0.19%	0.018%
70	18.389	2610	2613	2615	rBV	1125	1124	0.17%	0.016%
71	18.454	2622	2624	2627	rBV	901	953	0.14%	0.013%
72	18.507	2629	2633	2636	rBV	1054	1545	0.23%	0.021%
73	18.648	2655	2657	2660	rVB2	1516	1372	0.20%	0.019%
74	18.718	2664	2669	2672	rVV	1118	1743	0.26%	0.024%
75	18.830	2685	2688	2692	rVB2	1045	1422	0.21%	0.020%
76	18.883	2694	2697	2700	rBV3	1615	1897	0.28%	0.026%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083021\
 Data File : BG050059.D
 Acq On : 31 Aug 2021 10:56
 Operator : CG/JU
 Sample : PB138722BL
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK722

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
 Title : SVOA CALIBRATION

77	18.994	2715	2716	2718	rBV2	1630	1002	0.15%	0.014%
78	19.024	2718	2721	2722	rVV	1231	1110	0.17%	0.015%
79	19.059	2724	2727	2730	rVB	1382	1759	0.26%	0.024%
80	19.082	2730	2731	2734	rBV2	1938	1260	0.19%	0.017%
81	19.106	2734	2735	2737	rBV	2390	1669	0.25%	0.023%
82	19.270	2761	2763	2764	rBV2	1638	1090	0.16%	0.015%
83	19.300	2764	2768	2769	rBV2	1418	1783	0.27%	0.025%
84	19.323	2769	2772	2773	rBV2	2018	2102	0.31%	0.029%
85	19.364	2778	2779	2782	rBV2	1290	1334	0.20%	0.018%
86	19.411	2782	2787	2788	rBV2	5567	5736	0.85%	0.079%
87	19.452	2793	2794	2795	rBV	2728	1206	0.18%	0.017%
88	19.499	2799	2802	2803	rBV3	2426	2844	0.42%	0.039%
89	19.517	2803	2805	2807	rBV2	2217	1939	0.29%	0.027%
90	19.658	2827	2829	2830	rBV2	2858	1230	0.18%	0.017%
91	19.770	2842	2848	2854	rBV2	471769	671021	100.00%	9.257%
92	19.940	2875	2877	2879	rBV3	2151	2415	0.36%	0.033%
93	19.963	2879	2881	2884	rVB4	2870	2908	0.43%	0.040%
94	21.655	3163	3169	3177	rVB	228615	372110	55.45%	5.133%
95	24.663	3672	3681	3689	rBV2	219103	578540	86.22%	7.981%
96	24.886	3709	3719	3727	rBV3	135287	387650	57.77%	5.348%




Sum of corrected areas: 7248942

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083021\
Data File : BG050059.D
Acq On : 31 Aug 2021 10:56
Operator : CG/JU
Sample : PB138722BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK722

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

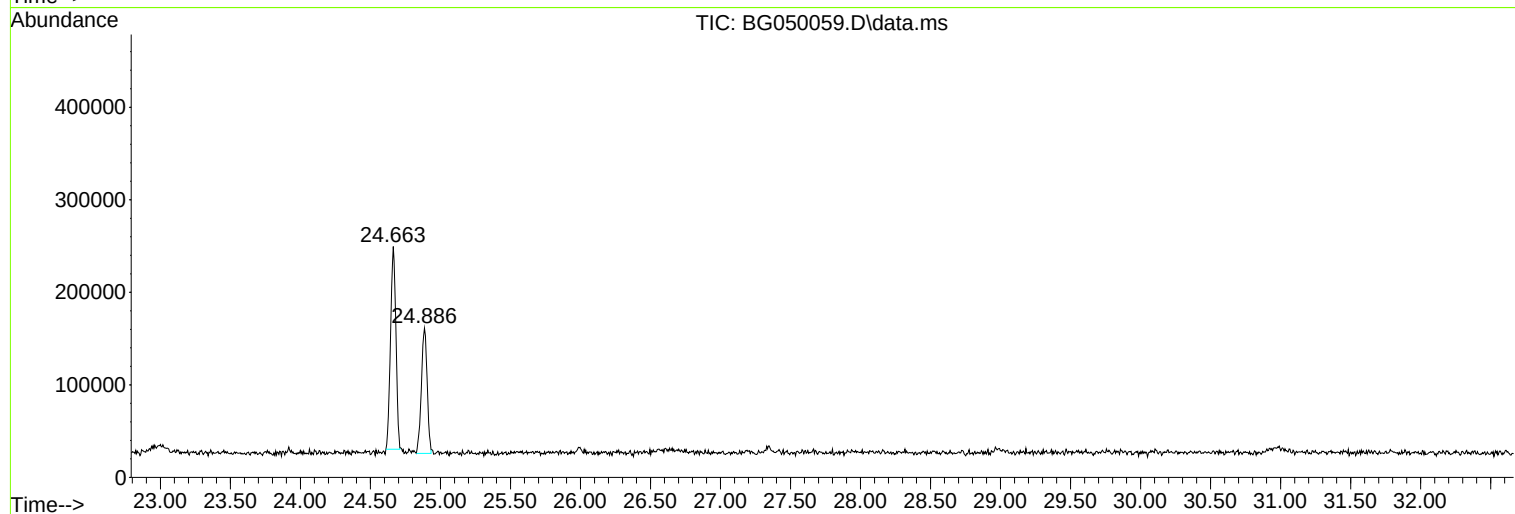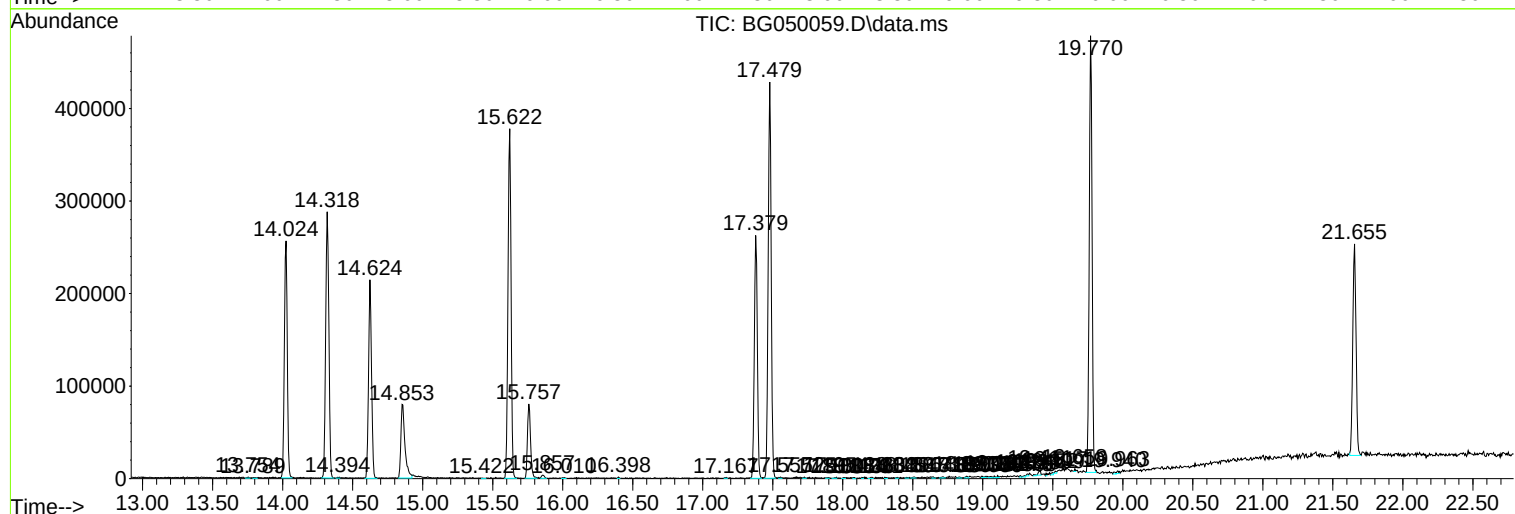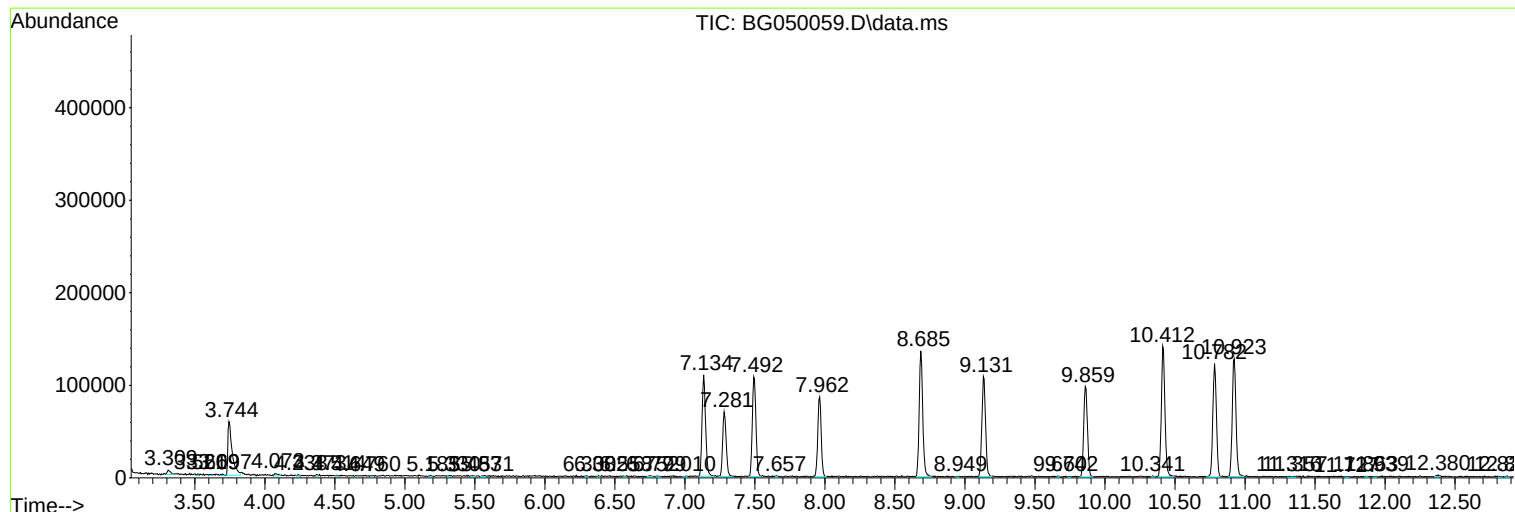

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083021\
Data File : BG050059.D
Acq On : 31 Aug 2021 10:56
Operator : CG/JU
Sample : PB138722BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK722

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083021\
Data File : BG050059.D
Acq On : 31 Aug 2021 10:56
Operator : CG/JU
Sample : PB138722BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK722

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------