

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083021\
 Data File : BG050090.D
 Acq On : 1 Sep 2021 9:35
 Operator : CG/JU
 Sample : PB138604BL
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK604

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
 Title : SVOA CALIBRATION

Signal : TIC: BG050090.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.316	45	47	55	rVB4	5836	6646	0.96%	0.089%
2	3.386	57	59	61	rBV2	1834	1441	0.21%	0.019%
3	3.422	63	65	66	rBV2	1245	1095	0.16%	0.015%
4	3.510	78	80	83	rBV4	1828	2050	0.30%	0.027%
5	3.745	118	120	132	rBV	59593	123335	17.87%	1.647%
6	4.044	169	171	175	rBV3	1098	1733	0.25%	0.023%
7	4.080	175	177	181	rVB5	1819	2157	0.31%	0.029%
8	4.391	228	230	232	rBV2	1239	1158	0.17%	0.015%
9	4.415	232	234	236	rVV3	1262	1191	0.17%	0.016%
10	4.485	244	246	248	rBV	976	1156	0.17%	0.015%
11	4.561	258	259	263	rVB3	1530	1671	0.24%	0.022%
12	4.696	281	282	284	rBV2	1928	1496	0.22%	0.020%
13	4.931	320	322	325	rBV	2037	1496	0.22%	0.020%
14	5.055	340	343	344	rBV3	1529	1490	0.22%	0.020%
15	5.777	464	466	468	rBV3	1208	1218	0.18%	0.016%
16	6.576	600	602	604	rBV2	1253	1332	0.19%	0.018%
17	6.729	625	628	629	rBV	1412	1287	0.19%	0.017%
18	7.128	690	696	710	rVB	111704	202806	29.39%	2.708%
19	7.281	714	722	734	rBV	74619	132295	19.17%	1.767%
20	7.493	751	758	767	rVB	111093	200287	29.03%	2.675%
21	7.640	782	783	786	rVB	1729	1122	0.16%	0.015%
22	7.669	786	788	794	rBV3	1190	2072	0.30%	0.028%
23	7.734	797	799	800	rBV	1139	1037	0.15%	0.014%
24	7.957	831	837	846	rBV	89548	155654	22.56%	2.079%
25	8.157	869	871	873	rBV2	1044	1009	0.15%	0.013%
26	8.491	926	928	932	rVB4	1150	1184	0.17%	0.016%
27	8.679	952	960	970	rBV	133533	246631	35.74%	3.293%
28	8.814	980	983	985	rBV3	941	1189	0.17%	0.016%
29	8.879	991	994	996	rBV2	1354	1393	0.20%	0.019%
30	9.061	1022	1025	1028	rBV3	923	1289	0.19%	0.017%
31	9.132	1029	1037	1045	rVV	113321	201885	29.26%	2.696%
32	9.502	1096	1100	1101	rBV	886	1069	0.15%	0.014%
33	9.672	1127	1129	1135	rVB4	824	1607	0.23%	0.021%
34	9.860	1154	1161	1169	rVB	103354	188523	27.32%	2.517%
35	10.342	1237	1243	1247	rBV3	1148	2207	0.32%	0.029%
36	10.406	1247	1254	1265	rBV	137842	260870	37.81%	3.484%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083021\
 Data File : BG050090.D
 Acq On : 1 Sep 2021 9:35
 Operator : CG/JU
 Sample : PB138604BL
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK604

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
 Title : SVOA CALIBRATION

37	10.659	1294	1297	1300	rBV2	822	1375	0.20%	0.018%
38	10.776	1310	1317	1327	rBV	125097	226649	32.85%	3.027%
39	10.917	1333	1341	1349	rBV	136336	253828	36.79%	3.390%
40	11.393	1418	1422	1425	rVB	976	1371	0.20%	0.018%
41	11.893	1505	1507	1508	rBV2	1155	1017	0.15%	0.014%
42	12.280	1571	1573	1576	rVB2	901	1120	0.16%	0.015%
43	12.321	1576	1580	1582	rBV2	799	1152	0.17%	0.015%
44	12.380	1584	1590	1595	rBV3	2552	5891	0.85%	0.079%
45	13.255	1734	1739	1742	rBV2	1093	1953	0.28%	0.026%
46	13.737	1818	1821	1824	rVB	1071	1072	0.16%	0.014%
47	13.814	1831	1834	1836	rBV	1307	1203	0.17%	0.016%
48	13.896	1844	1848	1851	rVB	1301	1532	0.22%	0.020%
49	14.019	1863	1869	1878	rVB	271218	387781	56.20%	5.178%
50	14.313	1913	1919	1928	rVB	289947	459435	66.58%	6.135%
51	14.618	1965	1971	1980	rVB	197105	318996	46.23%	4.260%
52	14.853	2005	2011	2028	rBV2	81980	163695	23.72%	2.186%
53	15.447	2109	2112	2114	rBV	1074	1091	0.16%	0.015%
54	15.617	2132	2141	2148	rBV	368827	562405	81.51%	7.510%
55	15.758	2160	2165	2176	rBV	80790	132476	19.20%	1.769%
56	15.858	2176	2182	2186	rVB4	3746	6125	0.89%	0.082%
57	16.028	2209	2211	2216	rBV	1280	1758	0.25%	0.023%
58	16.310	2256	2259	2263	rVB	932	1180	0.17%	0.016%
59	16.398	2270	2274	2276	rVB	1300	1380	0.20%	0.018%
60	17.050	2384	2385	2388	rVB	1074	1006	0.15%	0.013%
61	17.373	2431	2440	2446	rBV	258073	383354	55.56%	5.119%
62	17.473	2450	2457	2464	rBV2	416406	609170	88.28%	8.135%
63	18.730	2670	2671	2674	rBV2	1692	1662	0.24%	0.022%
64	18.883	2695	2697	2698	rBV2	1461	1015	0.15%	0.014%
65	18.989	2713	2715	2717	rBV2	1120	1213	0.18%	0.016%
66	19.012	2717	2719	2724	rVB2	1539	1709	0.25%	0.023%
67	19.071	2727	2729	2732	rVV2	1650	1199	0.17%	0.016%
68	19.130	2736	2739	2742	rVB2	1354	1814	0.26%	0.024%
69	19.159	2742	2744	2747	rBV	1735	1510	0.22%	0.020%
70	19.183	2747	2748	2751	rBV	1097	1203	0.17%	0.016%
71	19.218	2753	2754	2757	rBV2	1639	1381	0.20%	0.018%
72	19.330	2770	2773	2777	rVB2	3632	3715	0.54%	0.050%
73	19.365	2777	2779	2781	rVB2	1581	1313	0.19%	0.018%
74	19.400	2781	2785	2788	rBV2	6452	8618	1.25%	0.115%
75	19.453	2793	2794	2797	rBV2	2088	1240	0.18%	0.017%
76	19.500	2797	2802	2804	rBV4	2808	5515	0.80%	0.074%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083021\
 Data File : BG050090.D
 Acq On : 1 Sep 2021 9:35
 Operator : CG/JU
 Sample : PB138604BL
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK604

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
 Title : SVOA CALIBRATION

77	19.547	2808	2810	2812	rBV2	2072	2044	0.30%	0.027%
78	19.706	2835	2837	2839	rVB2	1683	1454	0.21%	0.019%
79	19.764	2839	2847	2853	rBV	477514	690019	100.00%	9.214%
80	19.841	2858	2860	2862	rVB3	1984	1477	0.21%	0.020%
81	19.864	2862	2864	2866	rBV	1405	1188	0.17%	0.016%
82	19.894	2868	2869	2871	rBV	2614	1980	0.29%	0.026%
83	19.999	2886	2887	2890	rVB2	1684	1035	0.15%	0.014%
84	20.023	2890	2891	2894	rVB	2706	2203	0.32%	0.029%
85	20.134	2908	2910	2911	rBV2	2030	1721	0.25%	0.023%
86	20.211	2921	2923	2924	rBV	2323	1107	0.16%	0.015%
87	20.381	2950	2952	2955	rVB4	1628	1047	0.15%	0.014%
88	20.481	2967	2969	2970	rBV2	1697	1371	0.20%	0.018%
89	20.716	3007	3009	3013	rVB3	2839	2826	0.41%	0.038%
90	20.745	3013	3014	3016	rBV2	2608	2024	0.29%	0.027%
91	20.833	3027	3029	3030	rBV2	2588	1743	0.25%	0.023%
92	20.916	3041	3043	3045	rBV3	2782	1839	0.27%	0.025%
93	21.650	3162	3168	3176	rVB	241981	383734	55.61%	5.124%
94	23.107	3414	3416	3417	rBV	6316	4640	0.67%	0.062%
95	23.459	3474	3476	3477	rBV2	4725	3331	0.48%	0.044%
96	24.652	3670	3679	3691	rVB3	227146	637404	92.37%	8.512%
97	24.875	3707	3717	3728	rVB	142540	413956	59.99%	5.528%
98	26.297	3957	3959	3964	rBV6	4443	6236	0.90%	0.083%
99	26.908	4062	4063	4066	rVB2	7903	4209	0.61%	0.056%
100	30.362	4649	4651	4653	rBV2	4058	2721	0.39%	0.036%


Sum of corrected areas: 7488512

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083021\
Data File : BG050090.D
Acq On : 1 Sep 2021 9:35
Operator : CG/JU
Sample : PB138604BL
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK604

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

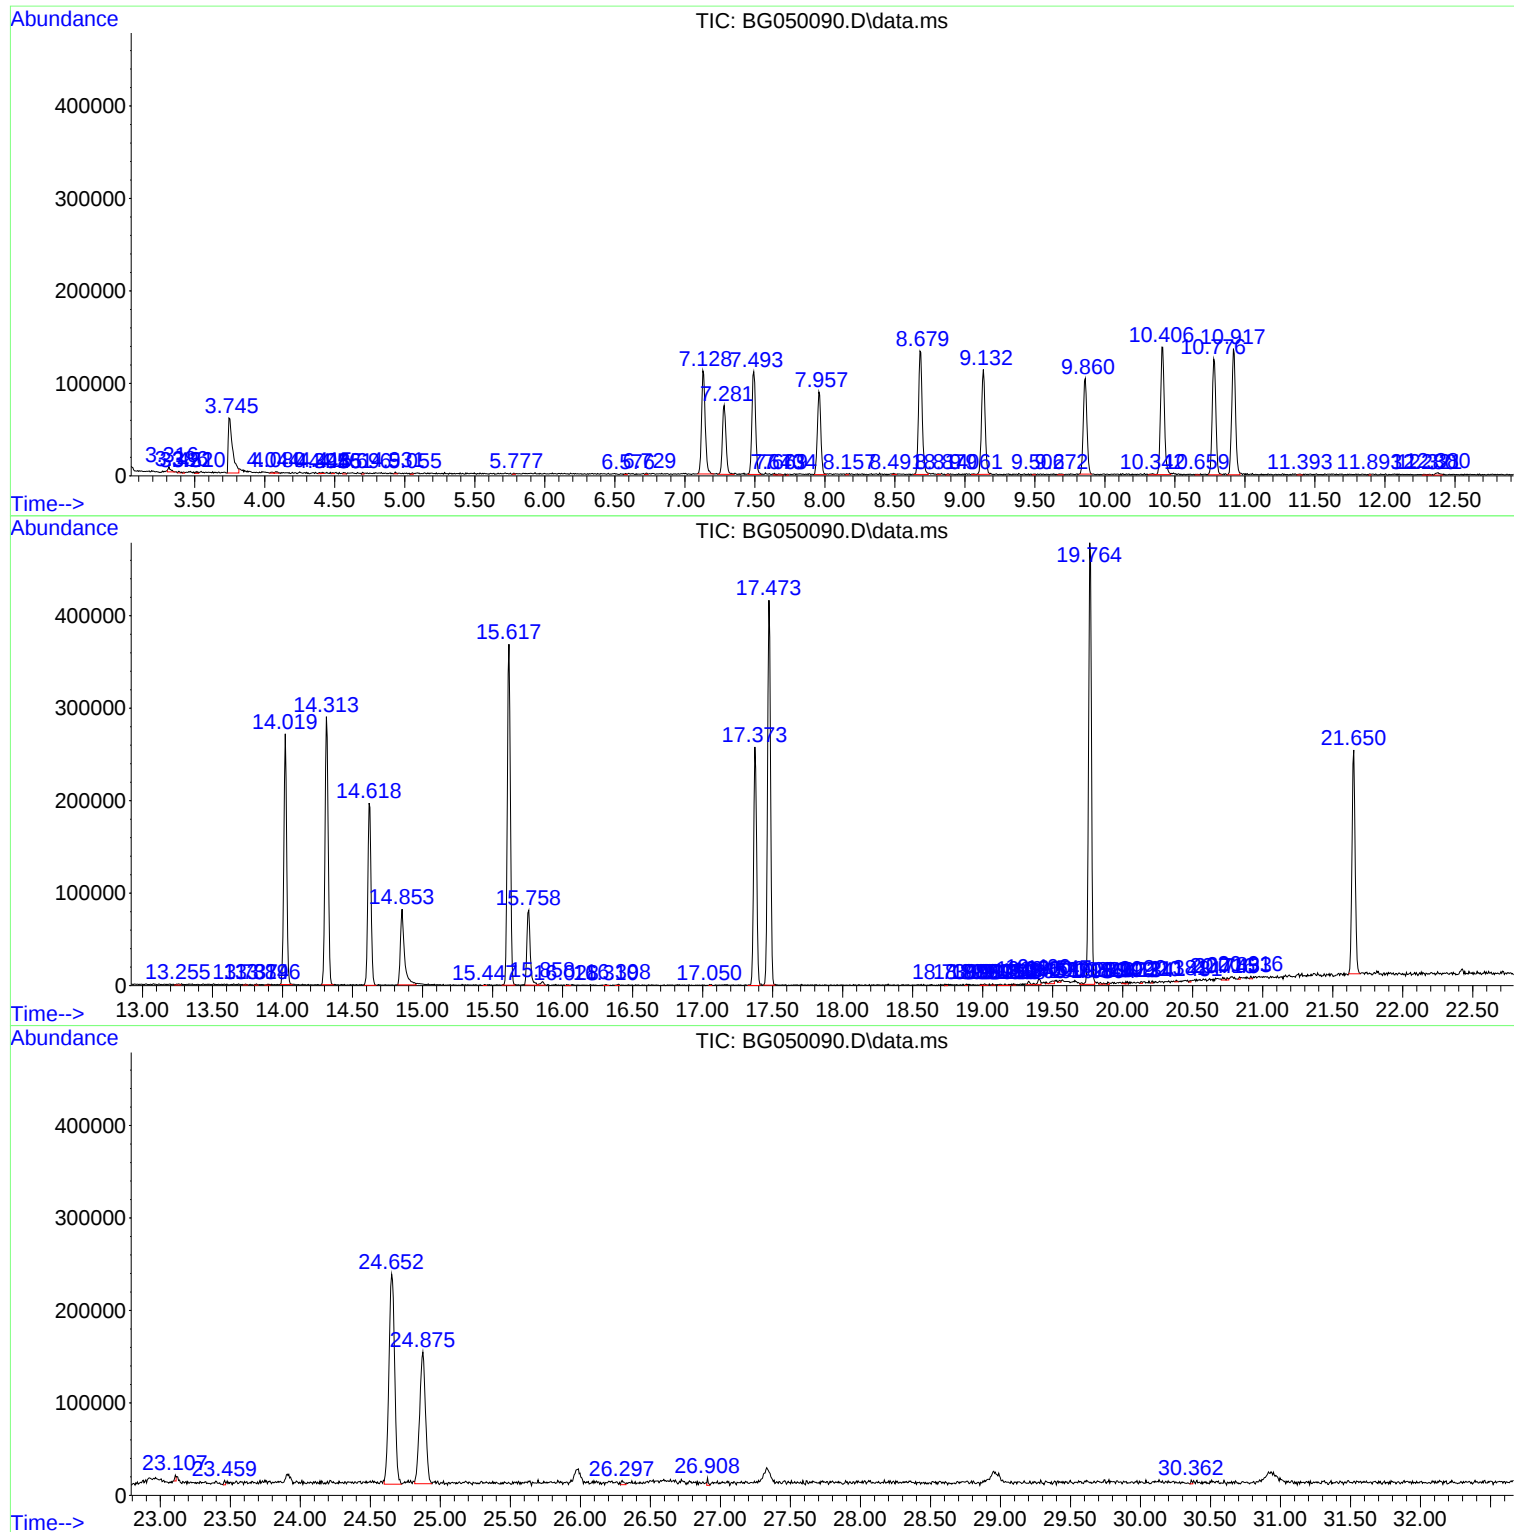

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083021\
Data File : BG050090.D
Acq On : 1 Sep 2021 9:35
Operator : CG/JU
Sample : PB138604BL
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK604

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083021\
Data File : BG050090.D
Acq On : 1 Sep 2021 9:35
Operator : CG/JU
Sample : PB138604BL
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK604

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
