

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083021\
 Data File : BG050095.D
 Acq On : 1 Sep 2021 13:01
 Operator : CG/JU
 Sample : M3464-07DL2 100X
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBKG0DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
 Title : SVOA CALIBRATION

Signal : TIC: BG050095.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.079	175	177	181	rVB	2303	1958	0.42%	0.068%
2	5.431	404	407	410	rVB3	3966	4418	0.94%	0.154%
3	7.034	677	680	681	rBV2	1052	1154	0.24%	0.040%
4	7.957	831	837	846	rVB	100930	172477	36.56%	6.004%
5	8.333	895	901	908	rBV	39452	66628	14.12%	2.319%
6	8.497	926	929	930	rBV2	2591	2125	0.45%	0.074%
7	10.171	1209	1214	1216	rBV2	2667	3223	0.68%	0.112%
8	10.412	1250	1255	1263	rVB5	5213	9757	2.07%	0.340%
9	10.776	1310	1317	1322	rBV	140080	256980	54.47%	8.946%
10	10.829	1322	1326	1333	rVB	115885	205674	43.60%	7.160%
11	10.953	1342	1347	1352	rVB2	8431	13537	2.87%	0.471%
12	11.605	1456	1458	1459	rBV	1332	1143	0.24%	0.040%
13	12.227	1562	1564	1568	rBV	1023	1205	0.26%	0.042%
14	12.445	1593	1601	1608	rBV	31636	52421	11.11%	1.825%
15	12.574	1619	1623	1628	rVB2	4410	6182	1.31%	0.215%
16	12.662	1633	1638	1645	rVB	21182	37317	7.91%	1.299%
17	13.455	1768	1773	1777	rVB4	4881	8802	1.87%	0.306%
18	13.937	1849	1855	1859	rBV3	3581	7414	1.57%	0.258%
19	13.990	1862	1864	1866	rBV2	1870	1512	0.32%	0.053%
20	14.178	1893	1896	1902	rVB2	1387	1833	0.39%	0.064%
21	14.313	1917	1919	1921	rBV2	2116	2411	0.51%	0.084%
22	14.618	1965	1971	1978	rBV	226782	359097	76.12%	12.501%
23	14.689	1978	1983	1989	rVB2	35888	54296	11.51%	1.890%
24	14.759	1992	1995	1999	rVB2	4071	4966	1.05%	0.173%
25	14.900	2015	2019	2020	rBV2	2324	2383	0.51%	0.083%
26	15.018	2035	2039	2044	rBV	14086	21027	4.46%	0.732%
27	15.417	2104	2107	2110	rBV	1175	1347	0.29%	0.047%
28	15.464	2110	2115	2117	rBV	935	1658	0.35%	0.058%
29	15.617	2137	2141	2146	rVB	4567	5497	1.17%	0.191%
30	15.670	2146	2150	2155	rBV2	14368	20823	4.41%	0.725%
31	16.093	2219	2222	2226	rVB	989	1156	0.25%	0.040%
32	16.181	2232	2237	2242	rBV3	1748	2476	0.52%	0.086%
33	16.345	2261	2265	2272	rBV3	2797	6011	1.27%	0.209%
34	16.557	2298	2301	2302	rBV	1280	1348	0.29%	0.047%
35	16.580	2302	2305	2311	rVB5	3288	5489	1.16%	0.191%
36	16.639	2312	2315	2318	rVV4	2296	2545	0.54%	0.089%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083021\
 Data File : BG050095.D
 Acq On : 1 Sep 2021 13:01
 Operator : CG/JU
 Sample : M3464-07DL2 100X
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBKG0DL2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
 Title : SVOA CALIBRATION

37	16.856	2349	2352	2353	rBV4	1968	1779	0.38%	0.062%
38	17.168	2400	2405	2408	rBV3	4327	6063	1.29%	0.211%
39	17.373	2435	2440	2446	rBV	291677	431379	91.44%	15.017%
40	17.473	2454	2457	2462	rVB4	5088	7845	1.66%	0.273%
41	17.784	2500	2510	2518	rVB	49825	76018	16.11%	2.646%
42	17.884	2523	2527	2533	rBV3	4467	8565	1.82%	0.298%
43	17.949	2534	2538	2542	rVB2	5945	7841	1.66%	0.273%
44	18.213	2580	2583	2584	rBV2	2581	2542	0.54%	0.088%
45	18.301	2595	2598	2602	rBV3	4024	5335	1.13%	0.186%
46	18.384	2608	2612	2616	rBV	4176	6301	1.34%	0.219%
47	18.548	2636	2640	2642	rBV4	1821	3367	0.71%	0.117%
48	18.636	2651	2655	2658	rVB	981	1300	0.28%	0.045%
49	18.695	2660	2665	2669	rBV3	1554	2668	0.57%	0.093%
50	18.836	2688	2689	2693	rVB3	1245	1199	0.25%	0.042%
51	19.071	2726	2729	2731	rBV	1171	1243	0.26%	0.043%
52	19.259	2759	2761	2766	rVB2	1230	1673	0.35%	0.058%
53	19.312	2768	2770	2773	rBV	1058	1364	0.29%	0.047%
54	19.764	2844	2847	2852	rVB	5785	8416	1.78%	0.293%
55	19.905	2869	2871	2873	rBV	1824	1607	0.34%	0.056%
56	20.169	2913	2916	2920	rBV3	2535	3585	0.76%	0.125%
57	20.228	2922	2926	2933	rBV	8705	16598	3.52%	0.578%
58	20.322	2941	2942	2945	rBV2	2190	2264	0.48%	0.079%
59	20.381	2950	2952	2955	rBV4	2997	3174	0.67%	0.110%
60	21.650	3162	3168	3174	rBV2	288284	450367	95.47%	15.678%
61	24.875	3709	3717	3728	rVB3	160729	471755	100.00%	16.423%




Sum of corrected areas: 2872538

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083021\
Data File : BG050095.D
Acq On : 1 Sep 2021 13:01
Operator : CG/JU
Sample : M3464-07DL2 100X
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBKG0DL2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

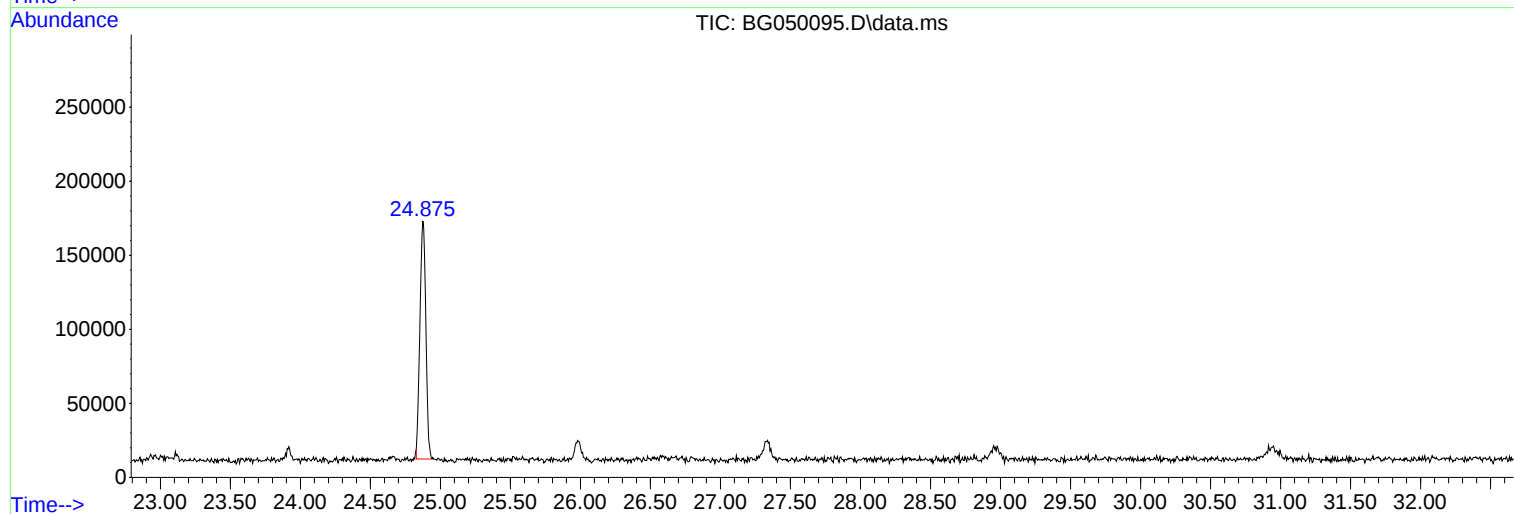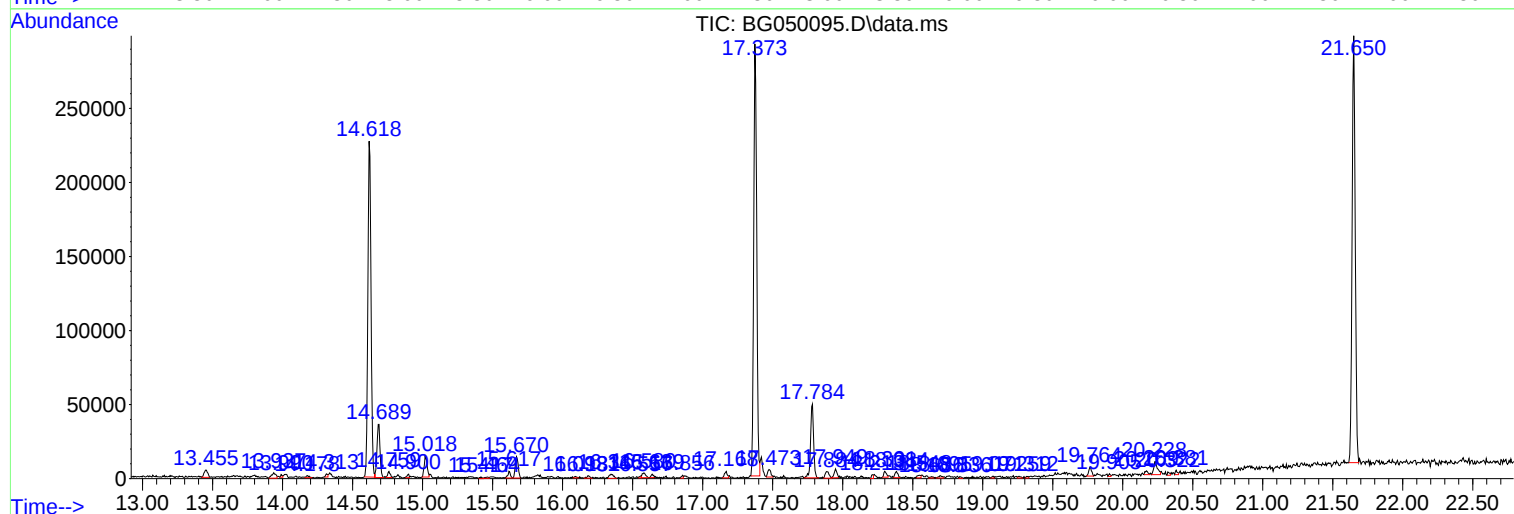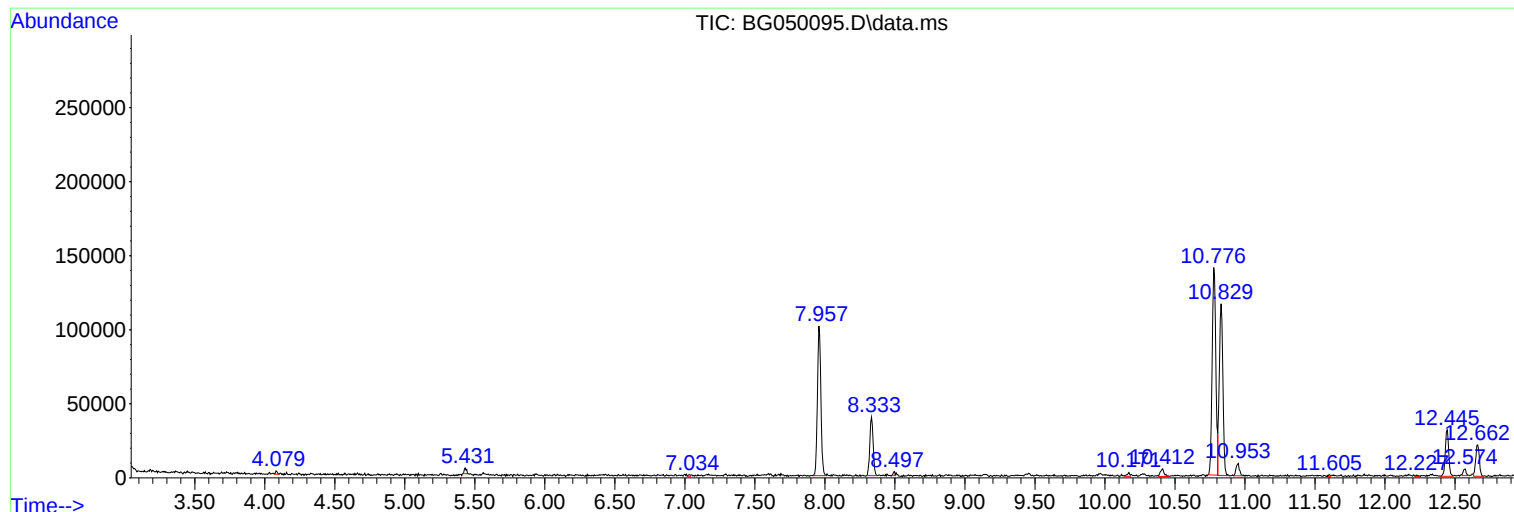

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083021\
Data File : BG050095.D
Acq On : 1 Sep 2021 13:01
Operator : CG/JU
Sample : M3464-07DL2 100X
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBKG0DL2










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Indane Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.333	7.73 ng/ul	66628	1,4-Dichlorobenzene-d4	7.962

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Indane			118	C9H10	000496-11-7	81
2	Benzene, cyclopropyl-			118	C9H10	000873-49-4	64
3	Indane			118	C9H10	000496-11-7	64
4	Indane			118	C9H10	000496-11-7	59
5	Benzene, (2-bromocyclopropyl)-			196	C9H9Br	036617-02-4	53

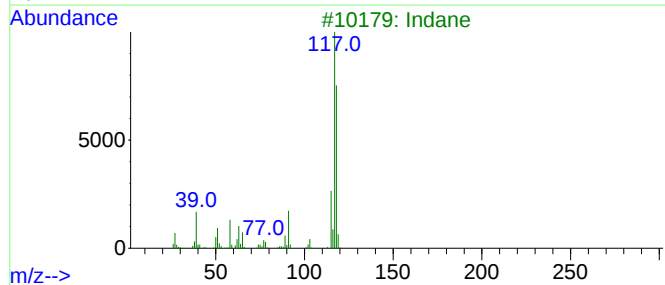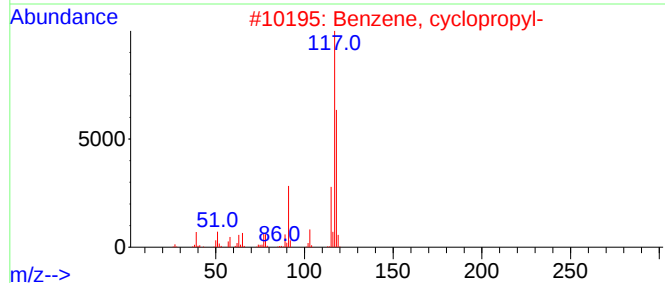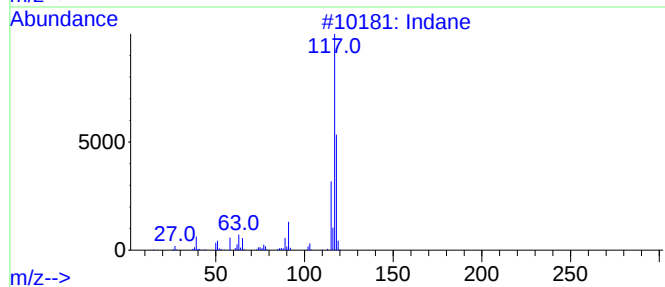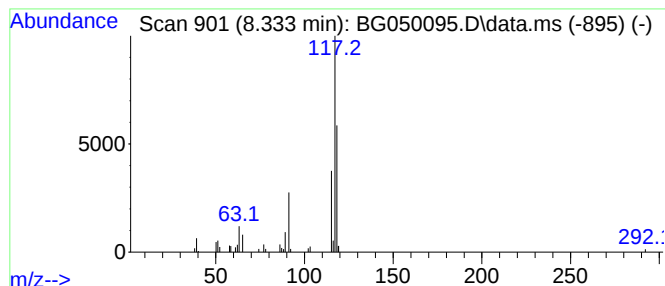

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083021\
Data File : BG050095.D
Acq On : 1 Sep 2021 13:01
Operator : CG/JU
Sample : M3464-07DL2 100X
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBKG0DL2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Indane	8.333	7.7	ng/ul	66628	1	7.962	172477	20.0