


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083022\
 Data File : BG054782.D
 Acq On : 30 Aug 2022 9:30
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 25 17:50:55 2022

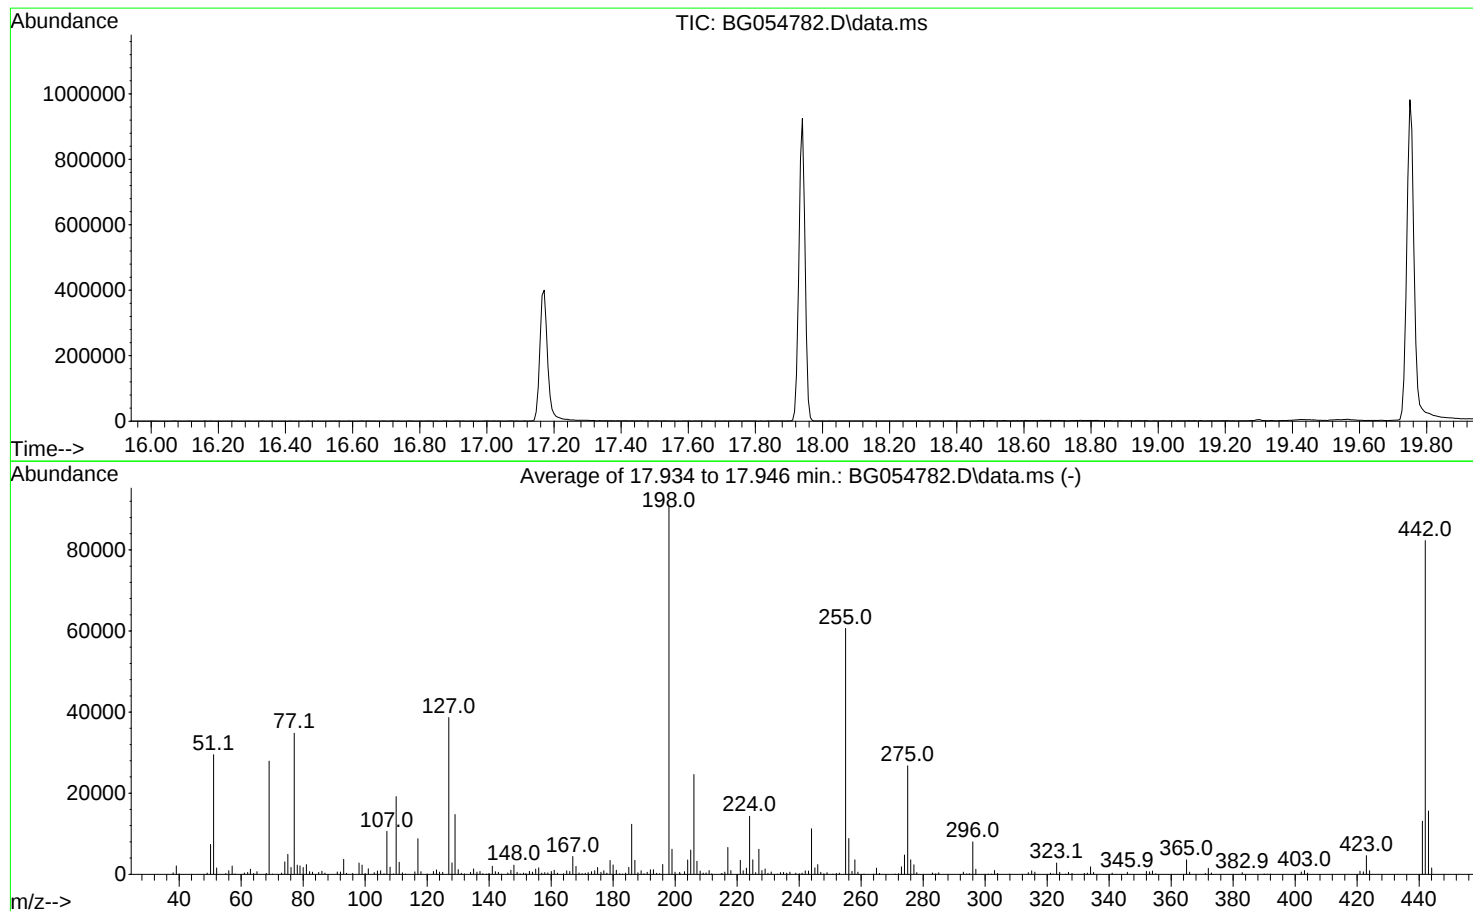




AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2486

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.5	29488	PASS
68	69	0.00	2	0.8	223	PASS
69	198	0.00	100	30.8	27912	PASS
70	69	0.00	2	0.2	53	PASS
127	198	10	80	42.6	38675	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	90725	PASS
199	198	5	9	6.8	6197	PASS
275	198	10	60	29.5	26744	PASS
365	198	1	100	4.0	3593	PASS
441	198	0.01	100	14.4	13084	PASS
442	442	50	100	100.0	82301	PASS
443	442	15	24	19.0	15603	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083022\
Data File : BG054782.D
Acq On : 30 Aug 2022 9:30
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 30 16:23:03 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 25 17:50:55 2022
Response via : Initial Calibration

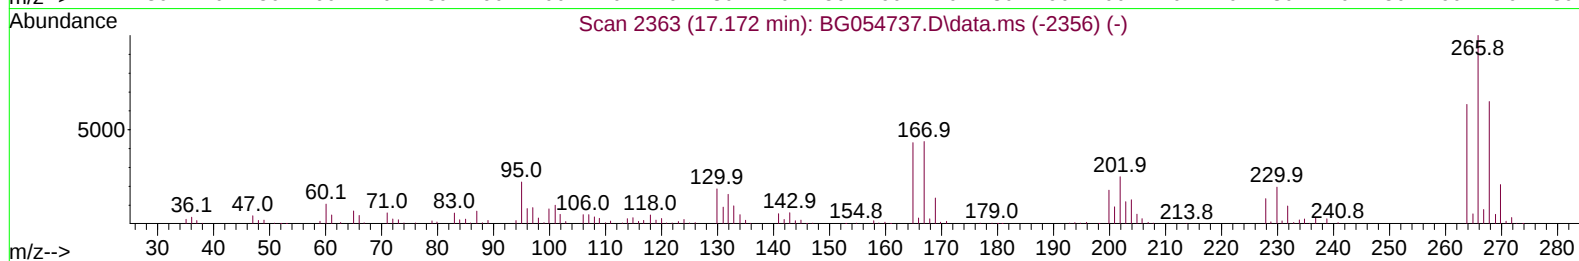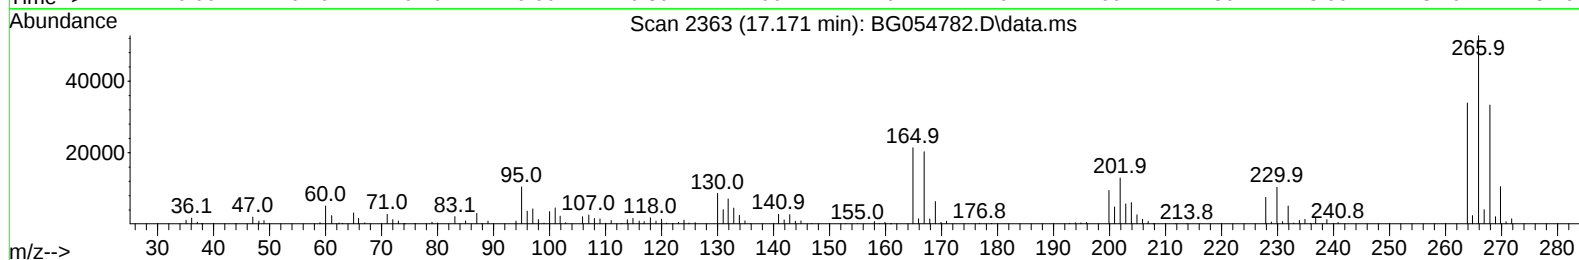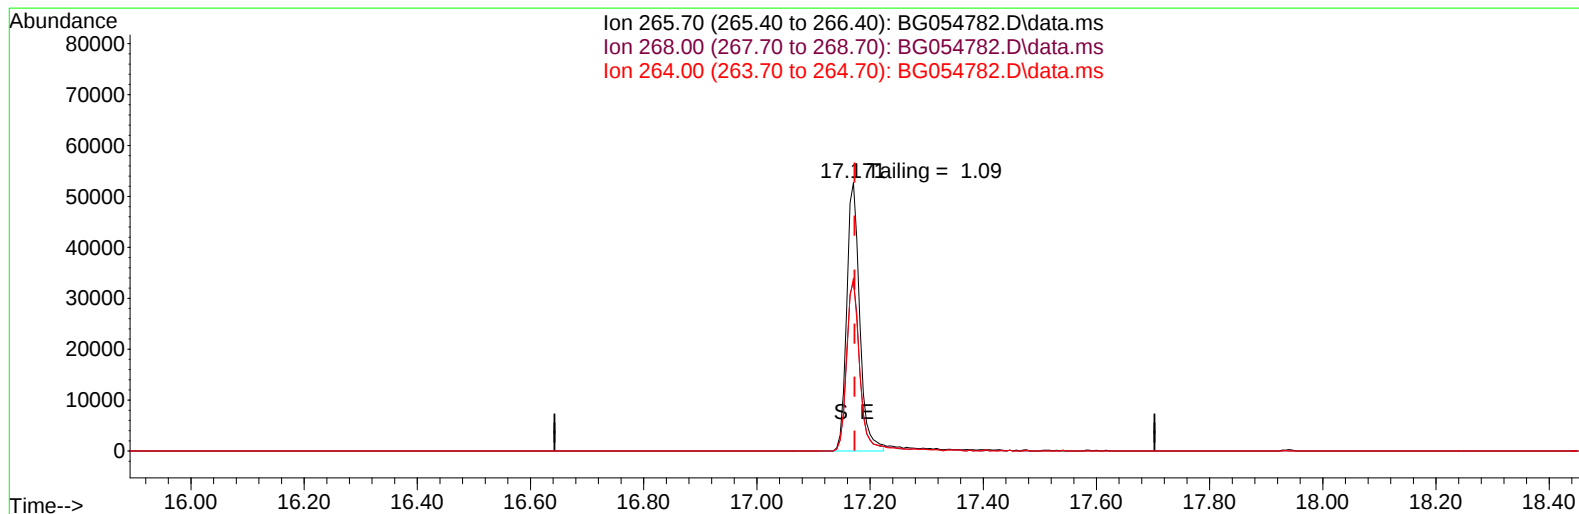

TIC: BG054782.D\data.ms

(70) Pentachlorophenol (C)

17.171min (-0.002) 22183.36 ng




response 86729

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	63.24
264.00	61.70	64.38
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083022\
Data File : BG054782.D
Acq On : 30 Aug 2022 9:30
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 30 16:23:03 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 25 17:50:55 2022
Response via : Initial Calibration

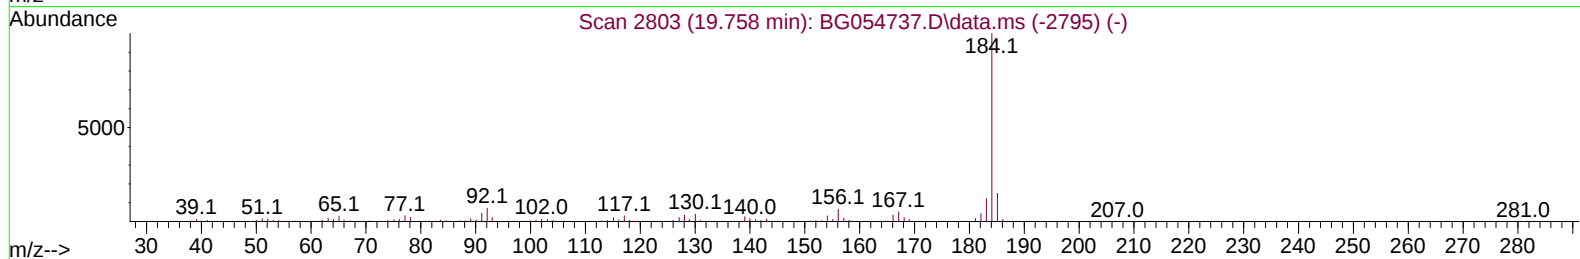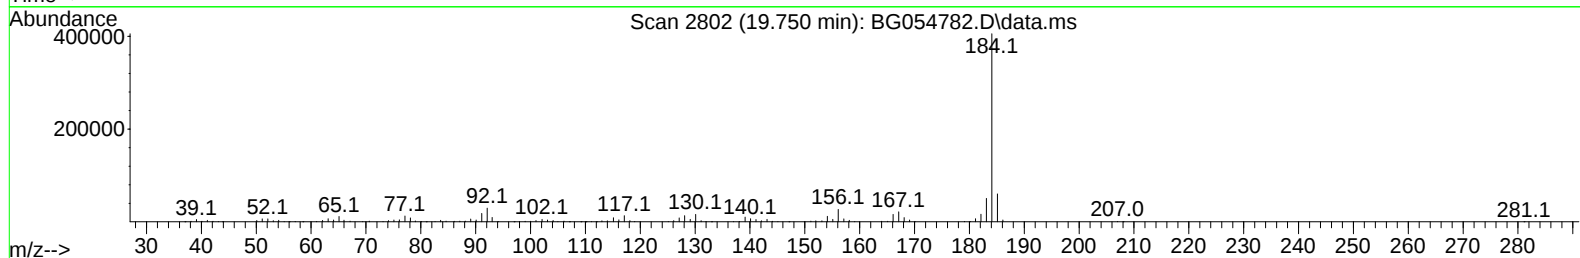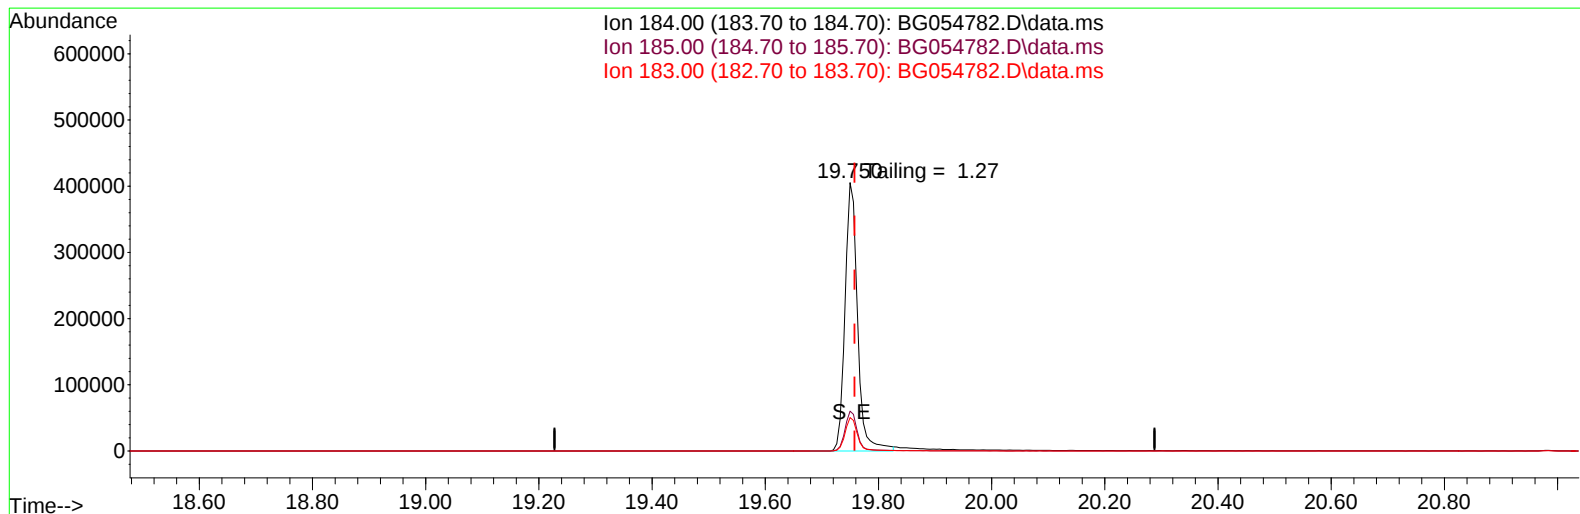

TIC: BG054782.D\data.ms

(77) Benzidine

19.750min (-0.008) 0.00 ng

response 640575

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.84
183.00	12.30	12.50
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/30/2022	BNA_G	BG054782.D
Compound Name	Response	Retention Time
DDT	304765	20.98
DDD	5599	20.53
DDE	0	19.9
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5599	310364	1.80

Instrument :
BNA_G
ClientSampleId :
DFTPP