
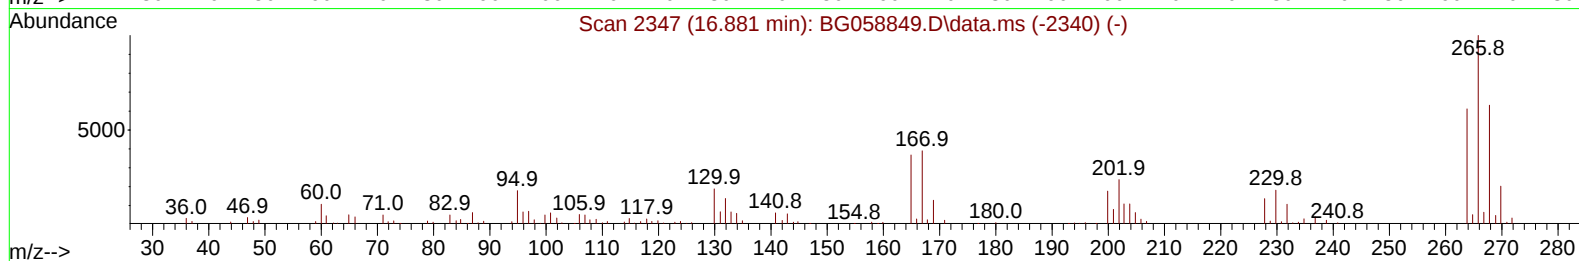
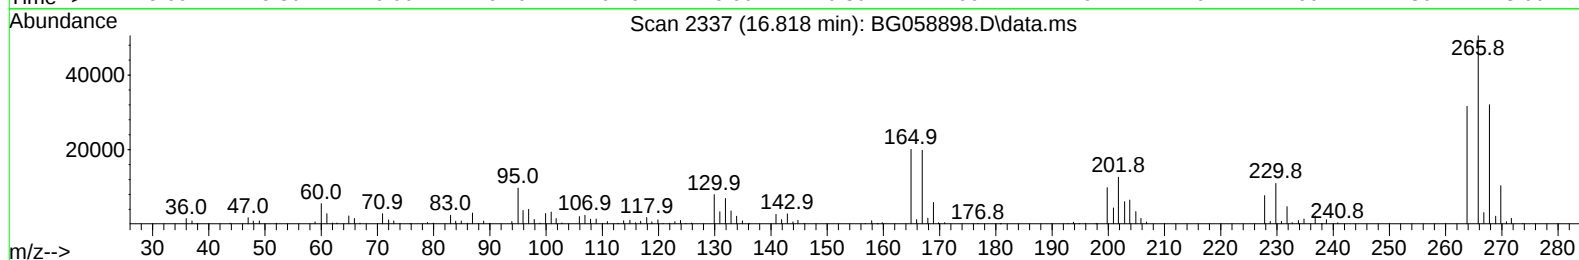


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083023\
Data File : BG058898.D
Acq On : 30 Aug 2023 16:17
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 31 04:51:21 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG081823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 31 01:27:35 2023
Response via : Initial Calibration

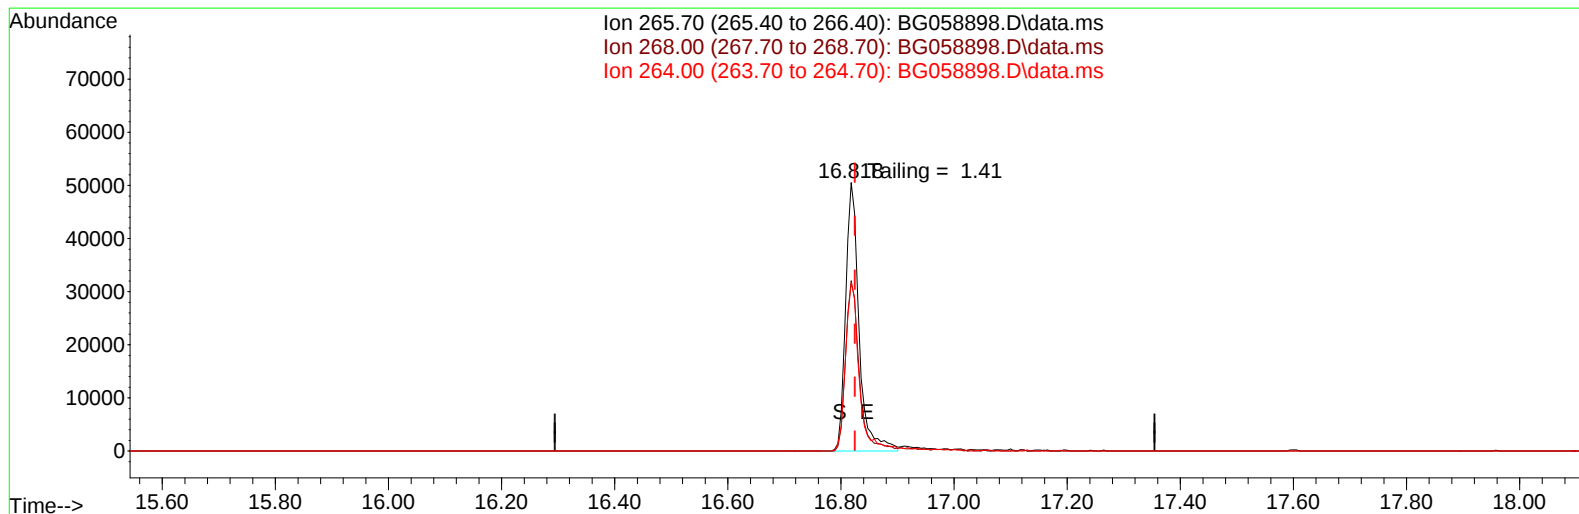

TIC: BG058898.D\data.ms

(70) Pentachlorophenol (C)




16.818min (-0.007) 37908.98 ng

response 83578

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.90	63.41
264.00	61.90	62.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083023\
Data File : BG058898.D
Acq On : 30 Aug 2023 16:17
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 31 04:51:21 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG081823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 31 01:27:35 2023
Response via : Initial Calibration

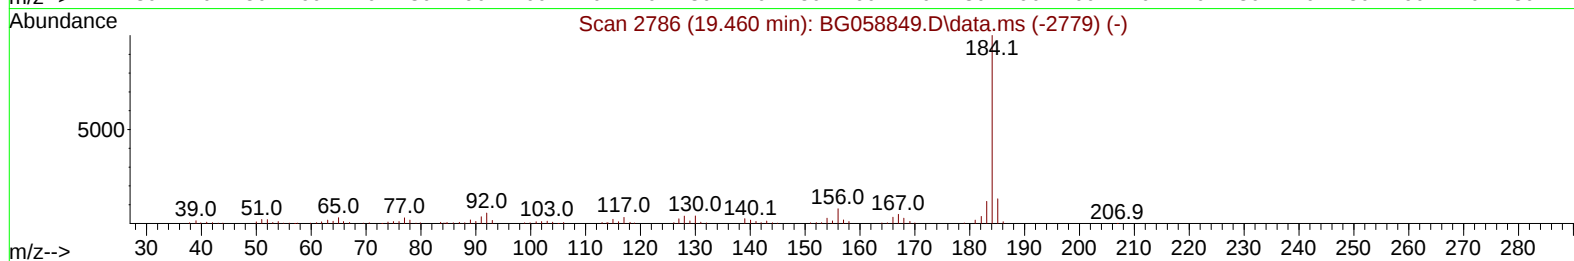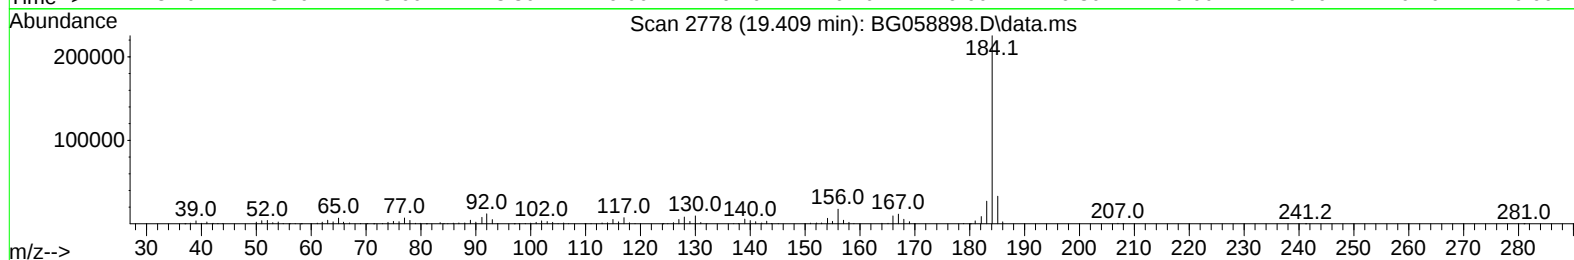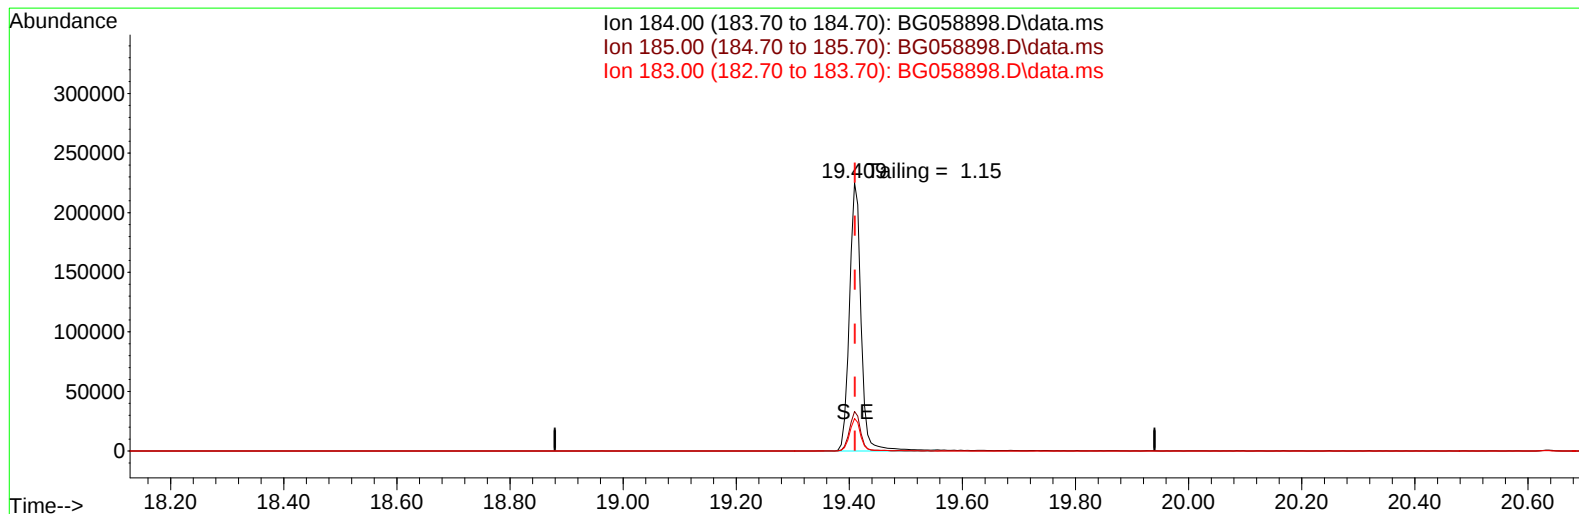

TIC: BG058898.D\data.ms

(77) Benzidine

19.409min (-0.001) 0.00 ng

response 321463

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.72
183.00	12.50	12.11
0.00	0.00	0.00