

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083023\
 Data File : BG058900.D
 Acq On : 30 Aug 2023 17:49
 Operator : MA/JU
 Sample : PB155191BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB155191BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG081823.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG058900.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.850	295	300	307	rBV	11871	17562	1.15%	0.305%
2	5.326	375	381	395	rVB	297128	456575	29.95%	7.919%
3	6.936	648	655	665	rBV	309401	516522	33.88%	8.958%
4	7.759	788	795	802	rVB	46543	72163	4.73%	1.252%
5	8.922	986	993	1010	rBV	174969	311183	20.41%	5.397%
6	10.556	1265	1271	1279	rBV	64129	113760	7.46%	1.973%
7	13.035	1686	1693	1700	rBV	497295	776284	50.92%	13.464%
8	14.410	1921	1927	1938	rBB	122451	193263	12.68%	3.352%
9	15.908	2175	2182	2197	rBV	548505	844313	55.38%	14.643%
10	17.160	2389	2395	2406	rBV	197918	288612	18.93%	5.006%
11	19.786	2836	2842	2850	rBV	1165870	1524597	100.00%	26.442%
12	21.396	3111	3116	3124	rBV2	186545	290292	19.04%	5.035%
13	21.578	3141	3147	3148	rBV5	10006	15696	1.03%	0.272%
14	24.428	3622	3632	3644	rBV2	115714	328085	21.52%	5.690%
15	25.444	3800	3805	3814	rBV2	6196	16903	1.11%	0.293%




Sum of corrected areas: 5765810

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083023\
Data File : BG058900.D
Acq On : 30 Aug 2023 17:49
Operator : MA/JU
Sample : PB155191BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB155191BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG081823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

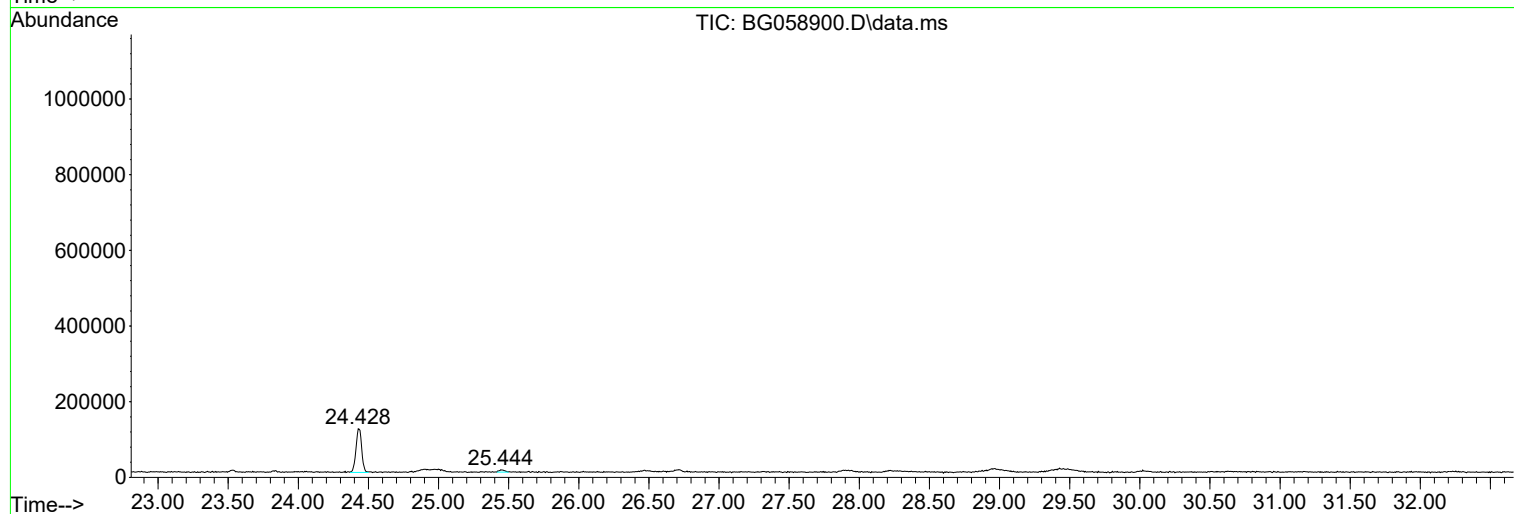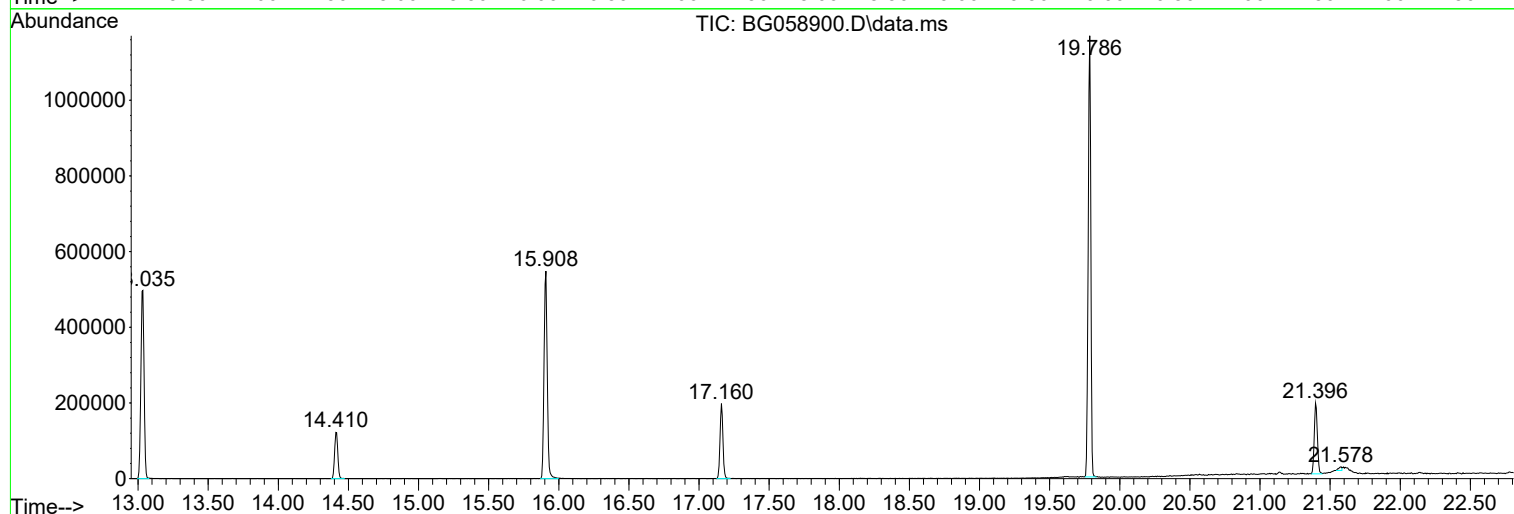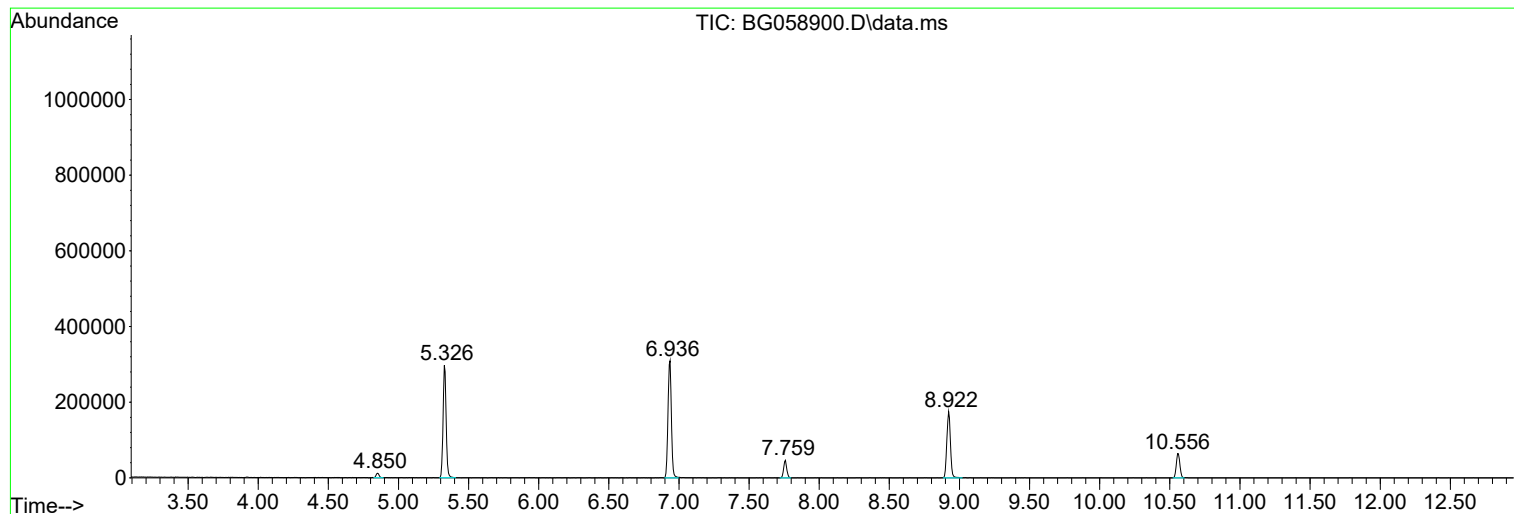

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083023\
Data File : BG058900.D
Acq On : 30 Aug 2023 17:49
Operator : MA/JU
Sample : PB155191BL
Misc :
ALS Vial : 3 Sample Multiplier: 1










Instrument :
BNA_G
ClientSampleId :
PB155191BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG081823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD			R.T.
4.850	4.87 ng	17562	1,4-Dichlorobenzene-d4			7.759
Hit# of 5	Tentative ID		MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-		116	C6H12O2	000123-42-2	72
2	Diacetamide		101	C4H7NO2	000625-77-4	7
3	2,3-Butanedione, monooxime		101	C4H7NO2	000057-71-6	7
4	2-Ethylbutylamine		101	C6H15N	000617-79-8	5
5	3,3-Dimethylbutylamine		101	C6H15N	015673-00-4	5

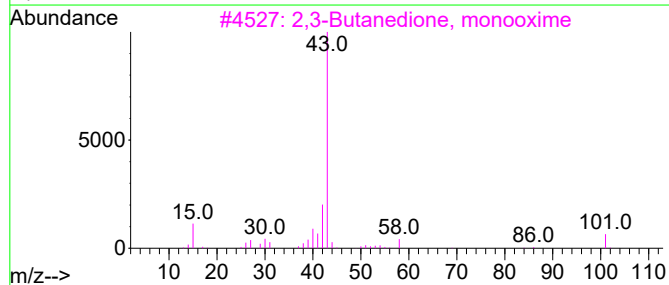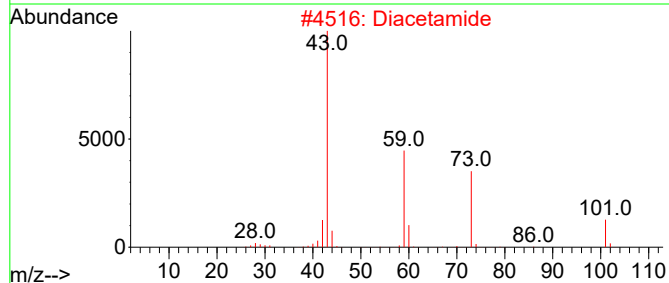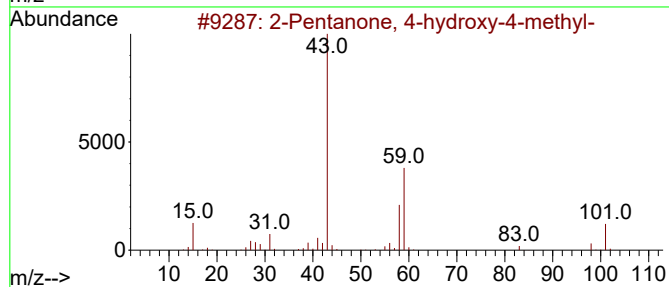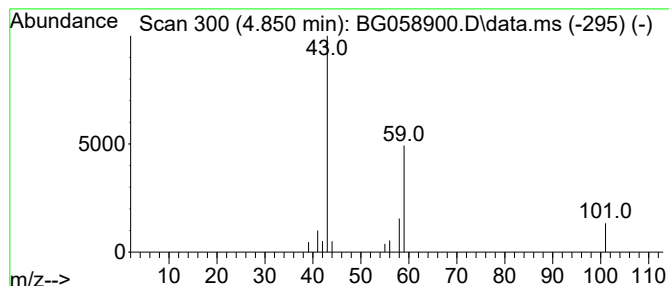

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083023\
Data File : BG058900.D
Acq On : 30 Aug 2023 17:49
Operator : MA/JU
Sample : PB155191BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB155191BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG081823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	4.850	4.9	ng	17562	1	7.759	72163	20.0