
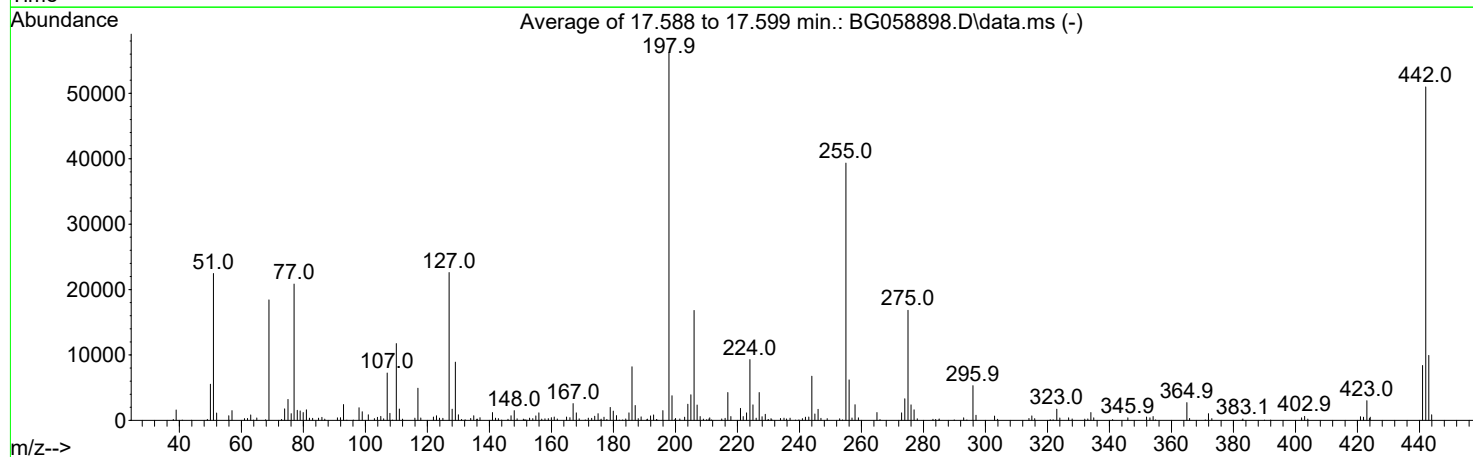


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083023\
Data File : BG058898.D
Acq On : 30 Aug 2023 16:17
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG081823.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Aug 31 01:27:35 2023

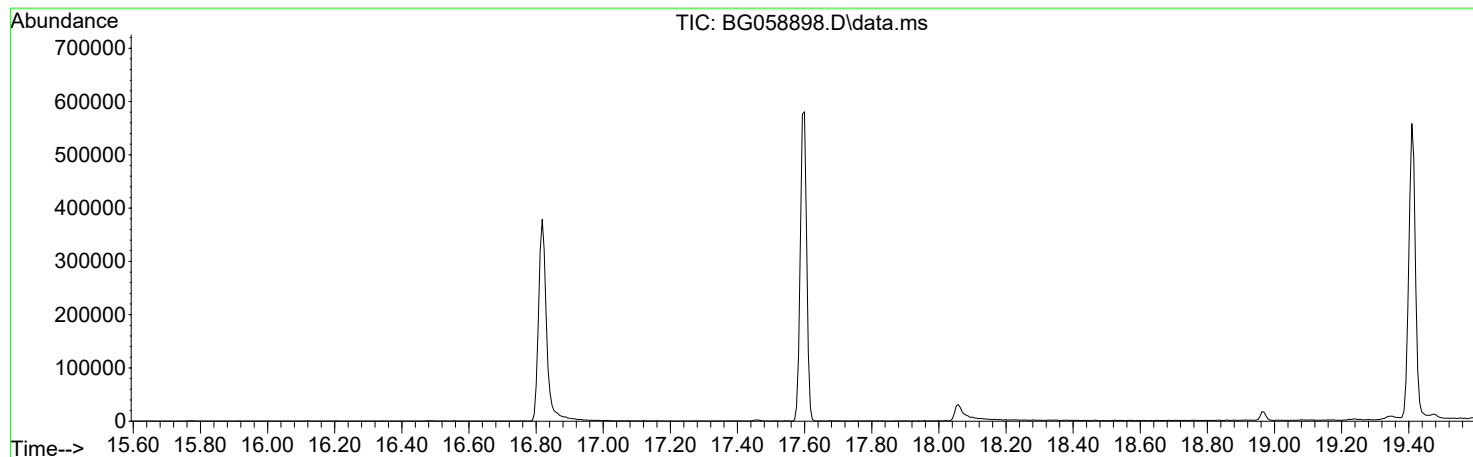

AutoFind: Scans 2468, 2469, 2470; Background Corrected with Scan 2462

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.9	22469	PASS
68	69	0.00	2	0.5	96	PASS
69	198	0.00	100	32.8	18422	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	40.2	22595	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	56245	PASS
199	198	5	9	6.7	3756	PASS
275	198	10	60	29.9	16830	PASS
365	198	1	100	4.9	2728	PASS
441	198	0.01	100	14.9	8399	PASS
442	442	50	100	100.0	50989	PASS
443	442	15	24	19.5	9941	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/30/2023	BNA_G	<u>BG058898.D</u>
Compound Name	Response	Retention Time
DDT	177669	20.637
DDD	3671	20.243
DDE	0	19.744
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3671	181340	2.02

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083023\
Data File : BG058898.D
Acq On : 30 Aug 2023 16:17
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 31 04:51:21 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG081823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 31 01:27:35 2023
Response via : Initial Calibration

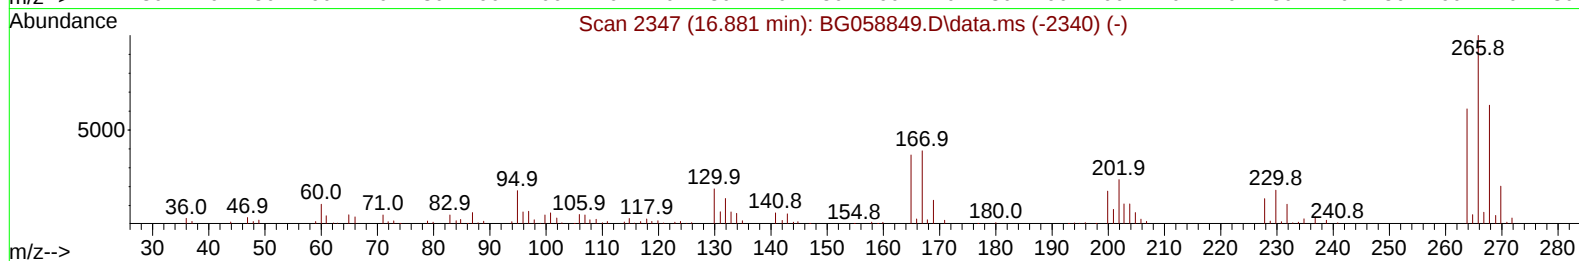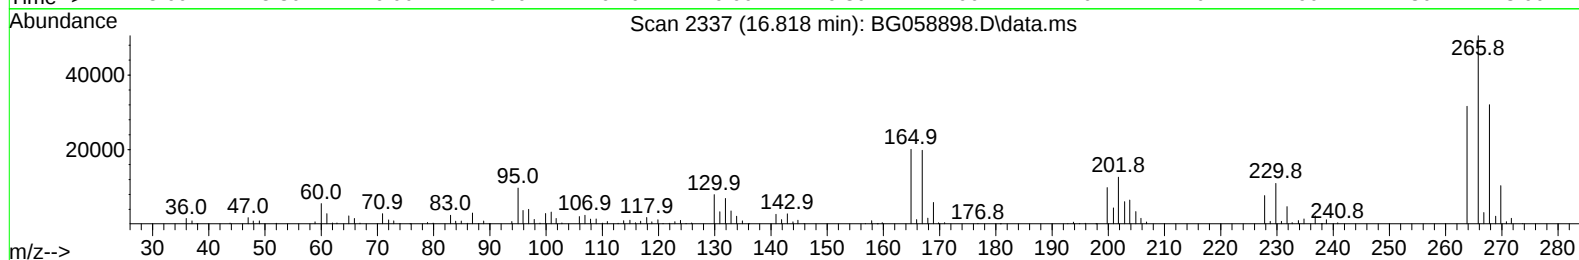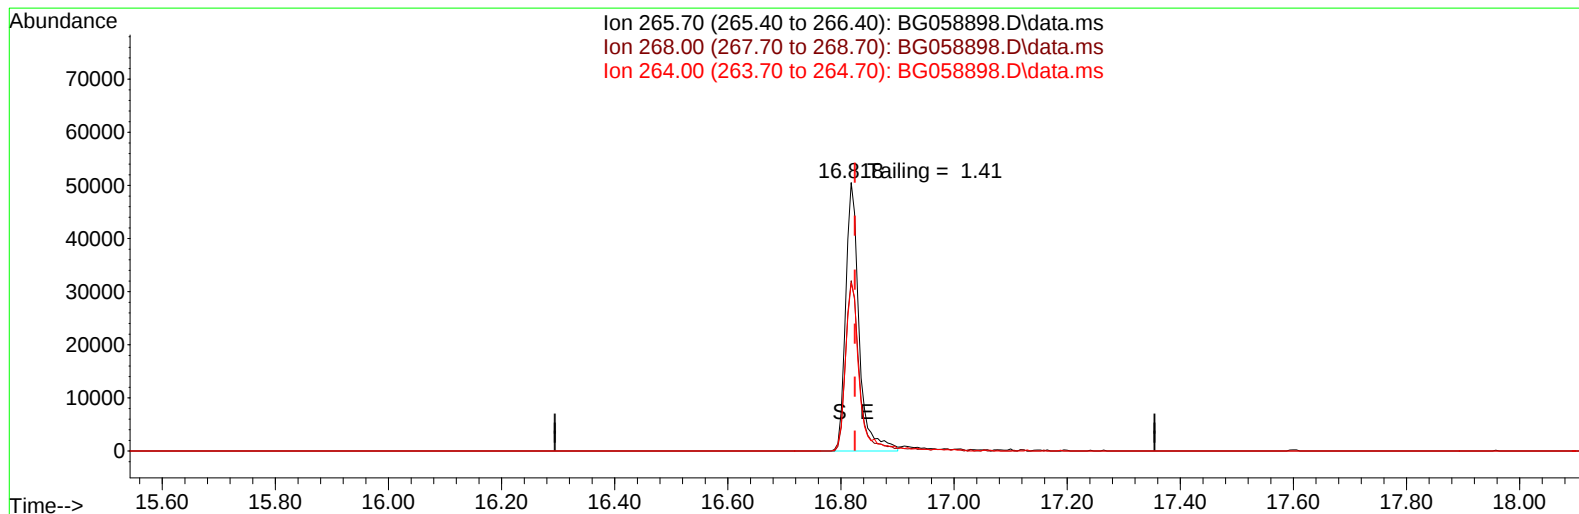

TIC: BG058898.D\data.ms

(70) Pentachlorophenol (C)

16.818min (-0.007) 37908.98 ng




response 83578

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.90	63.41
264.00	61.90	62.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083023\
Data File : BG058898.D
Acq On : 30 Aug 2023 16:17
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 31 04:51:21 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG081823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 31 01:27:35 2023
Response via : Initial Calibration

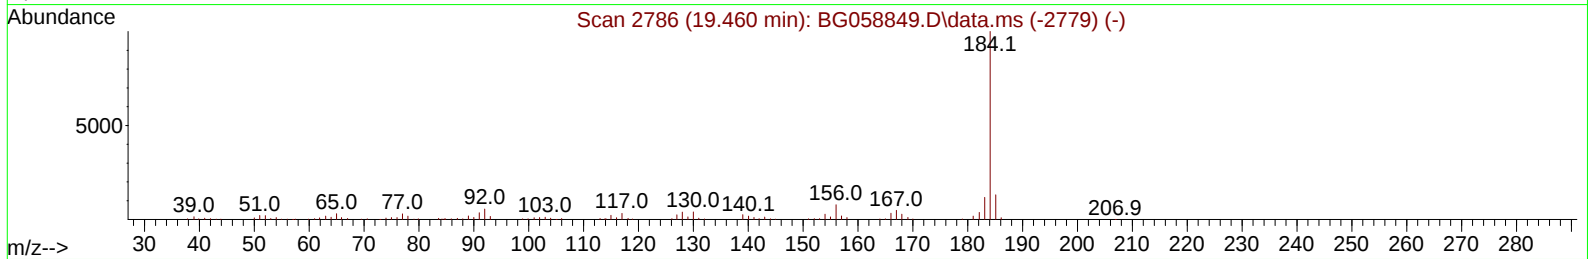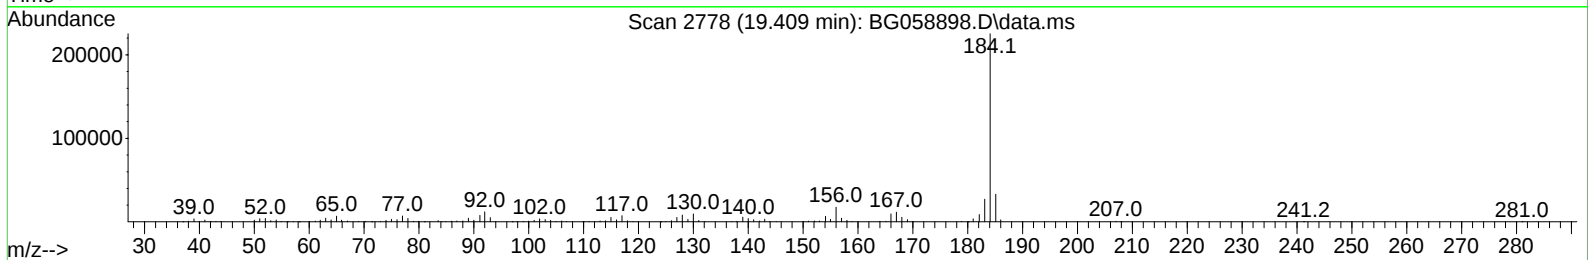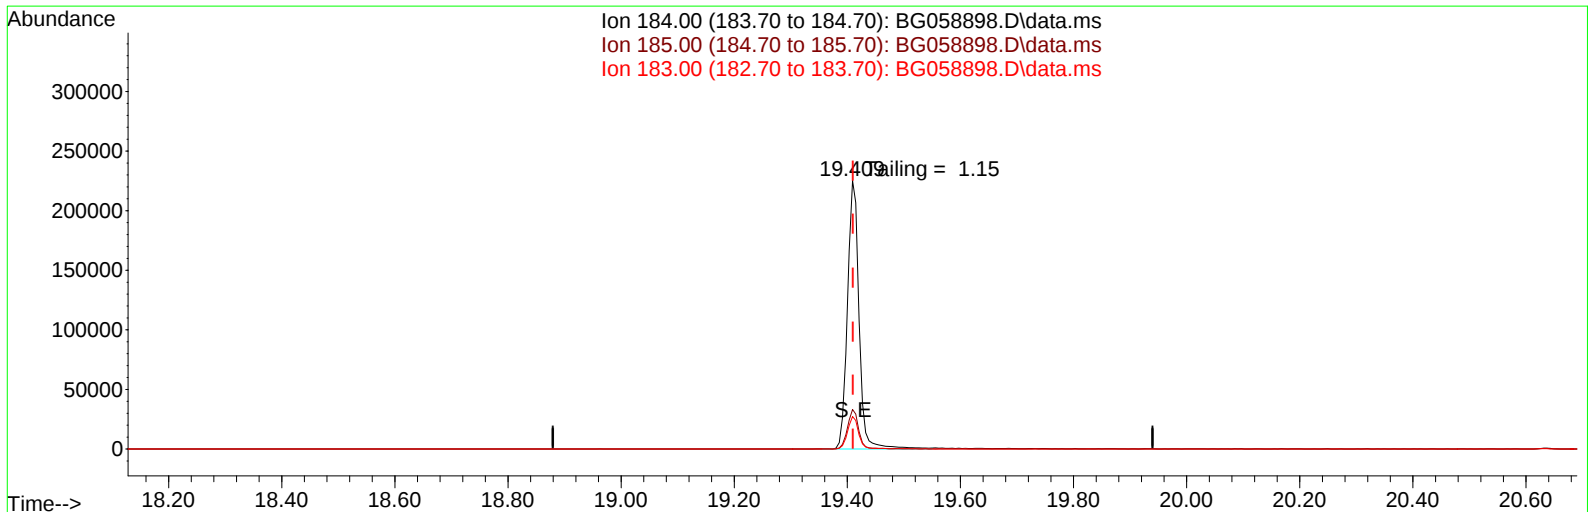

TIC: BG058898.D\data.ms

(77) Benzidine

19.409min (-0.001) 0.00 ng

response 321463

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.72
183.00	12.50	12.11
0.00	0.00	0.00