
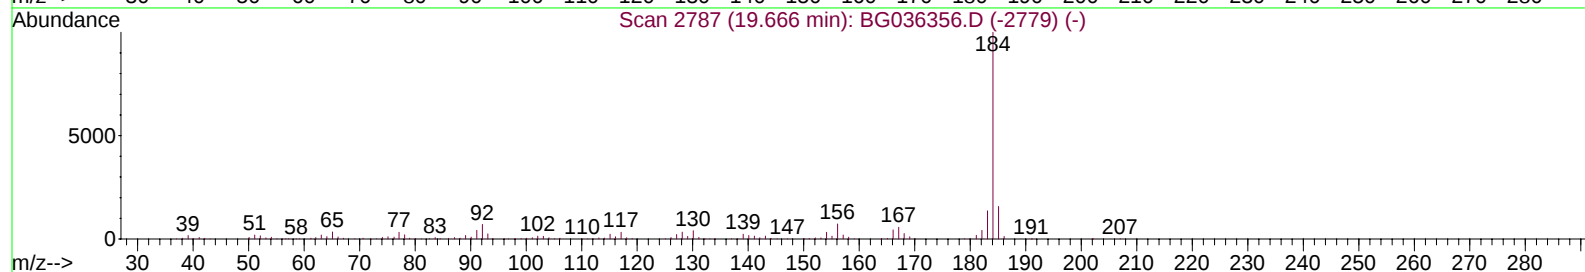
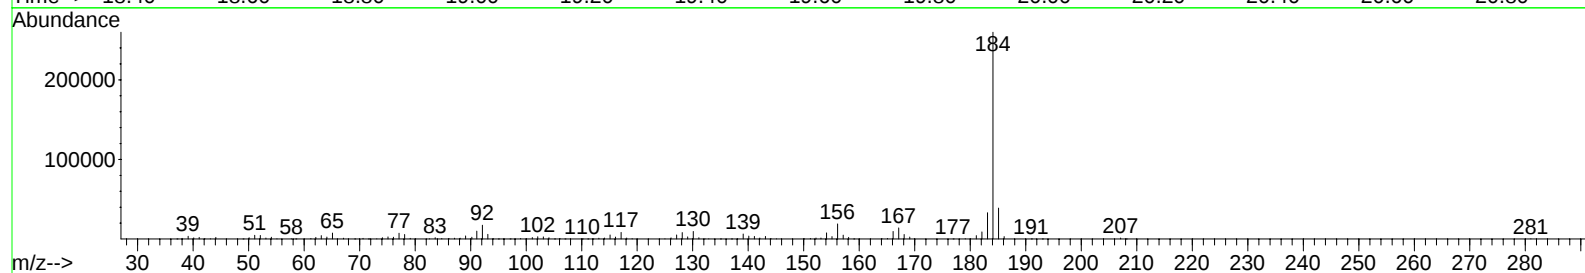


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG083118\
Data File : BG036499.D
Acq On : 31 Aug 2018 9:47
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 31 11:36:08 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 23 12:07:02 2018
Response via : Initial Calibration

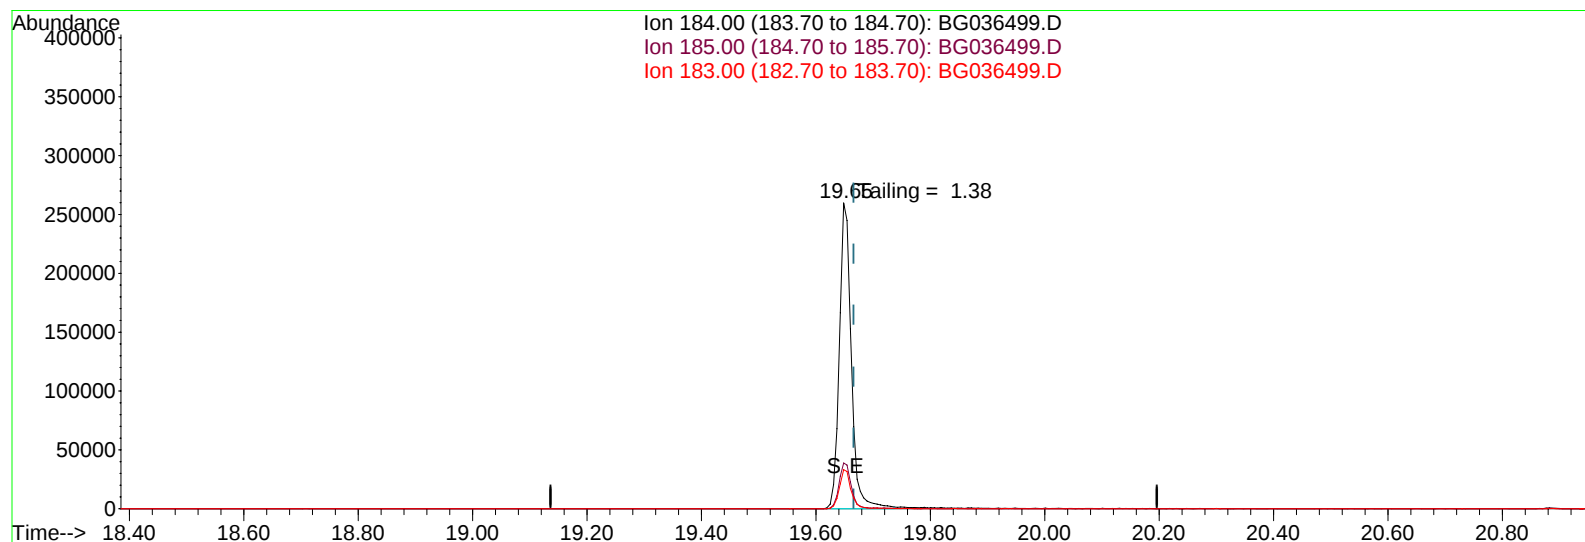

TIC: BG036499.D

(76) Benzidine




19.648min (-0.018) 11818.09ng

response 377050

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.97
183.00	13.60	12.78
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG083118\
Data File : BG036499.D
Acq On : 31 Aug 2018 9:47
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 31 11:36:08 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 23 12:07:02 2018
Response via : Initial Calibration

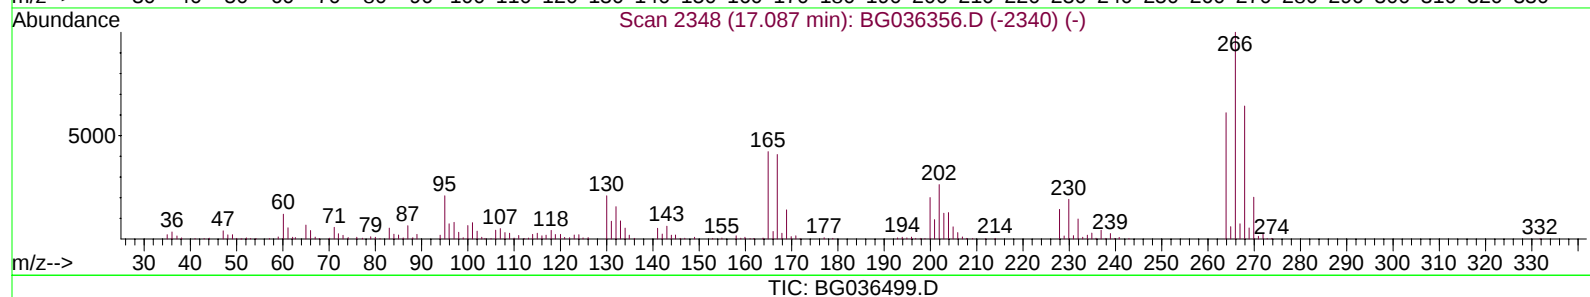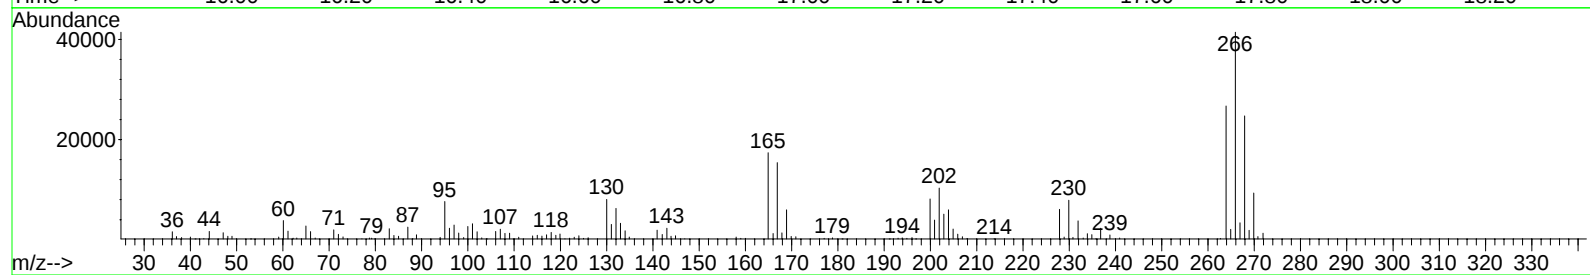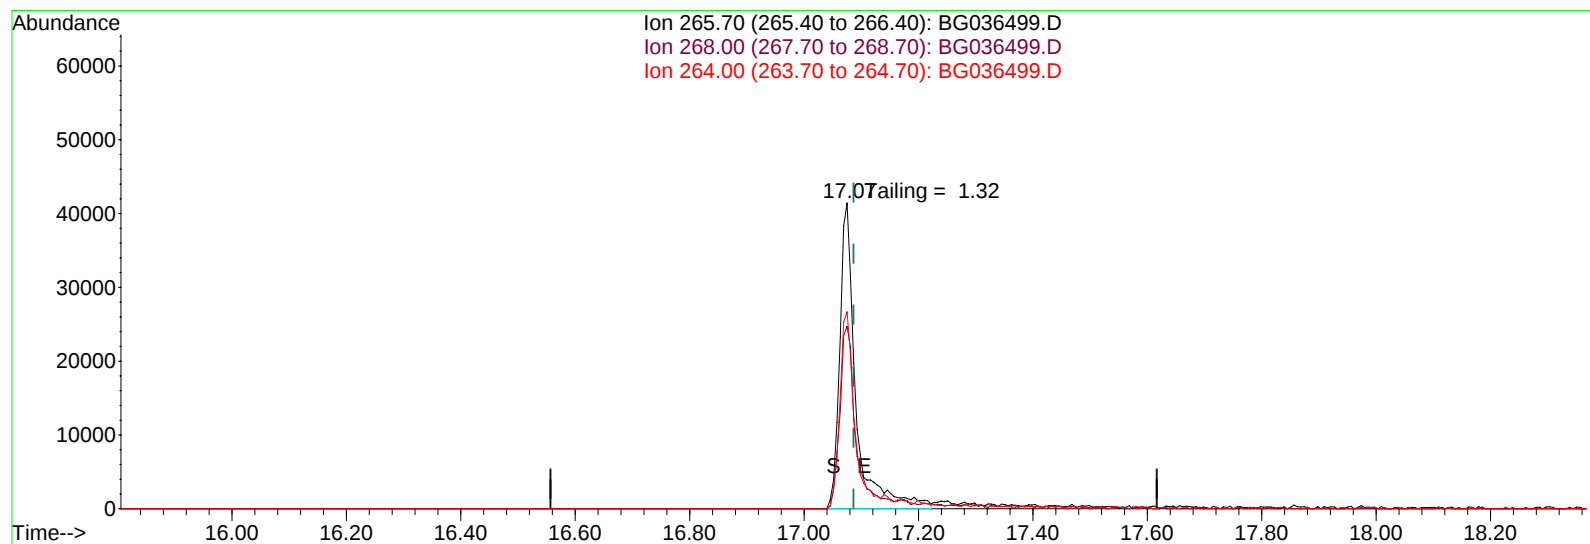

(69) Pentachlorophenol (C)

17.075min (-0.012) 8339.38ng

response 82238

Ion	Exp%	Act%
265.70	100	100
268.00	64.30	59.68
264.00	61.10	64.43
0.00	0.00	0.00