
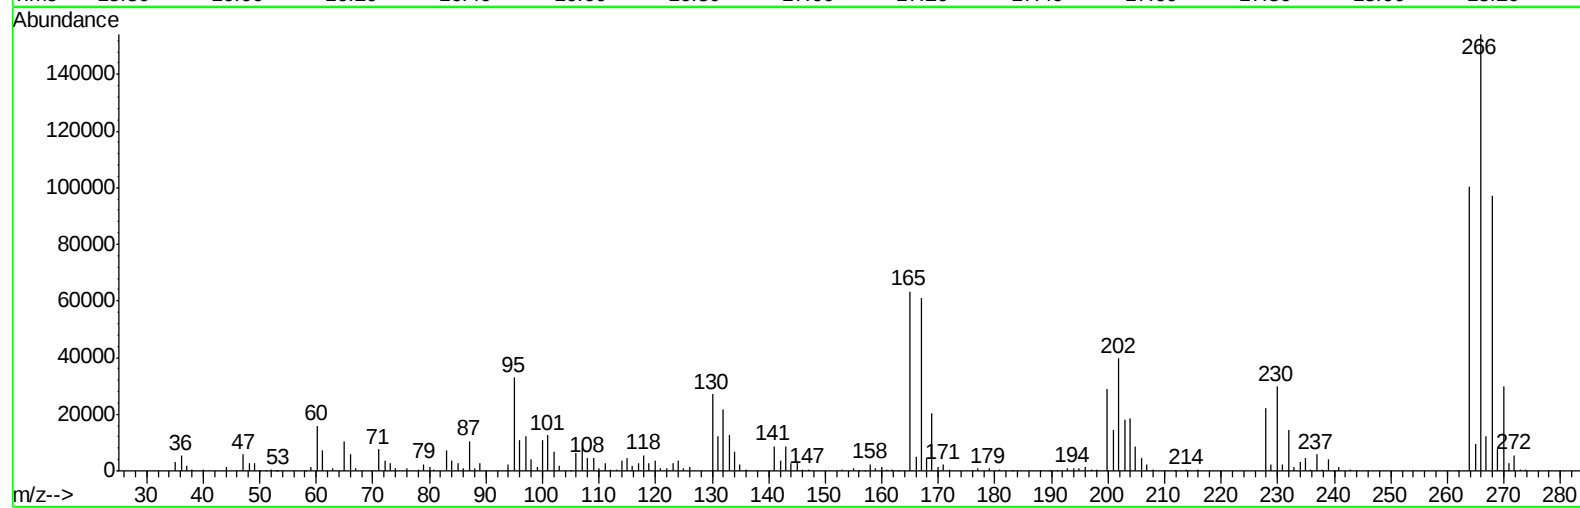


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG083118\
Data File : BG036516.D
Acq On : 31 Aug 2018 22:23
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 01 05:43:00 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 31 13:03:20 2018
Response via : Initial Calibration

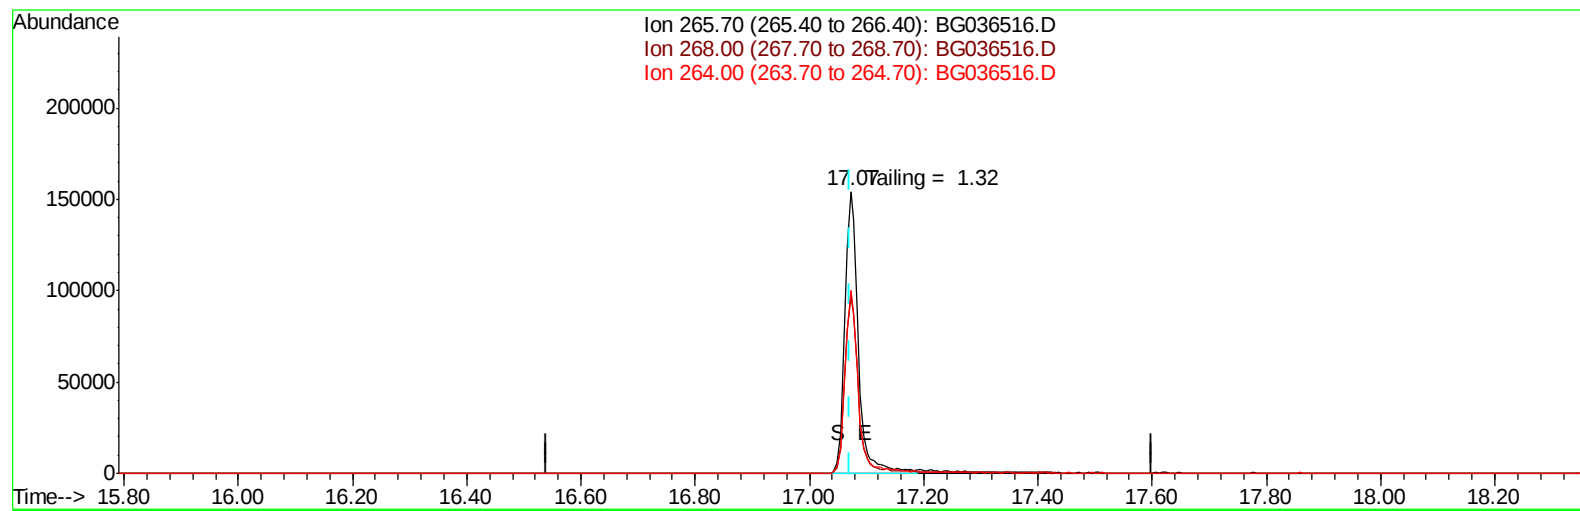

TIC: BG036516.D

(69) Pentachlorophenol (C)



17.072min (+0.001) 49796.23ng

response 254039

Ion	Exp%	Act%
265.70	100	100
268.00	64.30	62.96
264.00	61.10	65.18
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG083118\
Data File : BG036516.D
Acq On : 31 Aug 2018 22:23
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 01 05:43:00 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 31 13:03:20 2018
Response via : Initial Calibration

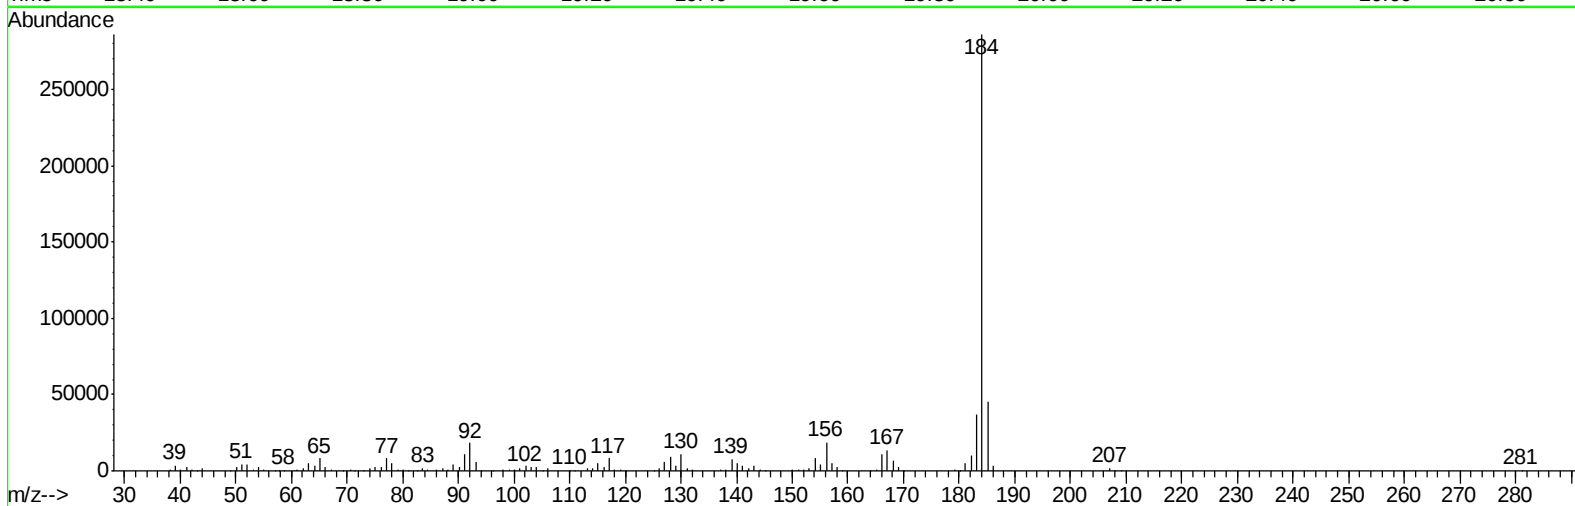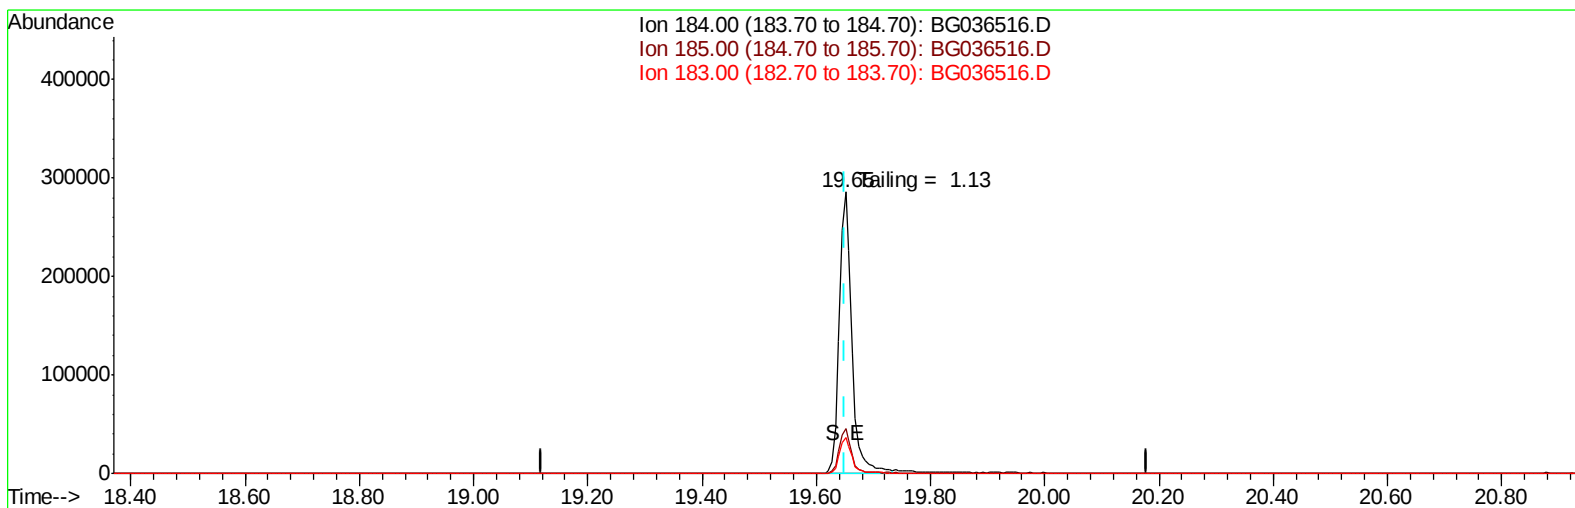

TIC: BG036516.D

(76) Benzidine

19.651min (+0.001) 25945.95ng

response 445352

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	15.84
183.00	13.60	12.93
0.00	0.00	0.00