


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG083118\
 Data File : BG036499.D
 Acq On : 31 Aug 2018 9:47
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 31 13:03:20 2018

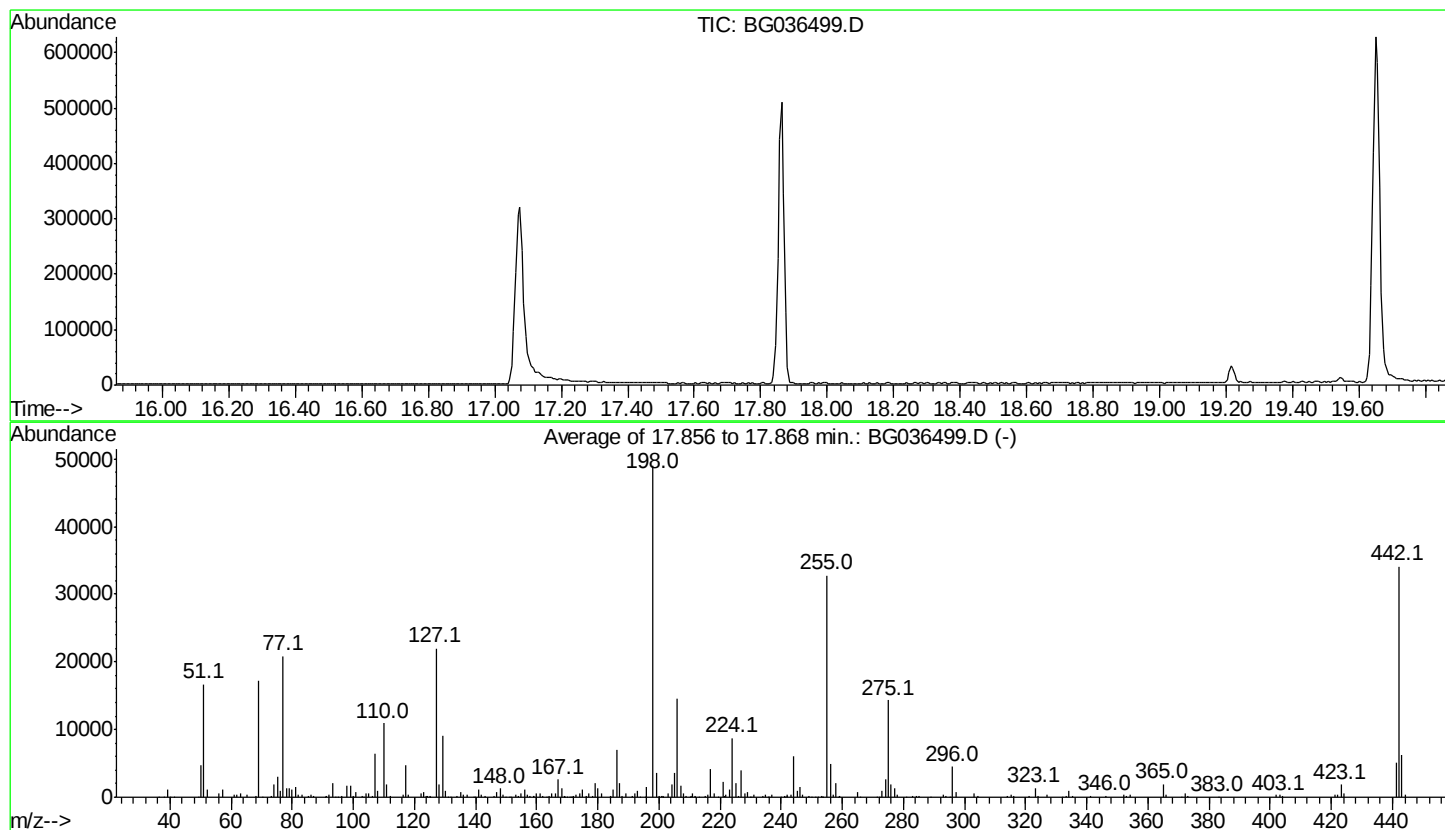

AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.2	16741	PASS
68	69	0.00	2	0.7	113	PASS
69	198	0.00	100	35.1	17207	PASS
70	69	0.00	2	0.4	72	PASS
127	198	10	80	44.9	21994	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	49008	PASS
199	198	5	9	7.2	3530	PASS
275	198	10	60	29.2	14324	PASS
365	198	1	100	3.9	1899	PASS
441	198	0.01	100	10.4	5115	PASS
442	198	50	100	69.5	34058	PASS
443	442	15	24	18.2	6182	PASS