

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG090120\
 Data File : BG046488.D
 Acq On : 1 Sep 2020 17:26
 Operator : CG/JU
 Sample : L3508-28
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 TR-08-082820

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.155	4	11	25	rVB	1179856	1868679	32.78%	7.741%
2	3.431	49	58	67	rVB	158516	204168	3.58%	0.846%
3	4.571	247	252	259	rBV	47933	67337	1.18%	0.279%
4	5.047	321	333	341	rBV2	241923	429411	7.53%	1.779%
5	5.517	406	413	425	rBV	1008128	1611025	28.26%	6.674%
6	7.103	675	683	697	rBV	855501	1486491	26.08%	6.158%
7	7.931	816	824	831	rBV	234600	396908	6.96%	1.644%
8	9.089	1009	1021	1035	rBV	704076	1303748	22.87%	5.401%
9	10.728	1293	1300	1315	rBV	309608	557745	9.79%	2.310%
10	13.184	1711	1718	1733	rBV	1984538	3107342	54.52%	12.872%
11	14.559	1942	1952	1961	rBV2	505967	812587	14.26%	3.366%
12	16.051	2199	2206	2220	rBV	1543758	2440381	42.82%	10.109%
13	17.303	2413	2419	2431	rBV	715594	1089974	19.12%	4.515%
14	19.923	2858	2865	2877	rBV	4330408	5699809	100.00%	23.612%
15	21.228	3083	3087	3092	rBV2	46866	63897	1.12%	0.265%
16	21.551	3135	3142	3149	rBV	838212	1328448	23.31%	5.503%
17	22.350	3273	3278	3289	rVB3	51680	100737	1.77%	0.417%
18	23.020	3387	3392	3398	rVB2	45282	83769	1.47%	0.347%
19	23.789	3518	3523	3530	rVB2	42468	90810	1.59%	0.376%
20	24.653	3661	3670	3686	rVB	481304	1396671	24.50%	5.786%


Sum of corrected areas: 24139937

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG090120\
Data File : BG046488.D
Acq On : 1 Sep 2020 17:26
Operator : CG/JU
Sample : L3508-28
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TR-08-082820

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

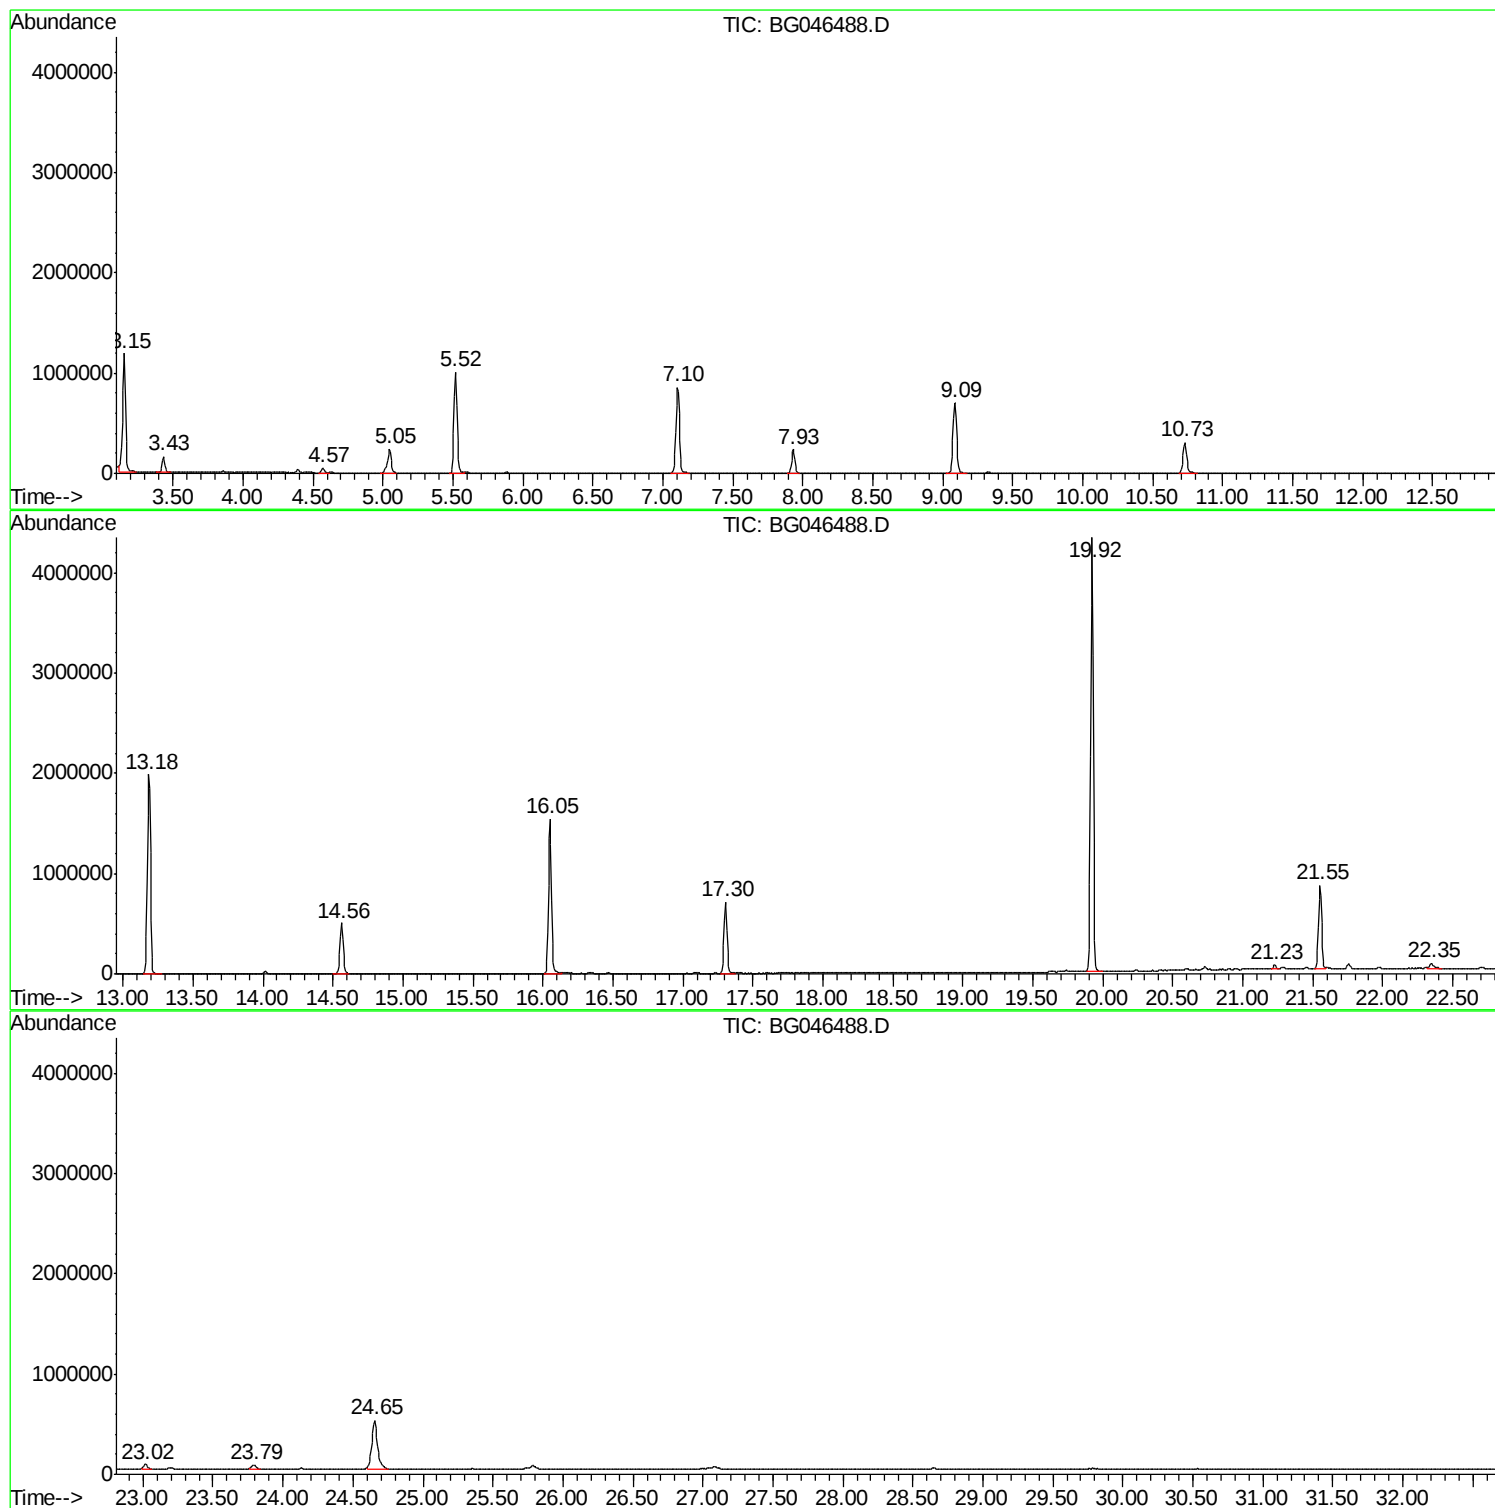

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG090120\
Data File : BG046488.D
Acq On : 1 Sep 2020 17:26
Operator : CG/JU
Sample : L3508-28
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TR-08-082820

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG090120\
Data File : BG046488.D
Acq On : 1 Sep 2020 17:26
Operator : CG/JU
Sample : L3508-28
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TR-08-082820

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc