


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG090120\
 Data File : BG046483.D
 Acq On : 1 Sep 2020 13:37
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 31 16:05:33 2020

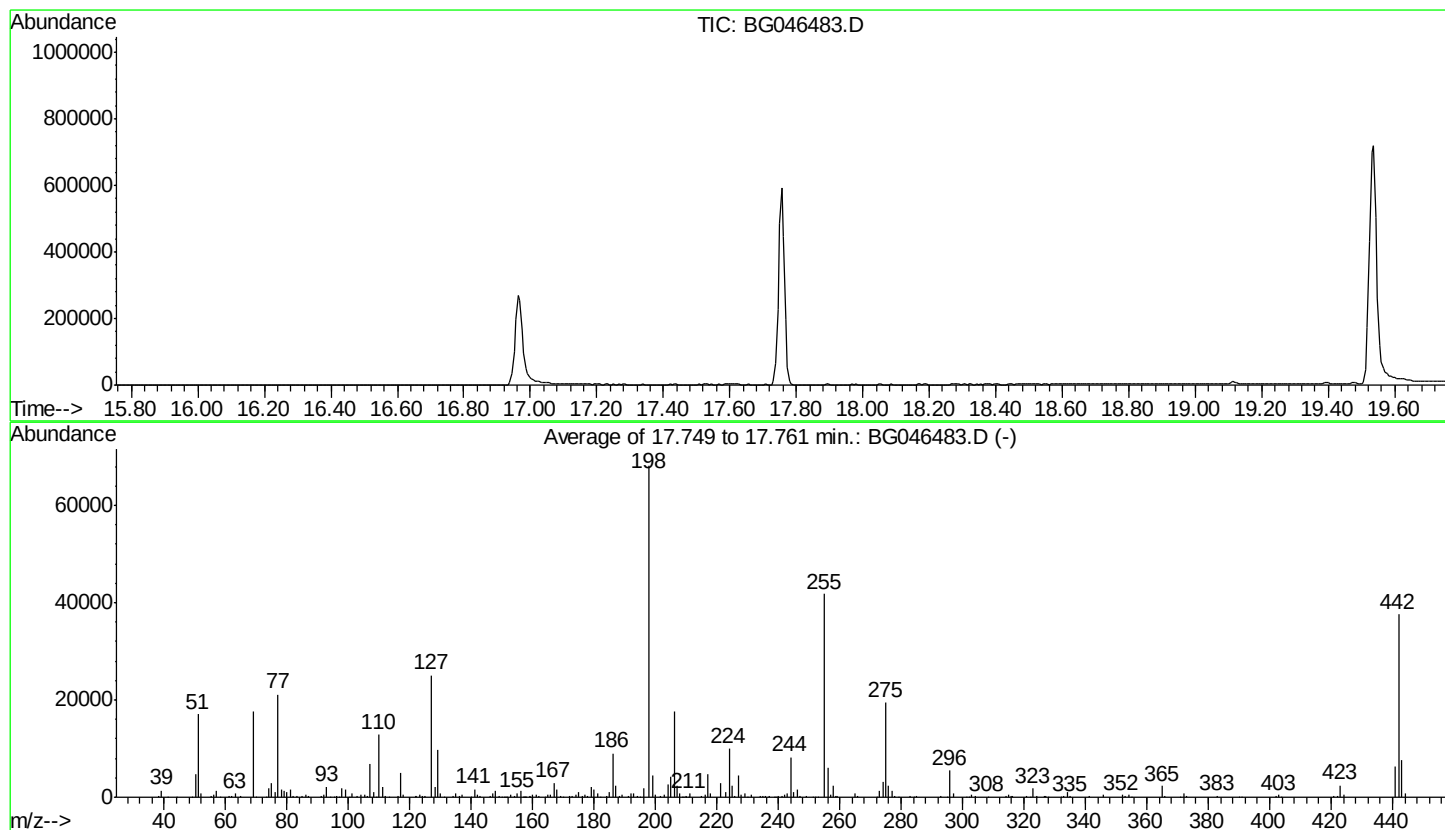

AutoFind: Scans 2495, 2496, 2497; Background Corrected with Scan 2489

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.9	16986	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	25.9	17659	PASS
70	69	0.00	2	0.3	51	PASS
127	198	10	80	36.8	25085	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	68178	PASS
199	198	5	9	6.6	4500	PASS
275	198	10	60	28.5	19416	PASS
365	198	1	100	3.3	2266	PASS
441	198	0.01	100	9.3	6344	PASS
442	198	50	100	55.1	37533	PASS
443	442	15	24	20.1	7550	PASS