
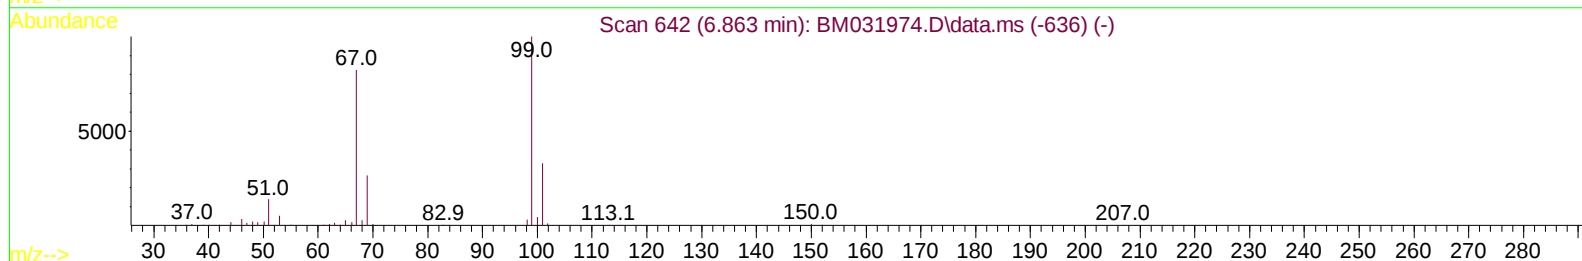
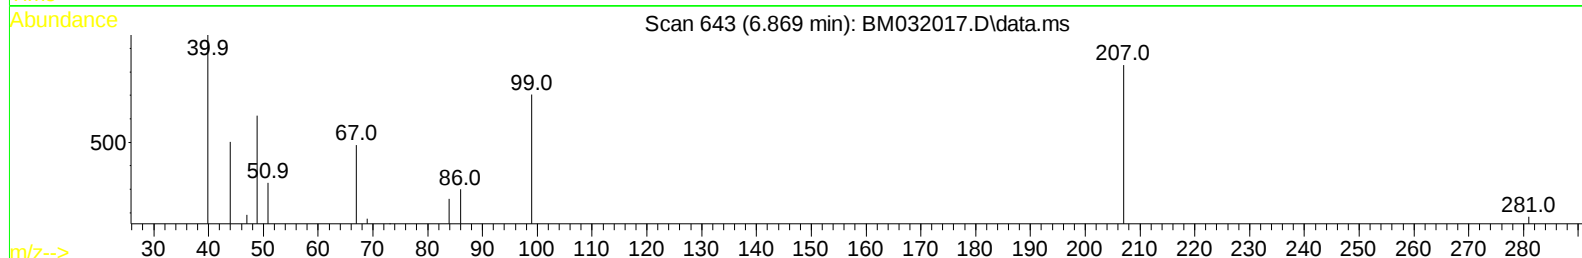


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
Data File : BM032017.D
Acq On : 01 Sep 2021 14:42
Operator : CG/JU
Sample : M3494-02DL2 100X
Misc :
ALS Vial : 32 Sample Multiplier: 1

Quant Time: Sep 01 15:15:53 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 01 11:29:00 2021
Response via : Initial Calibration

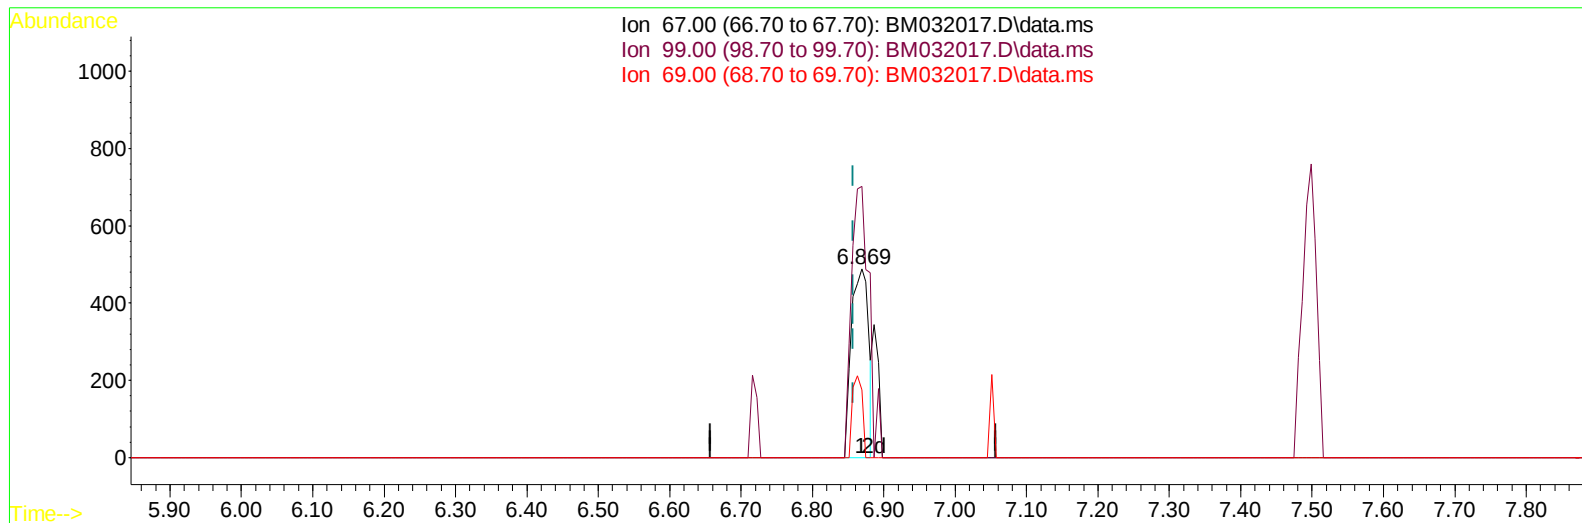

TIC: BM032017.D\data.ms

(9) Bis-(2-Chloroethyl)ether-d8 (S)




6.869min (+ 0.011) 0.35 ng/u1

response 810

Ion	Exp%	Act%
67.00	100.00	100.00
99.00	115.20	143.76#
69.00	30.80	35.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
Data File : BM032017.D
Acq On : 01 Sep 2021 14:42
Operator : CG/JU
Sample : M3494-02DL2 100X
Misc :
ALS Vial : 32 Sample Multiplier: 1

Quant Time: Sep 01 15:15:53 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 01 11:29:00 2021
Response via : Initial Calibration

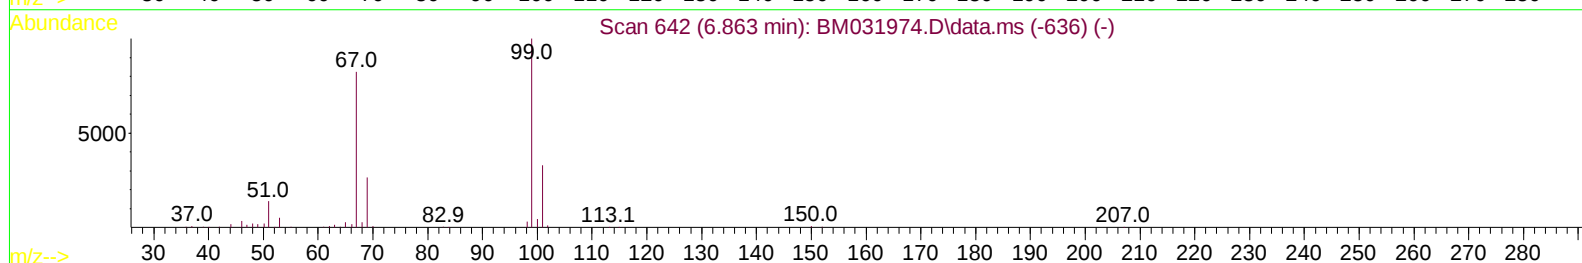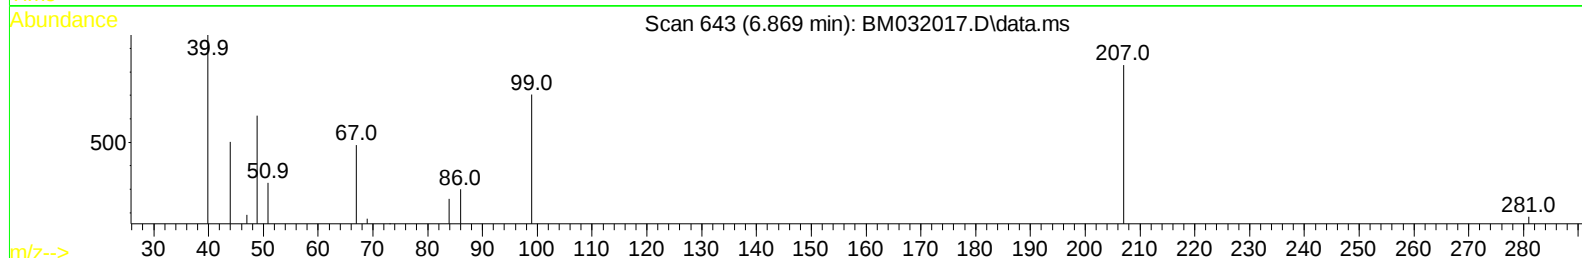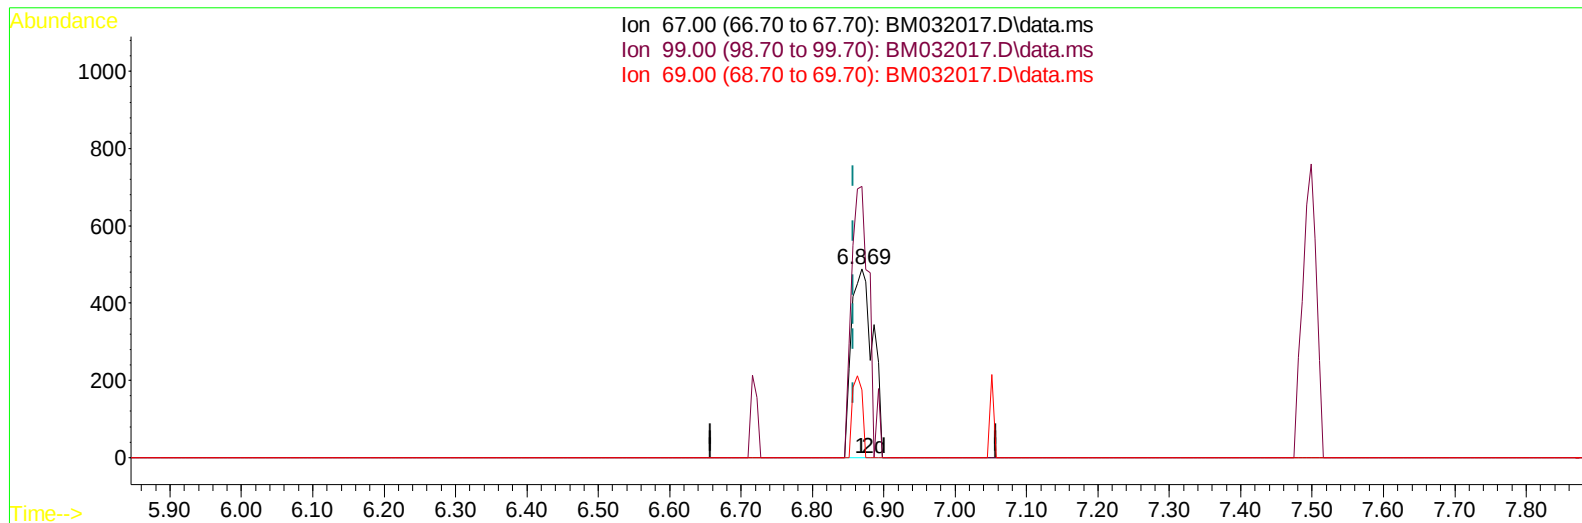

TIC: BM032017.D\data.ms

(9) Bis-(2-Chloroethyl)ether-d8 (S)




6.869min (+ 0.011) 0.44 ng/ul m

response 1019

Ion	Exp%	Act%
67.00	100.00	100.00
99.00	115.20	143.76#
69.00	30.80	35.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083021\
Data File : BM032017.D
Acq On : 01 Sep 2021 14:42
Operator : CG/JU
Sample : M3494-02DL2 100X
Misc :
ALS Vial : 32 Sample Multiplier: 1

Quant Time: Sep 01 15:15:53 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 01 11:29:00 2021
Response via : Initial Calibration

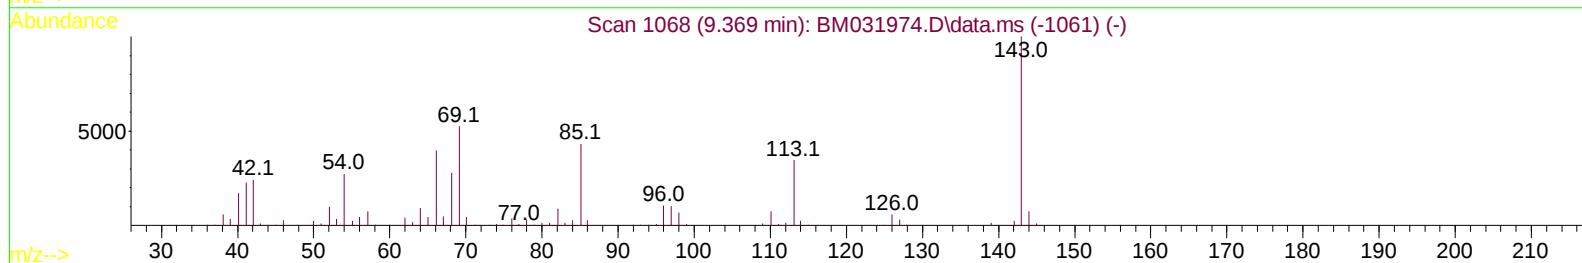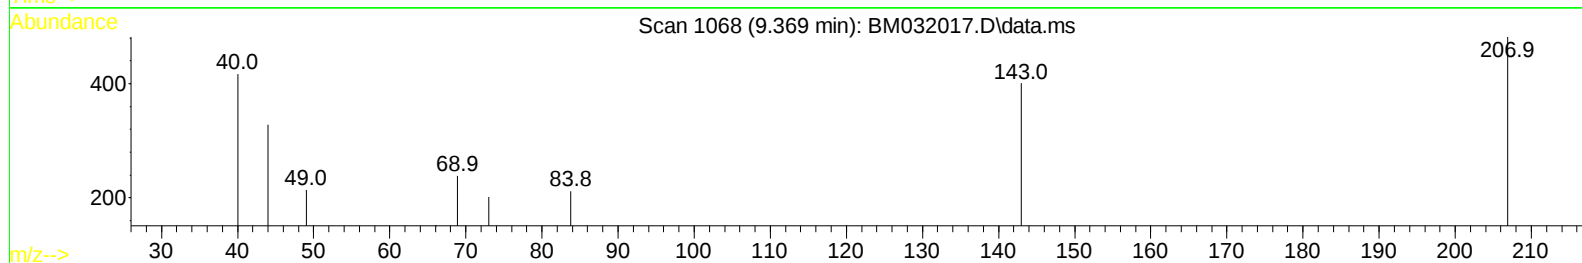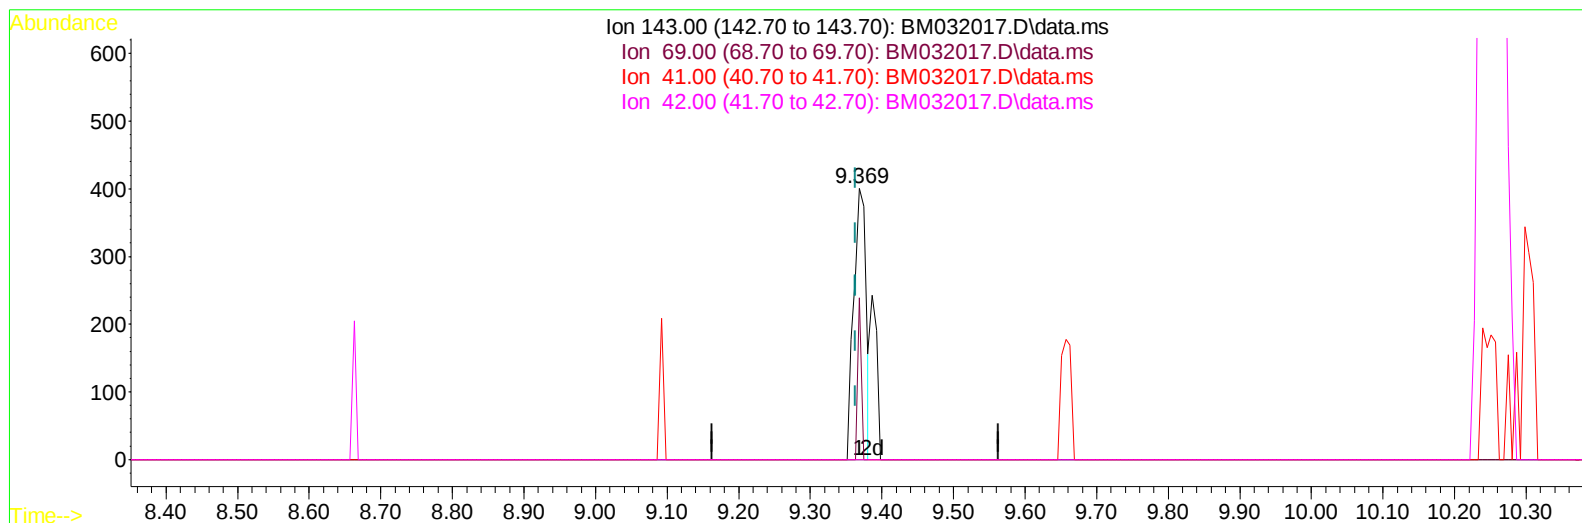

TIC: BM032017.D\data.ms

(24) 2-Nitrophenol-d4 (S)**9.369min (+ 0.006) 0.27 ng/ul****response 488**

Ion	Exp%	Act%
143.00	100.00	100.00
69.00	54.40	59.60
41.00	27.00	0.00#
42.00	27.70	0.00#