

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090221\
 Data File : BG050104.D
 Acq On : 2 Sep 2021 19:50
 Operator : CG/JU
 Sample : M3526-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EW7A9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
 Title : SVOA CALIBRATION

Signal : TIC: BG050104.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.936	489	493	498	rVB3	4085	6425	1.44%	0.195%
2	7.128	691	696	708	rVB2	20885	42803	9.62%	1.301%
3	7.275	716	721	728	rBV2	15994	27708	6.23%	0.842%
4	7.481	752	756	766	rVB3	23022	41308	9.28%	1.256%
5	7.951	830	836	843	rVB	95915	159098	35.75%	4.837%
6	8.491	925	928	929	rBV	1843	1633	0.37%	0.050%
7	8.673	954	959	971	rBV3	24915	49129	11.04%	1.494%
8	9.026	1017	1019	1021	rBV2	1458	1210	0.27%	0.037%
9	9.126	1031	1036	1042	rVB	25156	45933	10.32%	1.396%
10	9.748	1140	1142	1144	rBV	1447	1188	0.27%	0.036%
11	9.854	1154	1160	1168	rBV3	21026	40216	9.04%	1.223%
12	10.160	1208	1212	1220	rBV5	2632	5063	1.14%	0.154%
13	10.406	1248	1254	1260	rBV3	26371	51150	11.49%	1.555%
14	10.535	1274	1276	1281	rBV5	2864	5144	1.16%	0.156%
15	10.770	1307	1316	1323	rBV	128715	236363	53.11%	7.185%
16	10.917	1335	1341	1346	rBV	22125	40164	9.02%	1.221%
17	11.082	1368	1369	1372	rBV2	1196	1181	0.27%	0.036%
18	11.352	1414	1415	1420	rVB	1660	1297	0.29%	0.039%
19	11.563	1449	1451	1454	rBV2	1462	1392	0.31%	0.042%
20	11.687	1469	1472	1473	rBV2	2050	2150	0.48%	0.065%
21	11.775	1485	1487	1488	rBV2	1618	1236	0.28%	0.038%
22	11.951	1515	1517	1520	rBV2	1726	1545	0.35%	0.047%
23	12.174	1553	1555	1559	rVB	1698	1970	0.44%	0.060%
24	12.439	1595	1600	1606	rVB3	4539	7614	1.71%	0.231%
25	12.515	1611	1613	1615	rBV	1235	1321	0.30%	0.040%
26	13.056	1703	1705	1710	rVB2	1188	1245	0.28%	0.038%
27	13.138	1716	1719	1721	rBV2	1632	1865	0.42%	0.057%
28	14.013	1860	1868	1875	rVB	63119	96920	21.78%	2.946%
29	14.078	1877	1879	1884	rVB3	2567	2872	0.65%	0.087%
30	14.307	1912	1918	1928	rVB	72069	113128	25.42%	3.439%
31	14.418	1936	1937	1940	rBV	1316	1122	0.25%	0.034%
32	14.495	1948	1950	1954	rBV3	2204	2154	0.48%	0.065%
33	14.612	1964	1970	1977	rBV	210608	332563	74.72%	10.110%
34	14.871	2009	2014	2018	rBV5	7875	15048	3.38%	0.457%
35	15.012	2035	2038	2042	rVB4	3053	4503	1.01%	0.137%
36	15.282	2078	2084	2085	rBV2	1309	1713	0.38%	0.052%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090221\
 Data File : BG050104.D
 Acq On : 2 Sep 2021 19:50
 Operator : CG/JU
 Sample : M3526-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EW7A9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
 Title : SVOA CALIBRATION

37	15.399	2101	2104	2105	rBV3	1797	1840	0.41%	0.056%
38	15.611	2134	2140	2145	rBV	88626	136282	30.62%	4.143%
39	15.652	2145	2147	2152	rVB4	4085	5369	1.21%	0.163%
40	15.752	2160	2164	2169	rBV4	15807	22040	4.95%	0.670%
41	15.946	2193	2197	2198	rBV2	969	1291	0.29%	0.039%
42	15.958	2198	2199	2203	rVB3	2764	2186	0.49%	0.066%
43	16.104	2220	2224	2228	rBV2	2685	4115	0.92%	0.125%
44	16.198	2237	2240	2245	rVB	1538	2222	0.50%	0.068%
45	16.334	2255	2263	2267	rBV5	8234	15903	3.57%	0.483%
46	16.439	2277	2281	2282	rBV2	2030	2906	0.65%	0.088%
47	16.474	2284	2287	2290	rBV3	2139	2575	0.58%	0.078%
48	16.598	2306	2308	2311	rBV3	1270	1242	0.28%	0.038%
49	17.367	2433	2439	2444	rBV	273043	402332	90.40%	12.231%
50	17.467	2451	2456	2462	rBV	100990	145360	32.66%	4.419%
51	17.696	2493	2495	2496	rBV2	2056	1136	0.26%	0.035%
52	17.773	2504	2508	2510	rBV5	3653	4398	0.99%	0.134%
53	18.143	2569	2571	2573	rBV2	2975	2033	0.46%	0.062%
54	18.249	2586	2589	2593	rVB4	5672	7322	1.65%	0.223%
55	18.301	2594	2598	2600	rBV3	6662	8505	1.91%	0.259%
56	18.431	2618	2620	2622	rBV2	4736	4925	1.11%	0.150%
57	18.742	2671	2673	2674	rBV2	4518	1802	0.40%	0.055%
58	19.423	2786	2789	2793	rVB	36633	46423	10.43%	1.411%
59	19.758	2841	2846	2856	rBV2	141192	245858	55.24%	7.474%
60	21.638	3161	3166	3173	rBV2	263329	428963	96.38%	13.041%
61	24.857	3707	3714	3723	rVB2	161074	445065	100.00%	13.530%




Sum of corrected areas: 3289467

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090221\
Data File : BG050104.D
Acq On : 2 Sep 2021 19:50
Operator : CG/JU
Sample : M3526-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW7A9

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

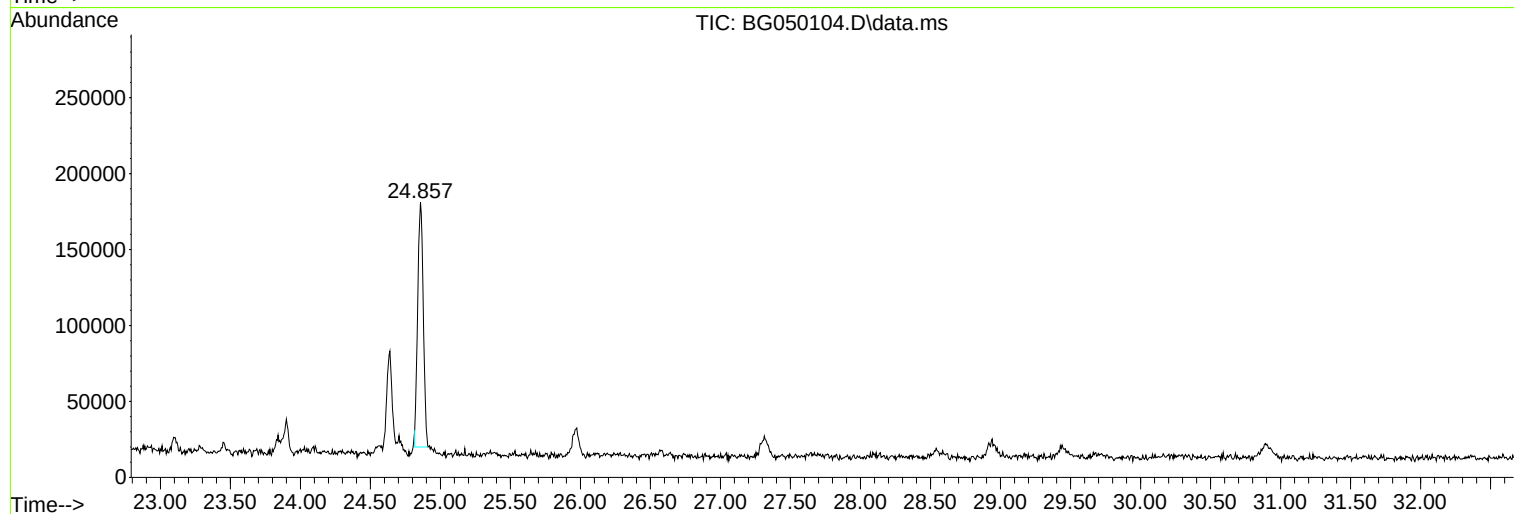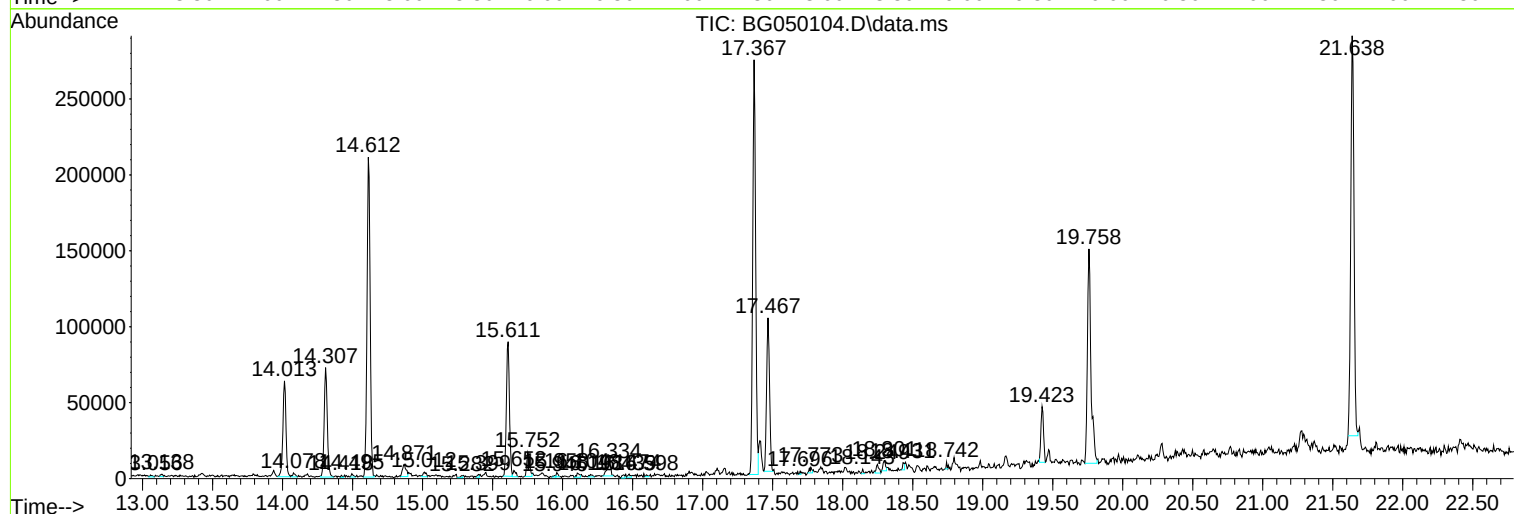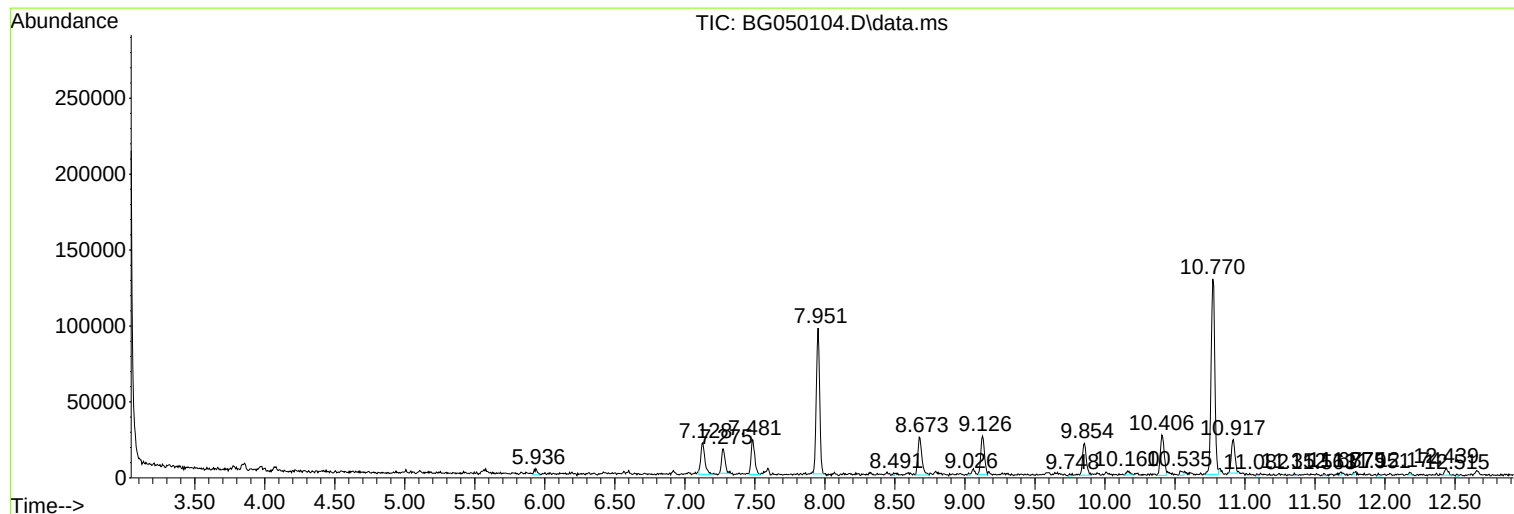

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090221\
Data File : BG050104.D
Acq On : 2 Sep 2021 19:50
Operator : CG/JU
Sample : M3526-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW7A9

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090221\
Data File : BG050104.D
Acq On : 2 Sep 2021 19:50
Operator : CG/JU
Sample : M3526-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW7A9

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
