

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090221\
 Data File : BG050110.D
 Acq On : 2 Sep 2021 23:56
 Operator : CG/JU
 Sample : M3526-15
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EW7C5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
 Title : SVOA CALIBRATION

Signal : TIC: BG050110.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.760	121	123	127	rBV4	5180	6119	1.60%	0.165%
2	3.965	156	158	160	rBV2	2867	2137	0.56%	0.058%
3	5.557	426	429	434	rVB5	3693	4324	1.13%	0.117%
4	5.933	489	493	498	rBV4	6188	9215	2.41%	0.249%
5	6.280	550	552	555	rVB3	1387	1203	0.31%	0.033%
6	7.020	675	678	683	rBV4	2664	4623	1.21%	0.125%
7	7.126	691	696	709	rVB2	42994	79302	20.76%	2.142%
8	7.273	715	721	729	rBV2	35471	62807	16.45%	1.697%
9	7.490	751	758	764	rVB2	43413	79709	20.87%	2.153%
10	7.560	766	770	771	rBV2	2809	2571	0.67%	0.069%
11	7.948	830	836	846	rVB	95837	165611	43.36%	4.474%
12	8.060	854	855	860	rVB2	2795	2965	0.78%	0.080%
13	8.201	876	879	883	rBV	1443	2004	0.52%	0.054%
14	8.395	911	912	915	rBV2	1651	1618	0.42%	0.044%
15	8.677	953	960	972	rBV2	39421	72988	19.11%	1.972%
16	8.771	975	976	978	rBV2	1752	1661	0.43%	0.045%
17	8.964	1007	1009	1013	rVB3	1686	1620	0.42%	0.044%
18	9.123	1029	1036	1043	rBV2	47818	89792	23.51%	2.426%
19	9.640	1121	1124	1126	rBV2	1214	1318	0.35%	0.036%
20	9.769	1143	1146	1150	rBV	1657	2086	0.55%	0.056%
21	9.851	1154	1160	1169	rVB2	40704	76541	20.04%	2.068%
22	10.410	1248	1255	1263	rBV	53091	99202	25.98%	2.680%
23	10.545	1275	1278	1283	rBV3	3506	4220	1.10%	0.114%
24	10.621	1289	1291	1295	rVB2	1105	1219	0.32%	0.033%
25	10.774	1306	1317	1323	rBV	130943	234901	61.51%	6.346%
26	10.915	1334	1341	1350	rBV2	38213	74696	19.56%	2.018%
27	11.790	1486	1490	1494	rVB3	3642	4453	1.17%	0.120%
28	12.184	1553	1557	1563	rVB4	4996	7207	1.89%	0.195%
29	12.366	1585	1588	1590	rBV2	1243	1195	0.31%	0.032%
30	12.436	1596	1600	1608	rVB3	17795	30192	7.91%	0.816%
31	12.659	1632	1638	1643	rBV	15761	24441	6.40%	0.660%
32	12.812	1662	1664	1668	rBV2	987	1305	0.34%	0.035%
33	12.894	1675	1678	1679	rBV	1316	1229	0.32%	0.033%
34	13.135	1714	1719	1723	rVB5	2862	4658	1.22%	0.126%
35	13.423	1763	1768	1775	rBV3	6830	11423	2.99%	0.309%
36	13.640	1802	1805	1807	rBV4	1481	2161	0.57%	0.058%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090221\
 Data File : BG050110.D
 Acq On : 2 Sep 2021 23:56
 Operator : CG/JU
 Sample : M3526-15
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EW7C5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
 Title : SVOA CALIBRATION

37	13.770	1823	1827	1829	rBV2	4149	5840	1.53%	0.158%
38	13.881	1844	1846	1849	rVB2	1827	1696	0.44%	0.046%
39	13.934	1849	1855	1860	rBV3	11691	19648	5.14%	0.531%
40	14.011	1860	1868	1875	rVB	109153	179235	46.93%	4.842%
41	14.075	1876	1879	1884	rVB2	5048	7598	1.99%	0.205%
42	14.116	1884	1886	1889	rBV2	1362	1307	0.34%	0.035%
43	14.175	1891	1896	1899	rBV2	6944	10117	2.65%	0.273%
44	14.310	1912	1919	1929	rBV	121251	203076	53.17%	5.486%
45	14.498	1945	1951	1956	rVB2	6192	9425	2.47%	0.255%
46	14.616	1962	1971	1977	rBV	206784	323509	84.71%	8.740%
47	14.815	2000	2005	2007	rBV2	1671	2850	0.75%	0.077%
48	14.856	2007	2012	2016	rBV5	21452	38719	10.14%	1.046%
49	15.015	2034	2039	2045	rVB3	9169	18396	4.82%	0.497%
50	15.091	2045	2052	2056	rBV5	4047	8412	2.20%	0.227%
51	15.144	2059	2061	2063	rBV	1711	1614	0.42%	0.044%
52	15.232	2073	2076	2082	rVB5	4813	6506	1.70%	0.176%
53	15.285	2082	2085	2089	rBV3	5737	6380	1.67%	0.172%
54	15.403	2098	2105	2109	rBV5	5747	12047	3.15%	0.325%
55	15.444	2109	2112	2118	rVB5	7925	12132	3.18%	0.328%
56	15.608	2134	2140	2145	rBV	159870	238284	62.39%	6.437%
57	15.650	2145	2147	2154	rVB4	11590	17386	4.55%	0.470%
58	15.749	2160	2164	2171	rBV2	34093	55496	14.53%	1.499%
59	15.855	2179	2182	2185	rBV3	3469	5038	1.32%	0.136%
60	15.955	2191	2199	2205	rBV5	7029	13247	3.47%	0.358%
61	16.020	2205	2210	2211	rBV2	1894	2641	0.69%	0.071%
62	16.073	2214	2219	2220	rBV3	2085	3041	0.80%	0.082%
63	16.108	2222	2225	2226	rBV2	3903	4338	1.14%	0.117%
64	16.225	2243	2245	2248	rVB	1415	1214	0.32%	0.033%
65	16.255	2248	2250	2253	rBV2	1917	1770	0.46%	0.048%
66	16.307	2256	2259	2260	rBV	7428	5777	1.51%	0.156%
67	16.519	2293	2295	2299	rVB3	2000	2410	0.63%	0.065%
68	16.619	2308	2312	2313	rBV2	1535	1625	0.43%	0.044%
69	16.654	2316	2318	2319	rBV2	2099	2047	0.54%	0.055%
70	16.819	2344	2346	2349	rVB2	3230	3199	0.84%	0.086%
71	16.907	2357	2361	2363	rBV4	7172	10642	2.79%	0.288%
72	17.024	2377	2381	2386	rVB6	5884	10104	2.65%	0.273%
73	17.059	2386	2387	2388	rBV	3376	1851	0.48%	0.050%
74	17.106	2391	2395	2399	rVB4	9487	14571	3.82%	0.394%
75	17.371	2433	2440	2444	rBV	246255	381905	100.00%	10.318%
76	17.412	2444	2447	2451	rVB	48724	63260	16.56%	1.709%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090221\
 Data File : BG050110.D
 Acq On : 2 Sep 2021 23:56
 Operator : CG/JU
 Sample : M3526-15
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EW7C5

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
 Title : SVOA CALIBRATION

77	17.471	2451	2457	2462	rBV	161564	250687	65.64%	6.773%
78	17.547	2468	2470	2474	rBV5	3490	4208	1.10%	0.114%
79	18.087	2560	2562	2566	rBV4	4036	5847	1.53%	0.158%
80	18.293	2595	2597	2601	rVB2	18942	19515	5.11%	0.527%
81	18.434	2617	2621	2625	rBV4	17026	32914	8.62%	0.889%
82	19.427	2785	2790	2796	rVB	126923	185148	48.48%	5.002%
83	19.762	2842	2847	2850	rBV	206025	322137	84.35%	8.703%




Sum of corrected areas: 3701525

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090221\
Data File : BG050110.D
Acq On : 2 Sep 2021 23:56
Operator : CG/JU
Sample : M3526-15
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW7C5

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

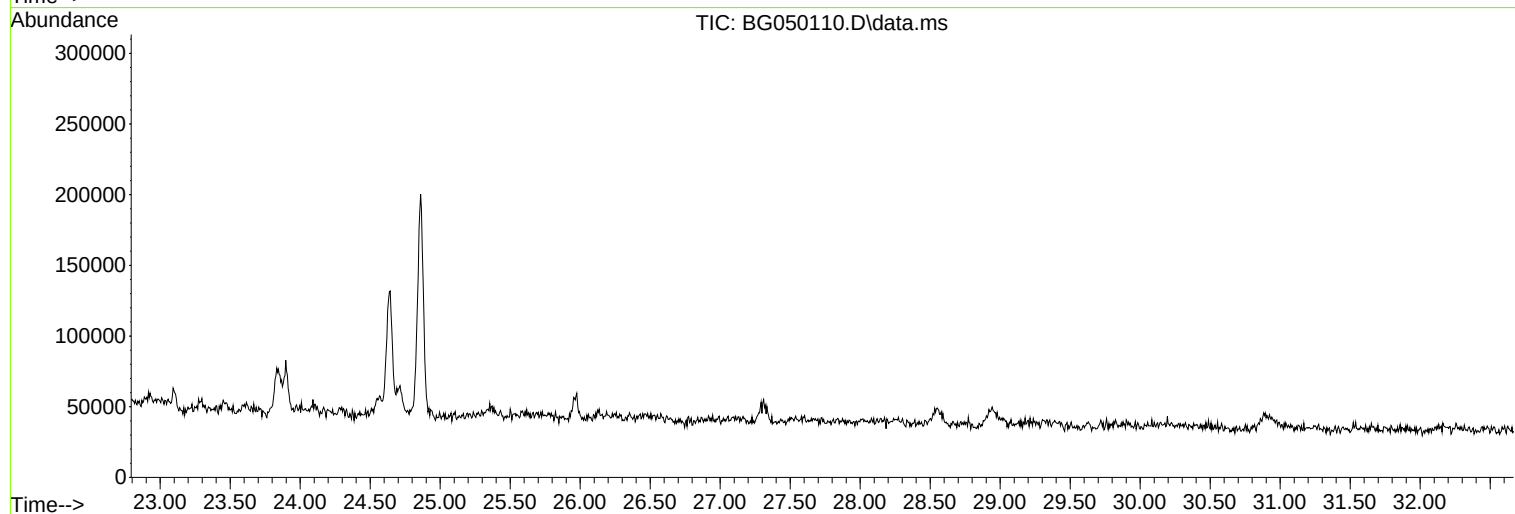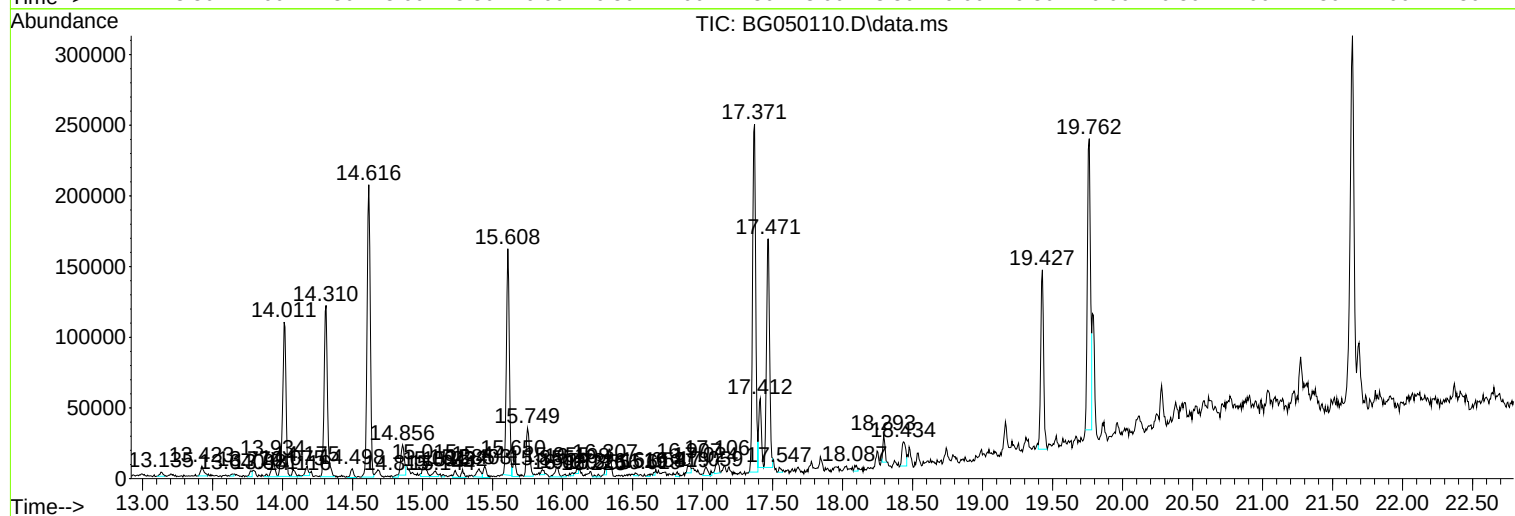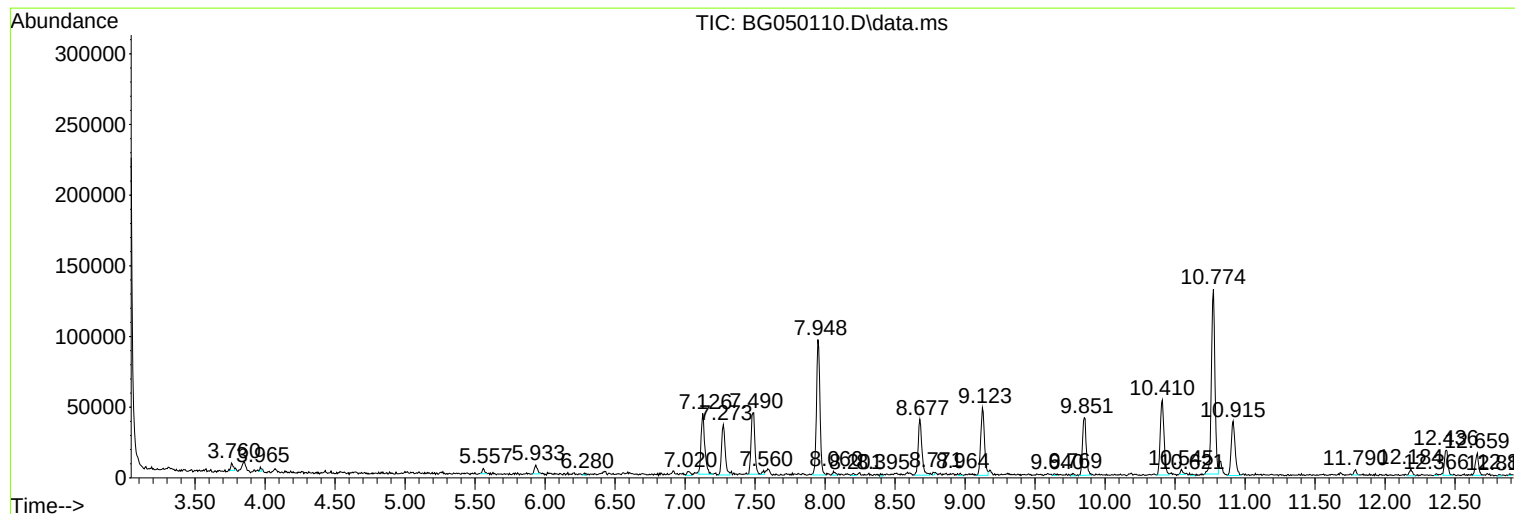

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090221\
Data File : BG050110.D
Acq On : 2 Sep 2021 23:56
Operator : CG/JU
Sample : M3526-15
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW7C5

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090221\
Data File : BG050110.D
Acq On : 2 Sep 2021 23:56
Operator : CG/JU
Sample : M3526-15
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW7C5

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
