

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090221\
 Data File : BG050124.D
 Acq On : 3 Sep 2021 10:07
 Operator : CG/JU
 Sample : M3553-03 10X
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AH6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
 Title : SVOA CALIBRATION

Signal : TIC: BG050124.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.150	17	19	22	rVB2	1751	1423	0.16%	0.019%
2	3.302	44	45	48	rBV3	2487	1666	0.19%	0.022%
3	3.743	117	120	131	rBV	19725	42454	4.91%	0.554%
4	4.060	172	174	177	rBV3	1964	2470	0.29%	0.032%
5	4.295	212	214	217	rBV3	1170	1269	0.15%	0.017%
6	4.325	217	219	222	rVV3	1402	1626	0.19%	0.021%
7	4.401	229	232	233	rBV2	1767	1852	0.21%	0.024%
8	5.476	413	415	418	rVB3	1627	1545	0.18%	0.020%
9	5.623	437	440	442	rBV2	960	1318	0.15%	0.017%
10	6.710	623	625	627	rBV2	1288	1473	0.17%	0.019%
11	7.127	690	696	702	rBV2	22986	43048	4.98%	0.562%
12	7.268	714	720	731	rBV	81520	144068	16.66%	1.880%
13	7.338	731	732	737	rVB3	1827	1774	0.21%	0.023%
14	7.479	750	756	765	rBV2	86104	157179	18.17%	2.051%
15	7.591	773	775	780	rVB2	1616	1738	0.20%	0.023%
16	7.691	789	792	794	rBV2	932	1239	0.14%	0.016%
17	7.949	829	836	843	rBV	94530	160253	18.53%	2.091%
18	8.008	843	846	851	rVB3	6420	9011	1.04%	0.118%
19	8.443	917	920	923	rBV	1458	1864	0.22%	0.024%
20	8.625	948	951	953	rBV2	1091	1579	0.18%	0.021%
21	8.672	953	959	972	rVV2	70883	132869	15.36%	1.734%
22	8.795	975	980	982	rVV4	2077	3920	0.45%	0.051%
23	8.842	985	988	990	rBV2	873	1284	0.15%	0.017%
24	9.124	1029	1036	1045	rVB	116818	212746	24.60%	2.776%
25	9.706	1134	1135	1139	rBV	1455	1325	0.15%	0.017%
26	9.852	1153	1160	1166	rBV	102771	184217	21.30%	2.404%
27	9.917	1170	1171	1174	rVB	1581	1255	0.15%	0.016%
28	10.399	1247	1253	1264	rBV	130570	236530	27.35%	3.087%
29	10.534	1272	1276	1281	rBV4	4527	8887	1.03%	0.116%
30	10.716	1304	1307	1308	rVB2	1381	1224	0.14%	0.016%
31	10.769	1308	1316	1323	rBV	129527	227826	26.34%	2.973%
32	10.910	1333	1340	1350	rBV	127311	237518	27.46%	3.099%
33	11.374	1415	1419	1421	rVB2	1530	1988	0.23%	0.026%
34	12.161	1551	1553	1557	rBV	1291	1224	0.14%	0.016%
35	12.361	1584	1587	1593	rBV3	2535	3799	0.44%	0.050%
36	14.011	1862	1868	1876	rBV	280867	415595	48.05%	5.423%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090221\
 Data File : BG050124.D
 Acq On : 3 Sep 2021 10:07
 Operator : CG/JU
 Sample : M3553-03 10X
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AH6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
 Title : SVOA CALIBRATION

37	14.305	1910	1918	1927	rBV	310596	486756	56.28%	6.352%
38	14.616	1964	1971	1978	rVB	201373	314796	36.40%	4.108%
39	14.857	2007	2012	2018	rBV3	14930	25408	2.94%	0.332%
40	15.609	2131	2140	2148	rBV	419085	611251	70.67%	7.976%
41	15.744	2158	2163	2173	rBV	119787	194680	22.51%	2.540%
42	15.850	2180	2181	2187	rVB3	4041	2636	0.30%	0.034%
43	17.154	2401	2403	2408	rVB2	1344	1904	0.22%	0.025%
44	17.366	2432	2439	2446	rBV	255939	384927	44.50%	5.023%
45	17.466	2450	2456	2467	rVB	472524	719041	83.13%	9.383%
46	18.024	2546	2551	2555	rVB2	2826	3938	0.46%	0.051%
47	18.071	2555	2559	2564	rVV	1299	1512	0.17%	0.020%
48	18.118	2564	2567	2571	rVB2	1017	1272	0.15%	0.017%
49	18.200	2579	2581	2585	rBV	759	1183	0.14%	0.015%
50	18.323	2597	2602	2604	rBV2	2316	2830	0.33%	0.037%
51	19.011	2717	2719	2722	rBV	921	1179	0.14%	0.015%
52	19.216	2751	2754	2757	rBV4	1249	1943	0.22%	0.025%
53	19.246	2757	2759	2763	rVB2	1138	1288	0.15%	0.017%
54	19.322	2768	2772	2778	rVB4	4763	7263	0.84%	0.095%
55	19.398	2781	2785	2788	rBV3	6038	7415	0.86%	0.097%
56	19.475	2795	2798	2800	rBV2	1120	1565	0.18%	0.020%
57	19.522	2803	2806	2808	rVV	2068	2421	0.28%	0.032%
58	19.545	2808	2810	2813	rVB4	1941	2195	0.25%	0.029%
59	19.580	2813	2816	2820	rBV4	1979	2439	0.28%	0.032%
60	19.657	2827	2829	2832	rVB2	2229	2384	0.28%	0.031%
61	19.757	2840	2846	2855	rBV	609371	864925	100.00%	11.287%
62	19.868	2861	2865	2866	rBV	1819	1917	0.22%	0.025%
63	20.162	2913	2915	2919	rVB4	1347	1483	0.17%	0.019%
64	20.209	2920	2923	2924	rVB2	1392	1163	0.13%	0.015%
65	20.221	2924	2925	2928	rVB2	2234	1422	0.16%	0.019%
66	20.250	2928	2930	2931	rBV2	1418	1173	0.14%	0.015%
67	20.279	2931	2935	2937	rVB3	2701	2951	0.34%	0.039%
68	20.473	2967	2968	2970	rBV	2374	1646	0.19%	0.021%
69	20.567	2982	2984	2987	rVB3	1816	1473	0.17%	0.019%
70	20.597	2987	2989	2990	rBV2	2259	1973	0.23%	0.026%
71	20.661	2998	3000	3002	rBV3	3854	3098	0.36%	0.040%
72	20.767	3015	3018	3022	rBV6	5431	6534	0.76%	0.085%
73	20.820	3025	3027	3033	rBV4	2585	4730	0.55%	0.062%
74	20.996	3055	3057	3060	rBV3	2739	3433	0.40%	0.045%
75	21.067	3067	3069	3071	rBV3	2899	2627	0.30%	0.034%
76	21.572	3153	3155	3156	rBV2	3371	2139	0.25%	0.028%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090221\
 Data File : BG050124.D
 Acq On : 3 Sep 2021 10:07
 Operator : CG/JU
 Sample : M3553-03 10X
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AH6

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
 Title : SVOA CALIBRATION

77	21.642	3160	3167	3173	rVV	259156	429146	49.62%	5.600%
78	21.807	3192	3195	3200	rVB6	5951	8951	1.03%	0.117%
79	24.638	3667	3677	3688	rVB	300813	813418	94.04%	10.614%
80	24.856	3704	3714	3726	rVB2	163676	464029	53.65%	6.055%
81	26.418	3978	3980	3982	rVB3	4436	1891	0.22%	0.025%
82	26.583	4006	4008	4010	rBV3	3640	2038	0.24%	0.027%
83	27.411	4148	4149	4151	rBV2	3786	2699	0.31%	0.035%
84	30.554	4682	4684	4685	rBV2	4861	3089	0.36%	0.040%
85	32.463	5007	5009	5010	rBV2	3665	2082	0.24%	0.027%




Sum of corrected areas: 7663312

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090221\
Data File : BG050124.D
Acq On : 3 Sep 2021 10:07
Operator : CG/JU
Sample : M3553-03 10X
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AH6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

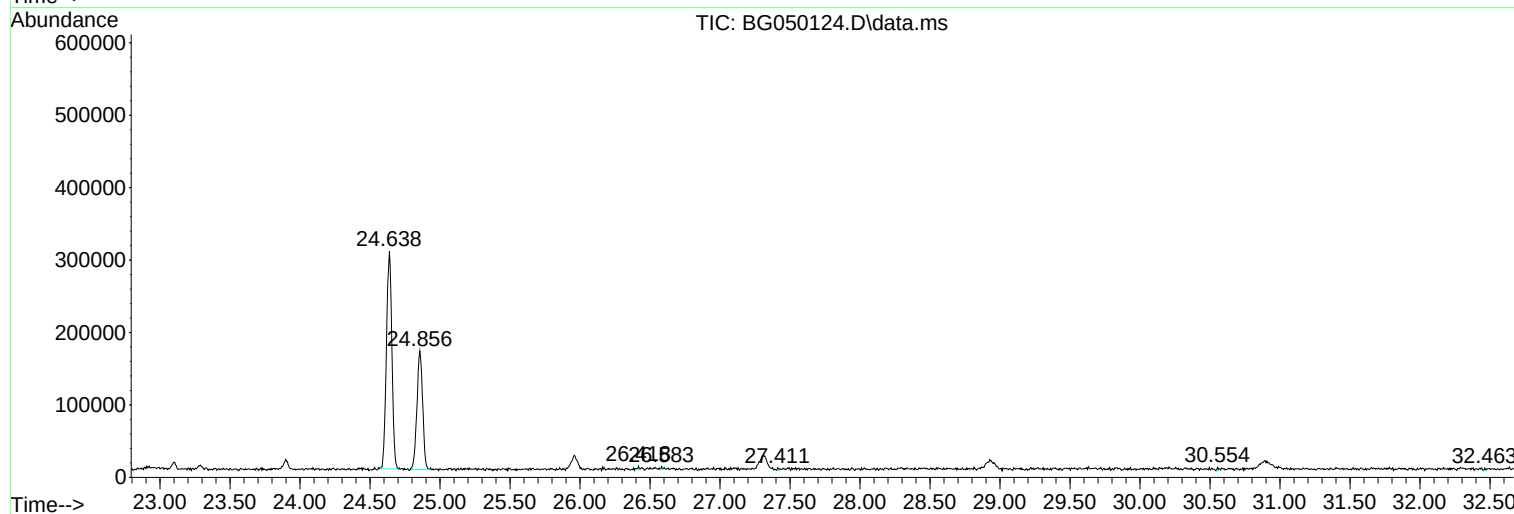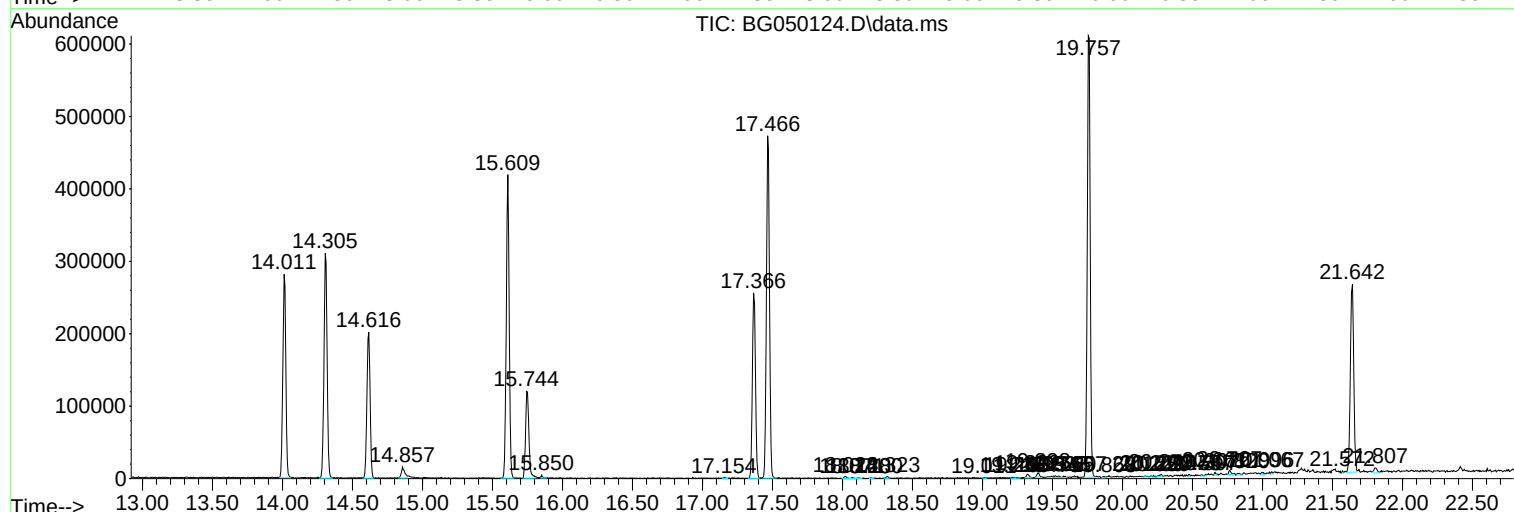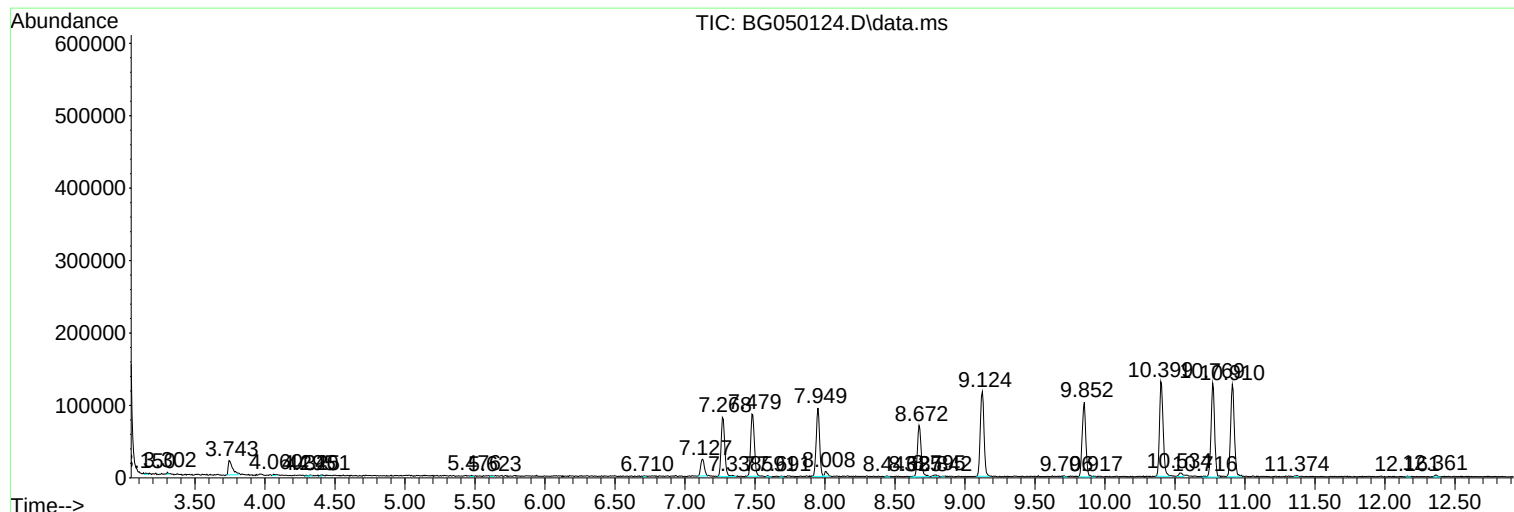

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090221\
Data File : BG050124.D
Acq On : 3 Sep 2021 10:07
Operator : CG/JU
Sample : M3553-03 10X
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AH6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090221\
Data File : BG050124.D
Acq On : 3 Sep 2021 10:07
Operator : CG/JU
Sample : M3553-03 10X
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AH6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
