

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090221\
 Data File : BG050131.D
 Acq On : 3 Sep 2021 14:51
 Operator : CG/JU
 Sample : PB138772BL
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK772

Integration Parameters: LSCINT.P

Integrator: RTE

Soothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
 Title : SVOA CALIBRATION

Signal : TIC: BG050131.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.310	42	46	53	rVB2	7230	11850	1.32%	0.130%
2	3.733	115	118	132	rBV	85407	166818	18.60%	1.828%
3	3.985	159	161	164	rBV3	1645	2010	0.22%	0.022%
4	4.062	172	174	175	rBV2	2860	2242	0.25%	0.025%
5	6.012	504	506	508	rBV2	1536	1313	0.15%	0.014%
6	7.122	688	695	709	rBV	146372	262844	29.30%	2.880%
7	7.275	714	721	730	rVV	100847	174623	19.47%	1.914%
8	7.480	750	756	764	rBV	148315	252979	28.20%	2.772%
9	7.950	829	836	843	rBV	92825	160232	17.86%	1.756%
10	8.180	873	875	876	rBV	1653	1323	0.15%	0.014%
11	8.555	935	939	942	rBV3	1170	1862	0.21%	0.020%
12	8.591	944	945	949	rVB3	1480	1370	0.15%	0.015%
13	8.673	951	959	972	rBV	183968	330682	36.87%	3.624%
14	8.849	984	989	991	rVB2	1508	2282	0.25%	0.025%
15	9.125	1029	1036	1044	rVB	140955	254273	28.35%	2.787%
16	9.384	1078	1080	1084	rBV3	1273	1839	0.21%	0.020%
17	9.848	1153	1159	1169	rBV	132472	237075	26.43%	2.598%
18	10.400	1247	1253	1268	rBV	178964	327049	36.46%	3.584%
19	10.659	1295	1297	1300	rBV2	1140	1340	0.15%	0.015%
20	10.770	1309	1316	1323	rBV	129013	229232	25.56%	2.512%
21	10.911	1332	1340	1350	rBV	171878	320274	35.71%	3.510%
22	11.810	1490	1493	1496	rBV	1020	1194	0.13%	0.013%
23	12.938	1683	1685	1688	rBV	1200	1295	0.14%	0.014%
24	13.502	1775	1781	1782	rVB2	971	1373	0.15%	0.015%
25	14.013	1862	1868	1875	rBV	341931	494190	55.10%	5.416%
26	14.248	1906	1908	1911	rBV2	875	1199	0.13%	0.013%
27	14.307	1911	1918	1928	rVV	371431	580995	64.77%	6.367%
28	14.371	1928	1929	1934	rVB	1463	1553	0.17%	0.017%
29	14.612	1964	1970	1979	rVB	203863	317760	35.43%	3.482%
30	14.841	2004	2009	2026	rBV4	96058	201515	22.47%	2.208%
31	15.611	2133	2140	2150	rBV	447288	699589	77.99%	7.667%
32	15.746	2158	2163	2175	rBV	123257	207858	23.17%	2.278%
33	15.851	2177	2181	2184	rBV2	2476	3524	0.39%	0.039%
34	16.022	2207	2210	2214	rBV	977	1209	0.13%	0.013%
35	17.367	2433	2439	2448	rVB	253993	382932	42.69%	4.196%
36	17.467	2448	2456	2463	rBV	529168	773803	86.27%	8.480%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090221\
 Data File : BG050131.D
 Acq On : 3 Sep 2021 14:51
 Operator : CG/JU
 Sample : PB138772BL
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK772

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
 Title : SVOA CALIBRATION

37	17.790	2507	2511	2513	rBV2	1008	1262	0.14%	0.014%
38	18.313	2598	2600	2606	rBV2	1552	2034	0.23%	0.022%
39	18.753	2671	2675	2678	rVB	1271	1333	0.15%	0.015%
40	19.006	2715	2718	2719	rBV	1292	1425	0.16%	0.016%
41	19.188	2747	2749	2752	rBV	1244	1554	0.17%	0.017%
42	19.229	2753	2756	2757	rVB2	2282	1533	0.17%	0.017%
43	19.247	2757	2759	2761	rBV2	2263	2098	0.23%	0.023%
44	19.288	2764	2766	2767	rBV2	2888	1921	0.21%	0.021%
45	19.323	2767	2772	2778	rBV5	6858	11748	1.31%	0.129%
46	19.394	2780	2784	2789	rBV5	8335	12330	1.37%	0.135%
47	19.435	2789	2791	2792	rBV	3080	1713	0.19%	0.019%
48	19.664	2829	2830	2834	rVB2	2256	1527	0.17%	0.017%
49	19.764	2840	2847	2853	rBV	619511	896969	100.00%	9.830%
50	19.881	2863	2867	2868	rBV	1605	1902	0.21%	0.021%
51	19.911	2871	2872	2876	rBV2	1650	2531	0.28%	0.028%
52	20.028	2891	2892	2895	rVB3	2388	1663	0.19%	0.018%
53	20.069	2895	2899	2900	rBV3	1935	2291	0.26%	0.025%
54	20.122	2906	2908	2910	rVB2	2489	1201	0.13%	0.013%
55	20.146	2910	2912	2915	rVB4	1731	1258	0.14%	0.014%
56	20.281	2933	2935	2936	rBV2	2275	1692	0.19%	0.019%
57	20.316	2940	2941	2945	rVB4	2412	1891	0.21%	0.021%
58	20.357	2945	2948	2949	rBV	2450	2093	0.23%	0.023%
59	20.651	2994	2998	2999	rBV4	3871	3160	0.35%	0.035%
60	21.097	3073	3074	3075	rVB	3734	1316	0.15%	0.014%
61	21.321	3110	3112	3113	rBV2	3086	1876	0.21%	0.021%
62	21.644	3161	3167	3174	rVB	258314	420179	46.84%	4.605%
63	21.973	3221	3223	3225	rBV3	3585	2966	0.33%	0.033%
64	24.205	3601	3603	3605	rBV3	3282	1942	0.22%	0.021%
65	24.299	3617	3619	3620	rBV2	4120	2499	0.28%	0.027%
66	24.640	3666	3677	3687	rBV2	319558	878545	97.95%	9.628%
67	24.857	3705	3714	3725	rVB2	147576	432800	48.25%	4.743%
68	27.007	4078	4080	4081	rBV2	3939	2012	0.22%	0.022%
69	28.517	4335	4337	4340	rBV4	3857	3834	0.43%	0.042%
70	29.627	4524	4526	4528	rBV3	3754	3232	0.36%	0.035%
71	31.724	4881	4883	4885	rBV3	3963	3241	0.36%	0.036%




Sum of corrected areas: 9125072

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090221\
Data File : BG050131.D
Acq On : 3 Sep 2021 14:51
Operator : CG/JU
Sample : PB138772BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK772

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

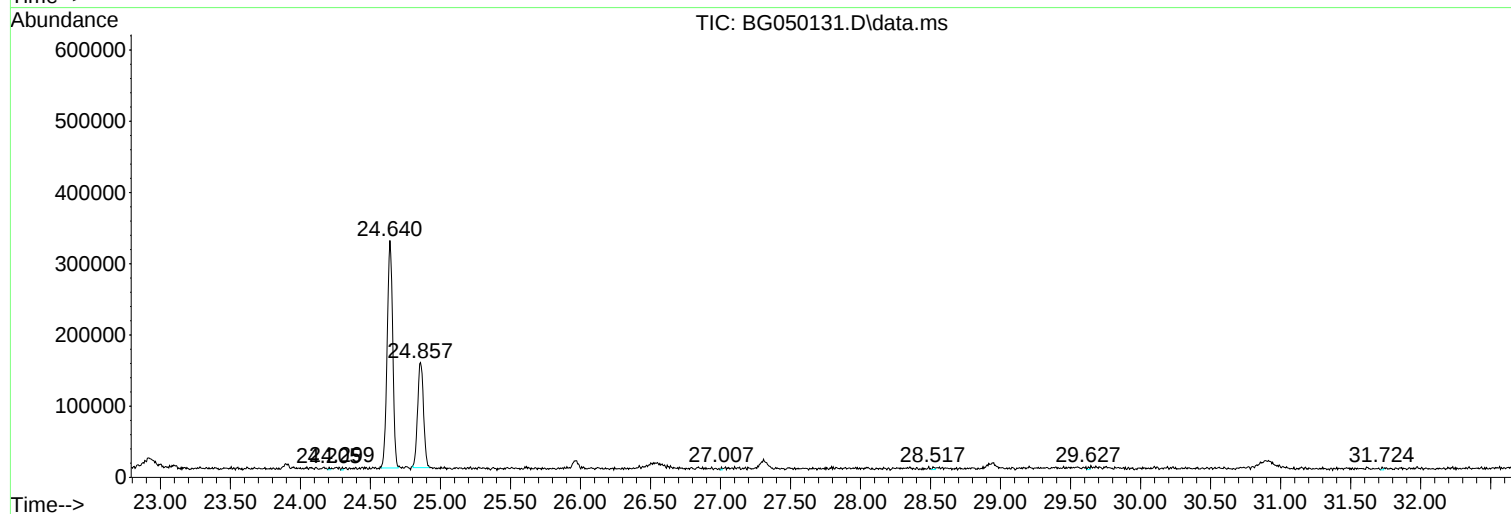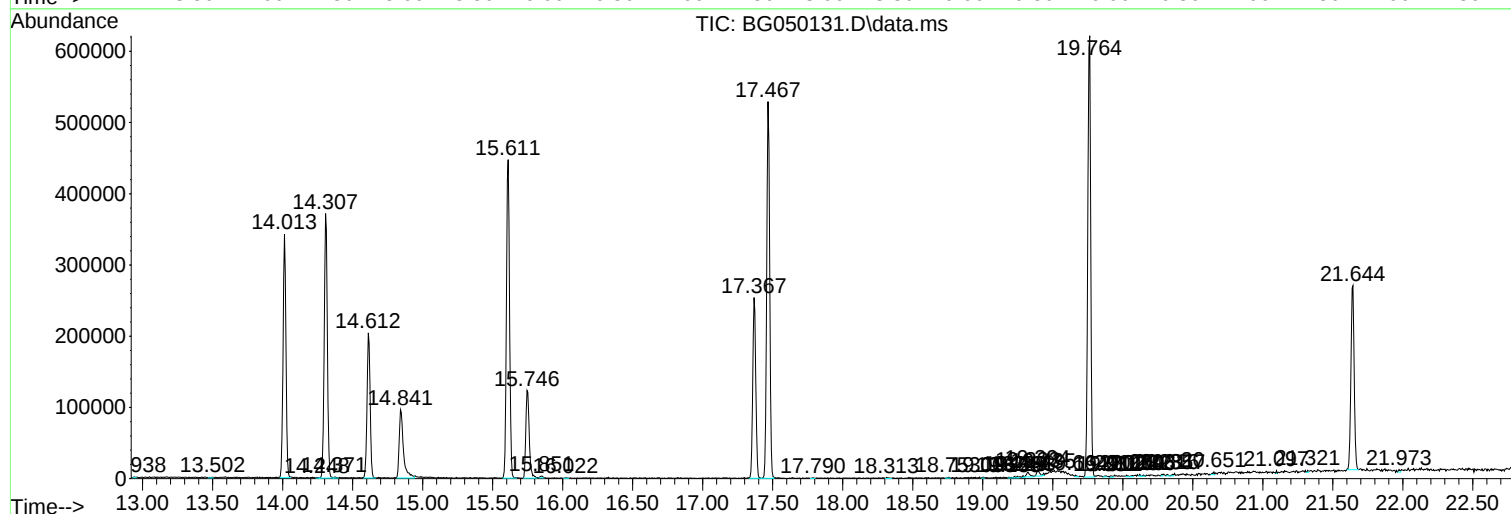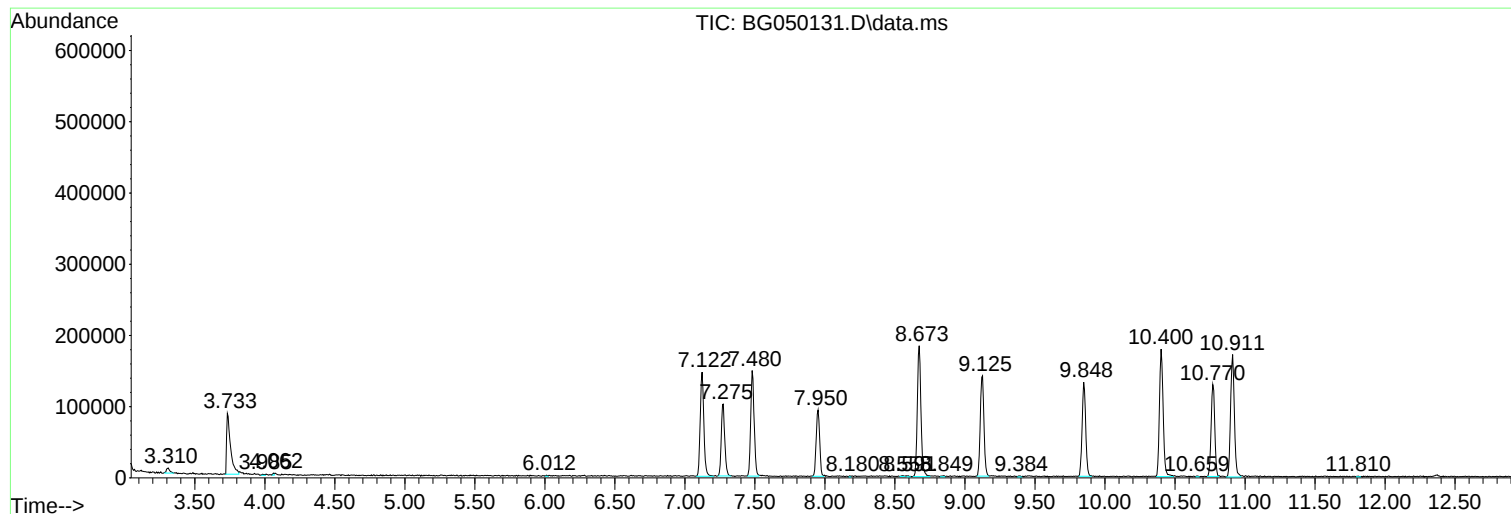

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090221\
Data File : BG050131.D
Acq On : 3 Sep 2021 14:51
Operator : CG/JU
Sample : PB138772BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK772

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090221\
Data File : BG050131.D
Acq On : 3 Sep 2021 14:51
Operator : CG/JU
Sample : PB138772BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK772

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
