

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090221\
 Data File : BG050157.D
 Acq On : 4 Sep 2021 9:20
 Operator : CG/JU
 Sample : M3566-21
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBKJ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
 Title : SVOA CALIBRATION

Signal : TIC: BG050157.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.302	42	45	51	rBV5	3610	6297	0.57%	0.067%
2	3.748	120	121	127	rBV4	10199	18844	1.70%	0.199%
3	3.966	154	158	162	rVB5	2268	3654	0.33%	0.039%
4	5.135	355	357	360	rVB	1633	1838	0.17%	0.019%
5	5.164	360	362	365	rBV2	1477	1732	0.16%	0.018%
6	5.611	435	438	441	rVB3	1302	1634	0.15%	0.017%
7	6.703	618	624	630	rBV2	1416	4315	0.39%	0.046%
8	6.921	658	661	663	rBV2	1623	1673	0.15%	0.018%
9	7.126	688	696	705	rBV	33753	64176	5.80%	0.678%
10	7.267	714	720	732	rVB	96864	173875	15.71%	1.838%
11	7.479	749	756	766	rBV	106411	199995	18.07%	2.114%
12	7.949	829	836	844	rVB	110703	187856	16.97%	1.985%
13	8.677	953	960	967	rBV	93071	169827	15.34%	1.795%
14	9.123	1028	1036	1044	rBV	140775	252982	22.85%	2.674%
15	9.846	1152	1159	1169	rVB2	123037	225968	20.41%	2.388%
16	10.398	1247	1253	1264	rBV2	157338	297492	26.87%	3.144%
17	10.539	1273	1277	1282	rBV5	7003	13732	1.24%	0.145%
18	10.768	1309	1316	1325	rVB	150800	261524	23.62%	2.764%
19	10.909	1333	1340	1347	rBV	126484	233365	21.08%	2.466%
20	12.360	1581	1587	1594	rBV2	3062	5138	0.46%	0.054%
21	12.631	1629	1633	1636	rBV2	1354	1851	0.17%	0.020%
22	13.206	1728	1731	1734	rVB3	1709	1635	0.15%	0.017%
23	13.271	1738	1742	1746	rBV2	854	1648	0.15%	0.017%
24	13.453	1767	1773	1780	rBV2	13509	19416	1.75%	0.205%
25	14.011	1862	1868	1876	rBV	384450	557171	50.33%	5.888%
26	14.305	1911	1918	1926	rVB	372003	580665	52.45%	6.137%
27	14.610	1963	1970	1977	rBV	230577	364207	32.90%	3.849%
28	14.857	2007	2012	2025	rBV4	18707	41524	3.75%	0.439%
29	14.980	2030	2033	2036	rBV2	2718	3914	0.35%	0.041%
30	15.350	2088	2096	2101	rBV4	6909	9849	0.89%	0.104%
31	15.603	2132	2139	2150	rVB	512393	790796	71.43%	8.358%
32	15.744	2157	2163	2174	rBV	168979	261977	23.66%	2.769%
33	15.850	2177	2181	2182	rVV3	2008	2604	0.24%	0.028%
34	16.502	2289	2292	2295	rVB	1778	1668	0.15%	0.018%
35	16.649	2312	2317	2322	rVB2	1842	3172	0.29%	0.034%
36	17.095	2389	2393	2399	rVB3	1997	3548	0.32%	0.037%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090221\
 Data File : BG050157.D
 Acq On : 4 Sep 2021 9:20
 Operator : CG/JU
 Sample : M3566-21
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBKJ6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
 Title : SVOA CALIBRATION

37	17.154	2399	2403	2405	rBV	1297	1901	0.17%	0.020%
38	17.365	2432	2439	2447	rBV	311872	446037	40.29%	4.714%
39	17.465	2449	2456	2466	rVB	620474	925301	83.58%	9.779%
40	17.641	2482	2486	2489	rBV	1392	1569	0.14%	0.017%
41	17.759	2501	2506	2509	rBV	1044	1567	0.14%	0.017%
42	18.017	2547	2550	2555	rBV3	3755	5514	0.50%	0.058%
43	18.135	2567	2570	2574	rBV	2330	2227	0.20%	0.024%
44	18.317	2597	2601	2605	rVB4	1954	3321	0.30%	0.035%
45	18.664	2657	2660	2663	rVB	1731	1895	0.17%	0.020%
46	18.758	2675	2676	2681	rVB2	2049	2294	0.21%	0.024%
47	19.316	2768	2771	2776	rVB3	6607	8940	0.81%	0.094%
48	19.392	2779	2784	2789	rVV	10327	13334	1.20%	0.141%
49	19.527	2806	2807	2810	rVB2	3472	2126	0.19%	0.022%
50	19.633	2824	2825	2827	rBV	2387	2088	0.19%	0.022%
51	19.756	2840	2846	2852	rBV	807041	1107028	100.00%	11.700%
52	19.985	2882	2885	2886	rVB3	2417	2187	0.20%	0.023%
53	20.044	2893	2895	2899	rBV5	1339	1689	0.15%	0.018%
54	20.244	2926	2929	2933	rBV4	3398	5409	0.49%	0.057%
55	20.761	3015	3017	3020	rVB4	5162	4224	0.38%	0.045%
56	20.808	3023	3025	3026	rVB2	4046	2324	0.21%	0.025%
57	21.013	3059	3060	3063	rBV3	3342	3021	0.27%	0.032%
58	21.060	3066	3068	3069	rBV2	3578	2389	0.22%	0.025%
59	21.225	3094	3096	3097	rBV2	3789	3669	0.33%	0.039%
60	21.266	3099	3103	3109	rVV8	16090	32121	2.90%	0.339%
61	21.636	3160	3166	3177	rVB	306780	511181	46.18%	5.402%
62	21.706	3177	3178	3179	rBV	4544	1754	0.16%	0.019%
63	21.724	3179	3181	3183	rVB3	3472	2004	0.18%	0.021%
64	23.193	3429	3431	3432	rBV2	3888	2376	0.21%	0.025%
65	23.398	3464	3466	3467	rBV	3633	2465	0.22%	0.026%
66	24.632	3665	3676	3687	rVB2	376335	1065378	96.24%	11.259%
67	24.849	3704	3713	3724	rVB2	178874	508912	45.97%	5.378%
68	26.083	3921	3923	3926	rBV3	4573	3939	0.36%	0.042%
69	27.951	4240	4241	4242	rVB	5354	1887	0.17%	0.020%
70	28.239	4287	4290	4293	rBV5	4515	6239	0.56%	0.066%
71	31.352	4818	4820	4821	rBV2	4014	2197	0.20%	0.023%




Sum of corrected areas: 9462069

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090221\
Data File : BG050157.D
Acq On : 4 Sep 2021 9:20
Operator : CG/JU
Sample : M3566-21
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBKJ6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

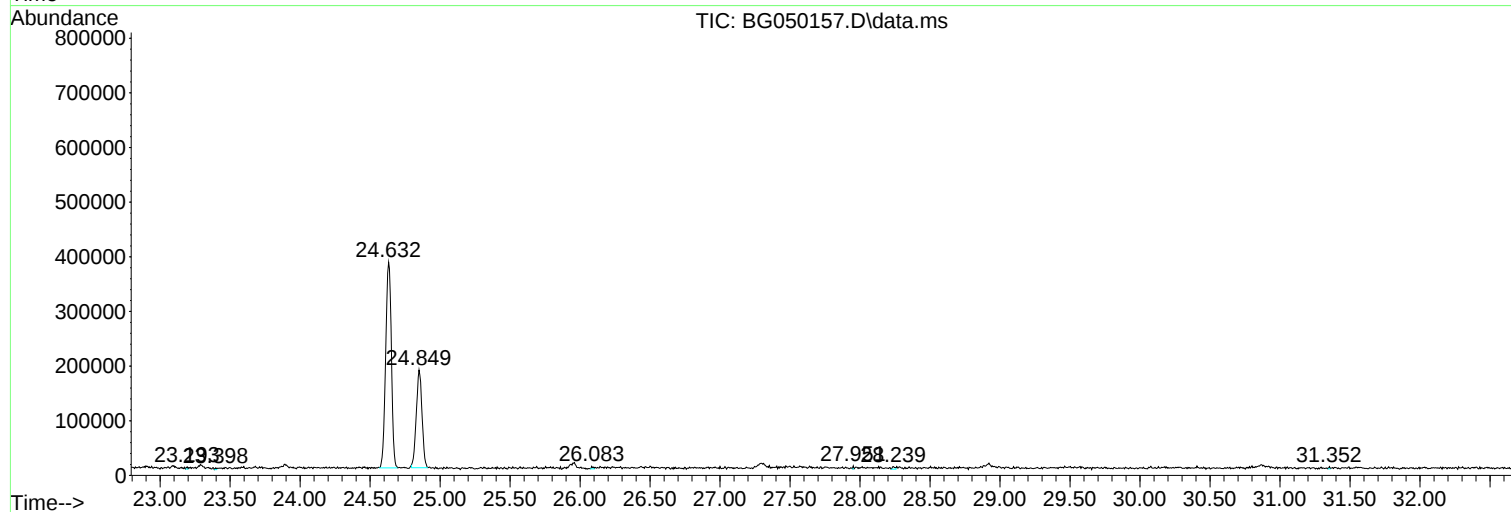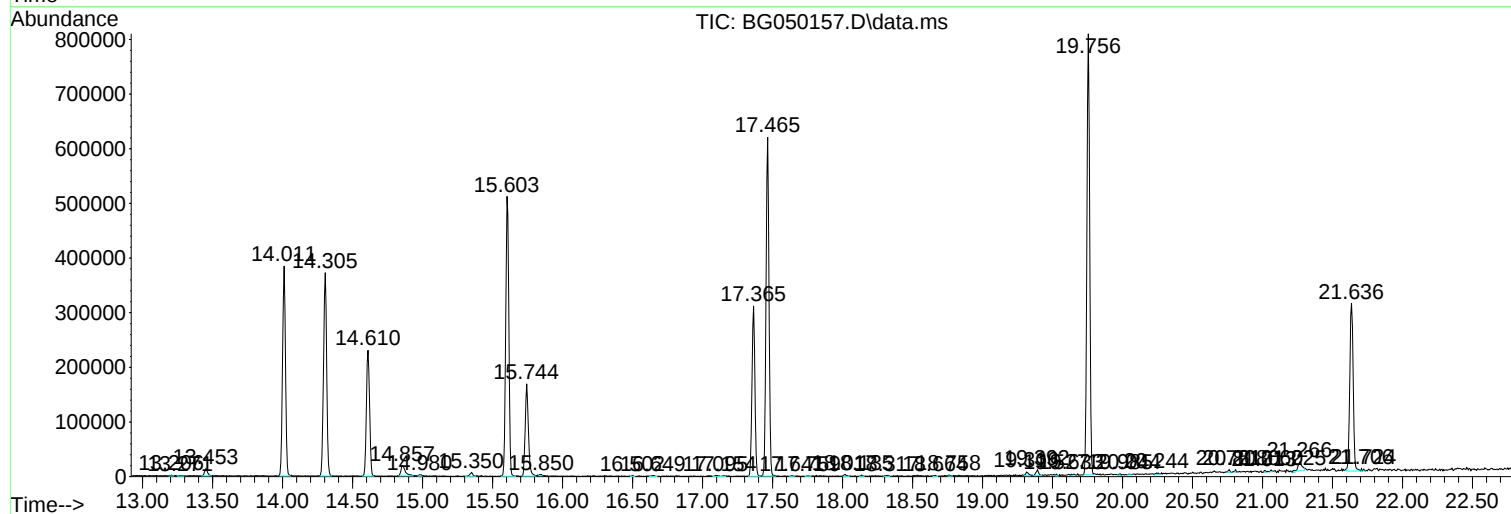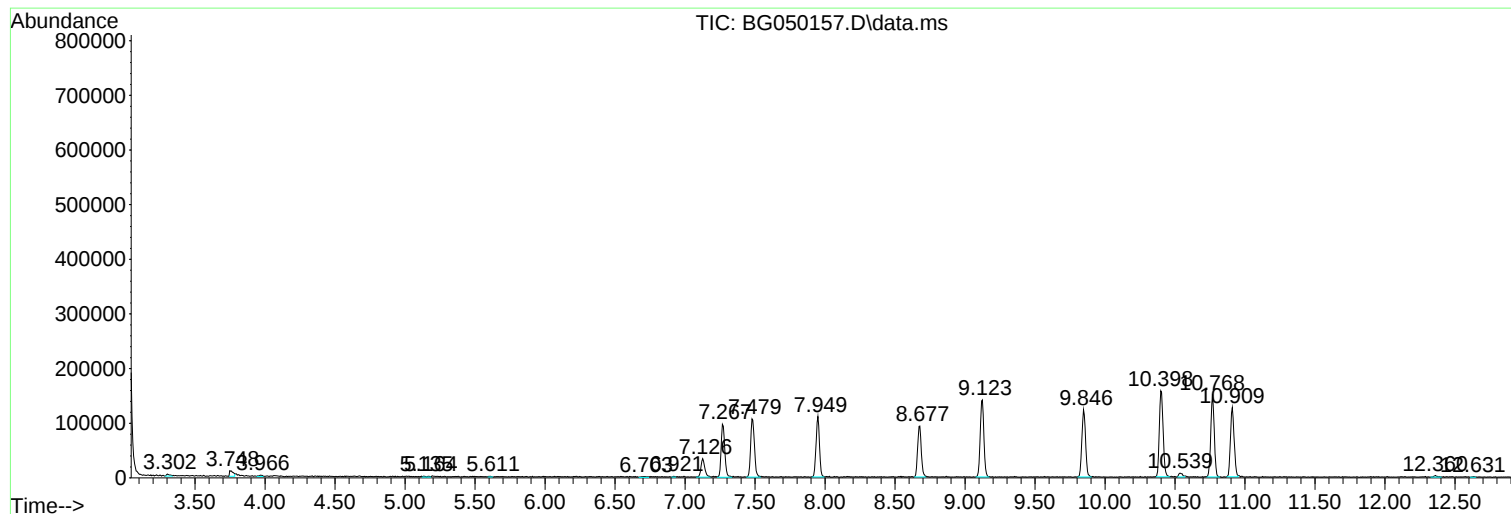

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090221\
Data File : BG050157.D
Acq On : 4 Sep 2021 9:20
Operator : CG/JU
Sample : M3566-21
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBKJ6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090221\
Data File : BG050157.D
Acq On : 4 Sep 2021 9:20
Operator : CG/JU
Sample : M3566-21
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBKJ6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
