


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090221\
 Data File : BG050099.D
 Acq On : 2 Sep 2021 16:25
 Operator : CG/JU
 Sample : DFTPP418
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP418

Integration File: LSCINT.P

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
 Title : SVOA CALIBRATION
 Last Update : Mon Aug 30 14:59:55 2021

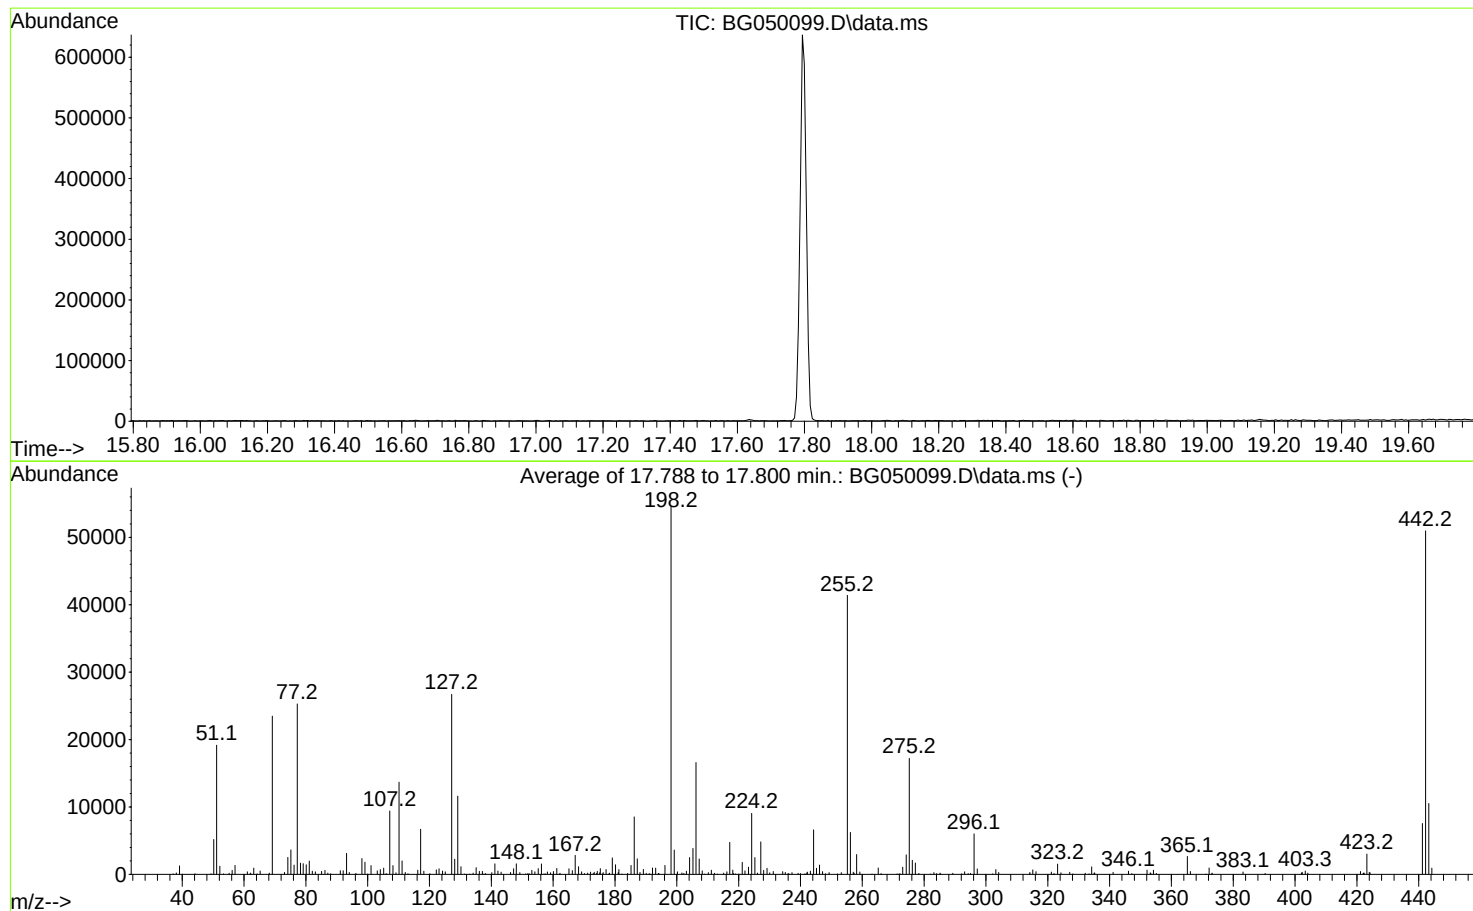

AutoFind: Scans 2511, 2512, 2513; Background Corrected with Scan 2506

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.1	19162	PASS
68	69	0.00	2	0.8	184	PASS
69	198	0.00	100	43.0	23483	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.9	26715	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	54581	PASS
199	198	5	9	6.6	3603	PASS
275	198	10	60	31.5	17213	PASS
365	198	1	100	4.9	2656	PASS
441	198	0.01	100	13.8	7550	PASS
442	198	50	100	93.4	50971	PASS
443	442	15	24	20.6	10510	PASS

m/z	Abundance
40.15	324.0
44.15	284.0
148.15	164.0
220.45	213.0
281.45	177.0

Instrument :
BNA_G
ClientSampleId :
DFTPP418

m/z	Abundance
38.05	195.0
39.15	1396.0
40.05	181.0
44.25	529.0
50.15	4765.0
51.15	15518.0
52.15	1163.0
55.15	198.0
56.15	663.0
57.05	1286.0
60.95	295.0
61.95	234.0
63.15	752.0
65.25	457.0
69.15	20240.0
73.15	279.0
74.15	1953.0
75.15	3207.0
76.15	1185.0
77.15	21272.0
78.25	1213.0
79.15	1599.0
80.15	1159.0
81.05	1768.0
82.05	301.0
83.05	483.0
85.15	454.0
86.25	474.0
87.05	283.0
91.15	779.0
92.05	342.0
93.15	2300.0
93.95	288.0
96.05	185.0
98.15	2111.0
99.05	1541.0
101.05	1052.0
103.15	604.0
104.15	780.0
105.15	811.0
105.85	166.0
107.15	7576.0
108.15	927.0
110.15	10605.0
111.15	1728.0
112.15	446.0
116.15	368.0
117.15	5123.0
118.15	357.0
122.15	547.0
123.15	565.0
124.15	354.0
125.15	182.0
127.15	20176.0
128.15	1953.0
129.15	9827.0
130.15	941.0
135.05	888.0
136.05	226.0
137.15	398.0
140.15	288.0
141.15	917.0
142.15	504.0
143.15	326.0
146.25	154.0
147.15	534.0
148.15	1400.0
149.25	191.0
152.25	167.0
153.05	368.0
154.15	255.0
155.15	782.0
156.15	1171.0
158.05	276.0
160.05	244.0
161.15	759.0
165.15	755.0
166.15	413.0
167.15	2024.0
168.15	947.0
169.25	270.0
170.15	211.0
171.25	153.0
172.95	429.0
174.05	454.0
175.05	698.0
176.15	348.0
177.05	523.0
178.05	219.0
179.15	1646.0
180.15	1277.0
181.05	855.0

Instrument :
BNA_G
ClientSampleId :
DFTPP418

184.15	271.0
185.25	997.0
186.25	5346.0
187.25	1771.0
188.15	246.0
189.15	493.0
192.15	753.0
193.15	717.0
194.05	178.0
196.15	936.0
198.15	41384.0
199.15	2665.0
200.15	207.0
203.05	362.0
204.15	1837.0
205.25	2656.0
206.25	11454.0
207.25	2168.0
208.15	422.0
211.05	553.0
216.15	239.0
217.15	3791.0
218.35	393.0
221.15	1655.0
223.25	684.0
224.15	6251.0
225.25	1722.0
226.05	237.0
227.15	3495.0
228.05	435.0
229.15	342.0
231.25	292.0
234.15	491.0
235.15	397.0
235.85	183.0
236.35	179.0
237.25	192.0
240.05	174.0
241.25	164.0
242.05	645.0
243.25	227.0
244.25	5183.0
245.15	801.0
246.15	810.0
247.15	283.0
253.15	243.0
255.15	28104.0
256.15	4299.0
257.05	688.0
258.15	2047.0
259.25	279.0
265.15	641.0
266.25	194.0
273.15	629.0
274.25	1784.0
275.15	10806.0
276.15	1516.0
277.15	1186.0
282.15	182.0
283.15	276.0
284.05	336.0
285.25	235.0
293.05	185.0
296.15	3896.0
297.15	454.0
303.25	491.0
304.15	299.0
314.05	265.0
315.15	443.0
316.15	328.0
321.15	326.0
323.15	910.0
324.35	183.0
334.25	533.0
334.95	198.0
335.25	187.0
341.15	160.0
346.25	253.0
352.05	423.0
353.15	286.0
354.15	427.0
365.15	1908.0
366.05	253.0
372.15	589.0
372.95	188.0
383.25	253.0
402.15	274.0
403.25	259.0
421.15	243.0
421.95	200.0
423.25	1995.0
423.95	434.0
441.15	4036.0
442.15	27976.0
443.25	6058.0
444.25	804.0

Instrument :
BNA_G
ClientSampleId :
DFTPP418

m/z	Abundance
38.05	193.0
39.15	1261.0
40.15	454.0
44.15	315.0
50.25	5700.0
51.15	22912.0
52.15	1424.0
56.15	595.0
57.15	1506.0
61.05	433.0
62.15	280.0
63.15	1215.0
65.15	449.0
69.15	29000.0
73.15	330.0
74.15	2807.0
75.15	4391.0
76.15	1778.0
77.25	30024.0
78.25	2163.0
79.15	1569.0
80.05	1851.0
81.15	2567.0
82.15	548.0
83.05	420.0
85.15	358.0
86.15	680.0
88.05	251.0
91.15	372.0
92.15	704.0
93.15	3780.0
94.05	236.0
96.25	286.0
98.15	2743.0
99.15	2087.0
101.15	1469.0
103.05	647.0
104.05	732.0
105.15	1207.0
106.15	277.0
107.15	11860.0
108.15	1711.0
109.15	459.0
110.15	16856.0
111.15	2235.0
112.15	383.0
116.15	923.0
117.15	8344.0
118.15	593.0
120.15	295.0
122.25	730.0
123.05	1293.0
124.25	664.0
125.15	665.0
127.15	33400.0
128.15	2849.0
129.15	13999.0
130.15	1351.0
131.35	169.0
133.05	157.0
134.15	390.0
135.15	981.0
136.15	491.0
137.15	488.0
138.15	174.0
140.15	202.0
141.15	1980.0
142.25	537.0
143.15	452.0
146.05	232.0
147.15	1015.0
148.05	2240.0
149.15	263.0
151.75	309.0
153.15	524.0
154.05	496.0
155.15	836.0
156.25	1939.0
157.05	207.0
158.15	436.0
159.15	381.0
160.15	620.0
161.15	794.0
161.95	172.0
162.25	203.0
165.05	738.0
166.25	698.0
167.15	3111.0
168.15	1215.0
169.15	525.0
171.05	204.0
172.05	600.0

Instrument :
BNA_G
ClientSampleId :
DFTPP418

173.25	577.0
174.25	856.0
175.25	1321.0
176.25	242.0
177.15	897.0
178.25	294.0
179.15	2873.0
180.15	1631.0
181.25	1432.0
182.25	159.0
184.05	192.0
185.15	1538.0
186.15	10168.0
187.15	2821.0
188.05	290.0
189.25	982.0
190.05	325.0
191.05	232.0
192.15	1093.0
193.15	1164.0
194.05	274.0
196.15	1695.0
198.15	64480.0
199.15	4412.0
200.15	549.0
201.75	414.0
202.35	175.0
203.15	442.0
204.15	2557.0
205.15	4200.0
206.25	19960.0
207.25	2194.0
208.15	491.0
209.05	175.0
210.25	423.0
211.15	689.0
212.25	196.0
213.15	156.0
215.15	329.0
216.25	498.0
217.15	5550.0
218.05	1046.0
219.05	195.0
221.15	1640.0
222.05	755.0
223.15	1290.0
224.25	11001.0
225.25	2349.0
226.15	355.0
227.15	5338.0
228.15	637.0
229.25	1318.0
230.05	371.0
231.15	628.0
234.25	506.0
235.15	187.0
236.05	179.0
237.25	301.0
239.25	280.0
239.95	185.0
242.25	485.0
243.25	684.0
244.25	7898.0
245.15	1000.0
246.15	1760.0
247.15	342.0
248.15	283.0
249.25	401.0
251.95	197.0
253.15	177.0
255.15	48280.0
256.15	7554.0
257.35	567.0
258.15	3082.0
259.05	223.0
265.15	1056.0
265.95	172.0
271.25	249.0
271.95	229.0
273.15	1231.0
274.15	3055.0
275.15	21152.0
276.25	2625.0
277.15	2218.0
278.35	295.0
283.15	491.0
285.05	313.0
289.35	241.0
292.15	258.0
293.05	548.0
294.35	188.0
294.95	174.0
296.15	6980.0
297.15	1001.0
302.15	222.0
303.15	712.0

Instrument :
BNA_G
ClientSampleId :
DFTPP418

304.15	388.0
314.25	416.0
315.25	748.0
316.15	466.0
321.15	387.0
321.95	192.0
323.25	1819.0
324.15	337.0
327.05	487.0
332.25	183.0
334.15	1422.0
335.05	369.0
341.15	413.0
346.05	593.0
347.25	161.0
352.15	770.0
353.35	449.0
354.25	778.0
355.05	248.0
365.15	3270.0
366.15	546.0
372.25	1052.0
373.15	179.0
383.05	491.0
390.35	203.0
401.95	377.0
402.45	298.0
403.35	627.0
404.05	205.0
421.25	518.0
422.15	544.0
423.25	3424.0
424.05	467.0
441.25	8233.0
442.15	56000.0
443.25	12349.0
444.25	1036.0

Instrument :
BNA_G
ClientSampleId :
DFTPP418

m/z	Abundance
37.05	186.0
38.15	276.0
39.15	1144.0
40.15	396.0
44.25	271.0
49.35	272.0
50.15	5053.0
51.15	19056.0
52.15	1021.0
53.35	223.0
55.25	318.0
56.15	526.0
57.15	1213.0
61.15	383.0
62.15	281.0
63.15	849.0
64.25	246.0
65.15	570.0
68.15	551.0
69.15	21208.0
73.05	263.0
74.15	2796.0
75.15	3337.0
76.25	1178.0
77.15	24560.0
78.25	1611.0
79.15	1624.0
80.15	1275.0
81.05	1609.0
82.15	580.0
83.15	263.0
85.05	510.0
86.15	599.0
87.15	316.0
91.15	487.0
92.15	602.0
93.15	3276.0
94.15	307.0
98.15	2197.0
99.15	1791.0
100.05	167.0
101.15	1384.0
103.05	332.0
104.15	661.0
105.15	765.0
107.15	8765.0
108.15	1249.0
109.15	253.0
110.15	13559.0
111.15	2014.0
113.05	255.0
116.25	536.0
117.15	6590.0
118.15	493.0
122.15	706.0
123.15	640.0
124.15	487.0
125.05	301.0
127.15	26568.0
128.15	1998.0
129.15	10993.0
130.15	1135.0
134.05	206.0
135.15	1108.0
136.15	641.0
137.05	488.0
137.65	163.0
138.15	168.0
140.15	277.0
141.15	1817.0
142.05	446.0
143.15	201.0
146.25	480.0
147.25	956.0
148.15	1534.0
149.25	366.0
151.15	224.0
152.15	203.0
153.05	869.0
154.15	395.0
155.15	933.0
156.25	1491.0
157.45	219.0
158.15	382.0
159.15	372.0
160.05	451.0
161.15	1051.0
162.15	273.0
165.15	984.0
166.15	597.0
167.15	3323.0
168.25	1275.0

Instrument :
BNA_G
ClientSampleId :
DFTPP418

169.25	357.0
170.15	173.0
171.15	253.0
172.15	386.0
173.35	383.0
174.25	485.0
175.25	1275.0
175.85	201.0
176.25	199.0
177.15	705.0
178.15	259.0
179.15	2794.0
180.15	1358.0
181.25	730.0
185.15	1450.0
186.15	10034.0
187.15	2304.0
188.05	323.0
189.15	737.0
190.15	162.0
191.25	299.0
192.05	1020.0
193.15	936.0
194.25	273.0
196.15	1382.0
198.15	57880.0
199.15	3732.0
200.25	423.0
201.55	249.0
202.15	275.0
203.15	632.0
204.15	3068.0
205.15	4706.0
206.15	18392.0
207.25	2484.0
208.25	671.0
210.15	359.0
211.25	593.0
212.15	279.0
215.15	235.0
216.15	412.0
217.15	4938.0
218.15	852.0
220.05	173.0
220.35	173.0
221.15	2085.0
222.05	785.0
223.15	1232.0
224.25	9918.0
225.25	3374.0
227.15	5598.0
228.15	739.0
229.15	1085.0
230.05	318.0
231.15	382.0
234.35	245.0
235.05	274.0
236.15	180.0
237.25	286.0
239.25	241.0
241.55	181.0
242.25	509.0
243.15	522.0
244.25	6731.0
245.25	892.0
246.15	1566.0
247.15	565.0
249.25	386.0
253.25	385.0
255.15	47816.0
256.15	6797.0
257.15	340.0
258.15	3711.0
259.25	581.0
263.15	153.0
265.15	1181.0
272.25	191.0
273.05	1361.0
274.15	3833.0
275.25	19680.0
276.15	2150.0
277.15	1634.0
278.15	169.0
285.35	224.0
289.15	236.0
293.15	406.0
294.15	172.0
295.05	237.0
296.15	7155.0
297.25	943.0
303.25	914.0
304.25	188.0
314.15	448.0
315.05	830.0
316.25	438.0
321.15	291.0

Instrument :
BNA_G
ClientSampleId :
DFTPP418

322.15	202.0
323.25	1819.0
324.35	193.0
327.15	428.0
328.15	236.0
332.05	300.0
333.35	237.0
334.25	1398.0
335.15	455.0
341.15	366.0
346.15	546.0
347.15	224.0
352.15	740.0
353.15	401.0
354.15	624.0
355.15	209.0
365.15	2791.0
366.25	504.0
371.15	168.0
372.25	1225.0
373.25	425.0
383.25	353.0
390.25	232.0
402.25	597.0
403.25	631.0
404.15	356.0
421.05	522.0
422.35	584.0
423.15	3631.0
424.25	747.0
441.15	10382.0
442.25	68936.0
443.25	13123.0
444.25	970.0

Instrument :
BNA_G
ClientSampleId :
DFTPP418