
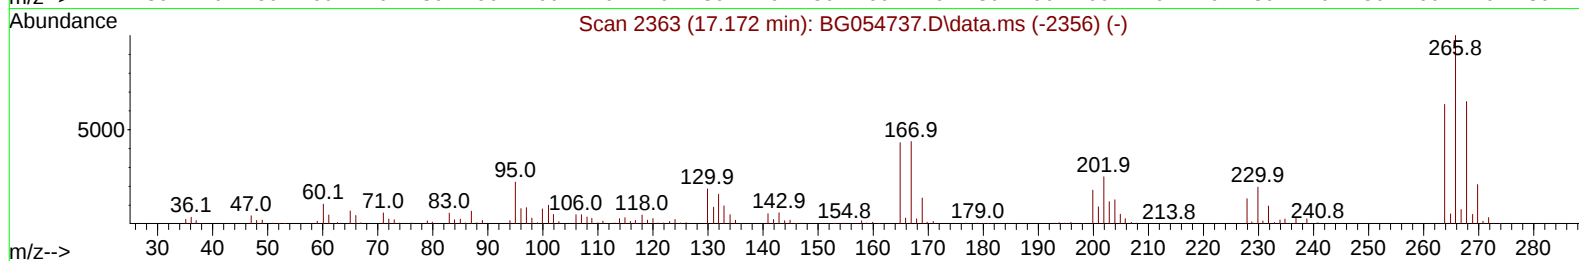
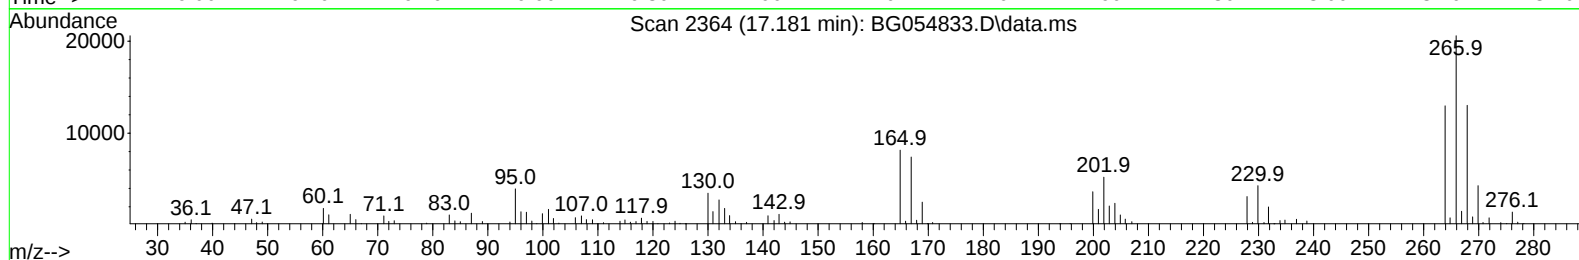


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090222\
Data File : BG054833.D
Acq On : 2 Sep 2022 9:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 03 02:36:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 25 17:50:55 2022
Response via : Initial Calibration

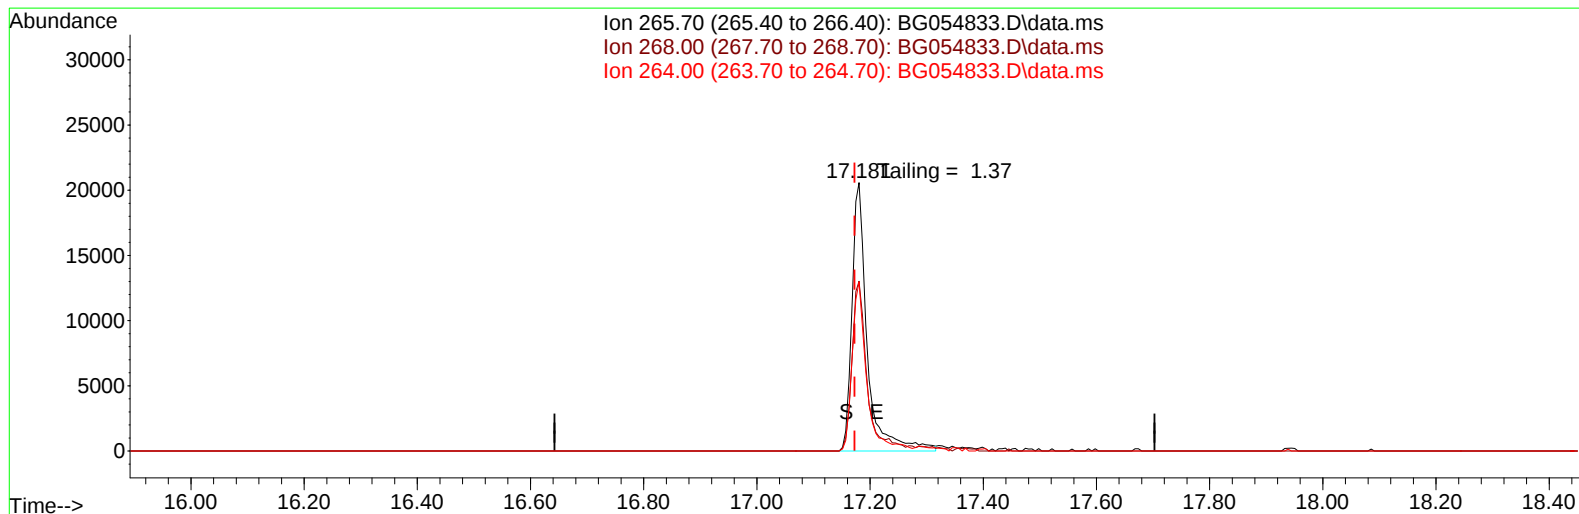

TIC: BG054833.D\data.ms

(70) Pentachlorophenol (C)




17.181min (+ 0.008) 16728.96 ng

response 39265

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	63.24
264.00	61.70	63.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090222\
Data File : BG054833.D
Acq On : 2 Sep 2022 9:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 03 02:36:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 25 17:50:55 2022
Response via : Initial Calibration

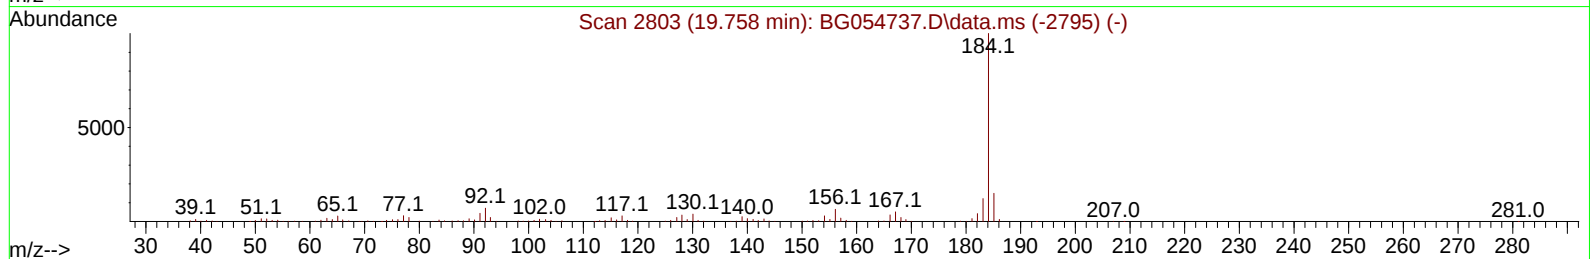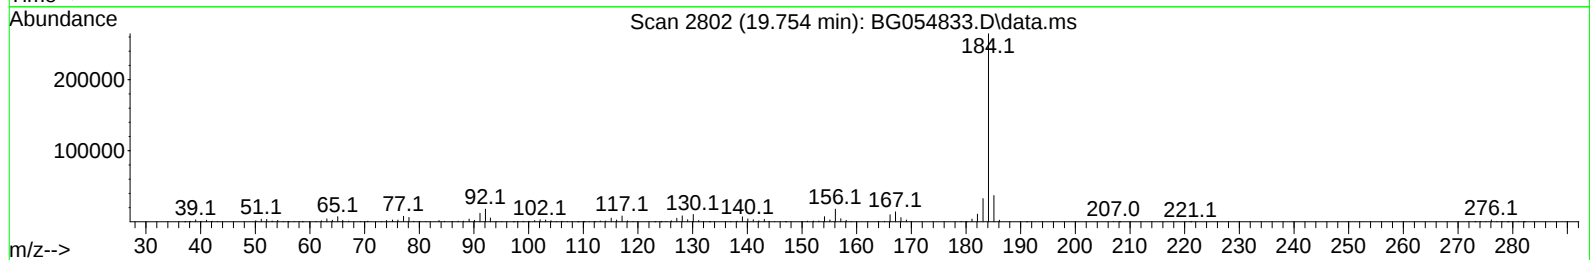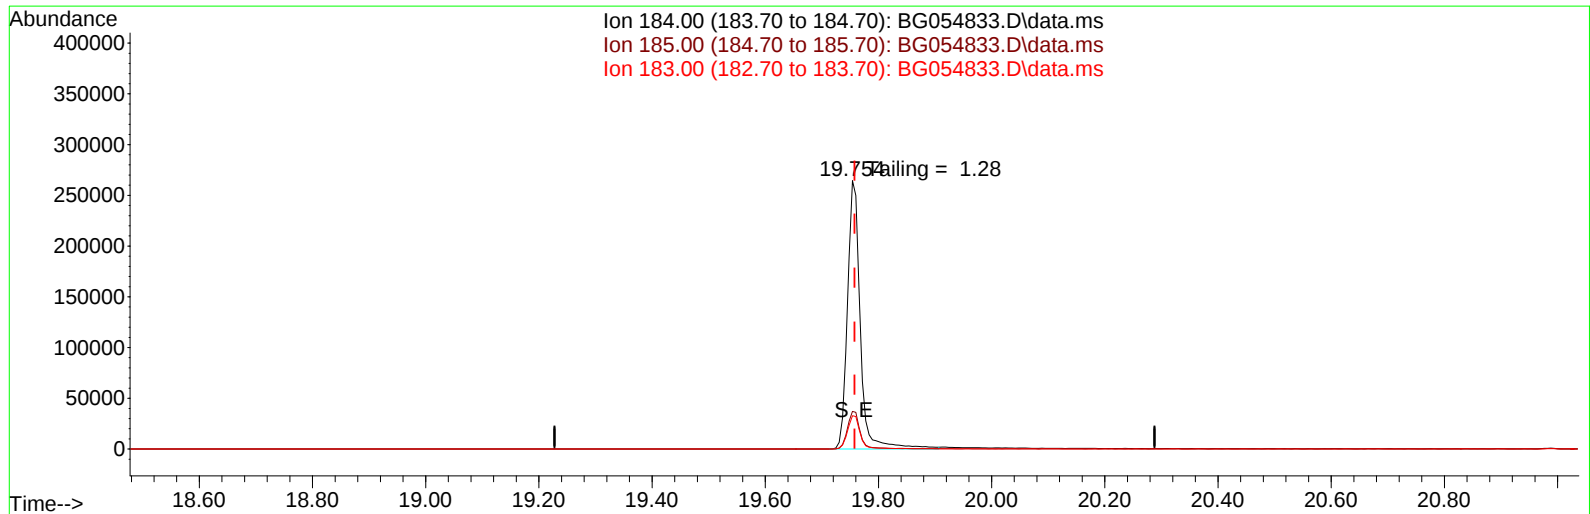

TIC: BG054833.D\data.ms

(77) Benzidine

19.754min (-0.004) 0.00 ng

response 417661

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.03
183.00	12.30	12.43
0.00	0.00	0.00