
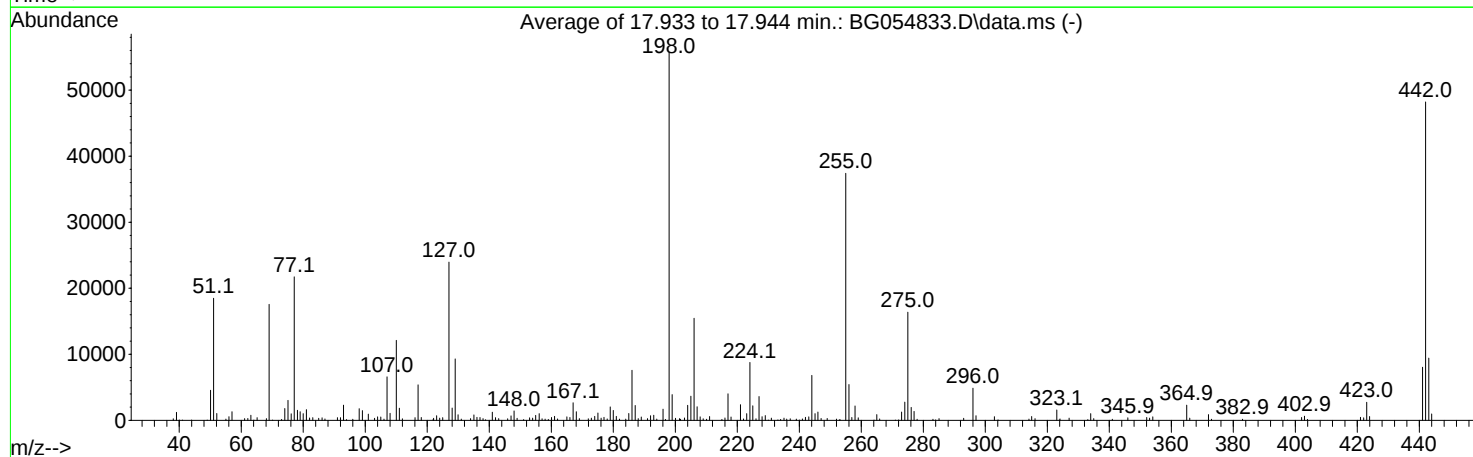


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090222\
 Data File : BG054833.D
 Acq On : 2 Sep 2022 9:15
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 25 17:50:55 2022

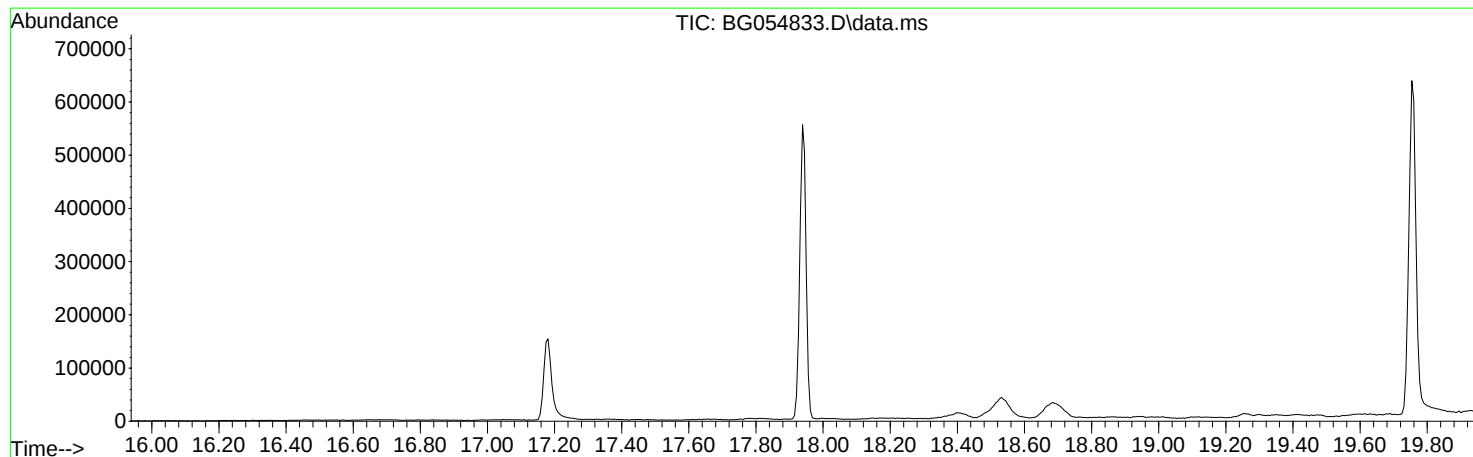

AutoFind: Scans 2492, 2493, 2494; Background Corrected with Scan 2485

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.2	18477	PASS
68	69	0.00	2	1.5	267	PASS
69	198	0.00	100	31.6	17573	PASS
70	69	0.00	2	0.3	53	PASS
127	198	10	80	43.0	23949	PASS
197	198	0.00	2	0.3	156	PASS
198	198	100	100	100.0	55696	PASS
199	198	5	9	7.0	3903	PASS
275	198	10	60	29.4	16369	PASS
365	198	1	100	4.1	2308	PASS
441	198	0.01	100	14.4	8034	PASS
442	442	50	100	100.0	48213	PASS
443	442	15	24	19.6	9435	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
9/2/2022	BNA_G	<u>BG054833.D</u>
Compound Name	Response	Retention Time
DDT	191726	20.988
DDD	6727	20.541
DDE	835	20.036
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7562	199288	3.79

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090222\
 Data File : BG054833.D
 Acq On : 2 Sep 2022 9:15
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Sep 03 02:36:47 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 25 17:50:55 2022
 Response via : Initial Calibration

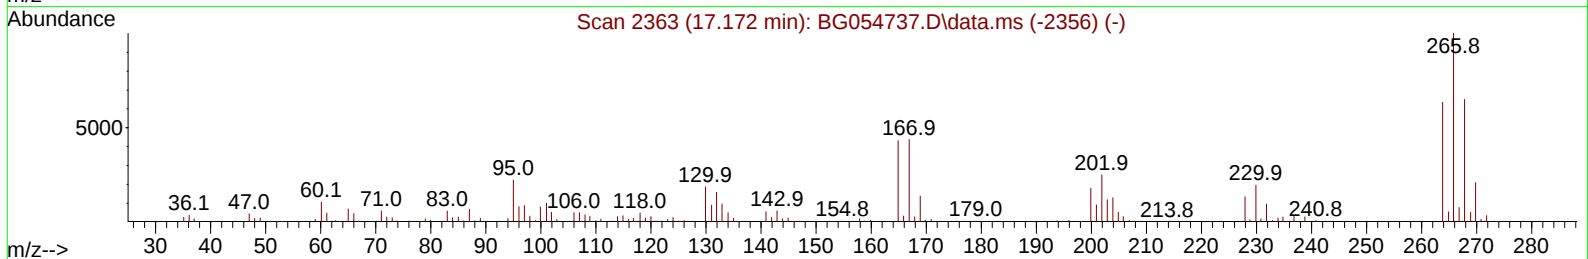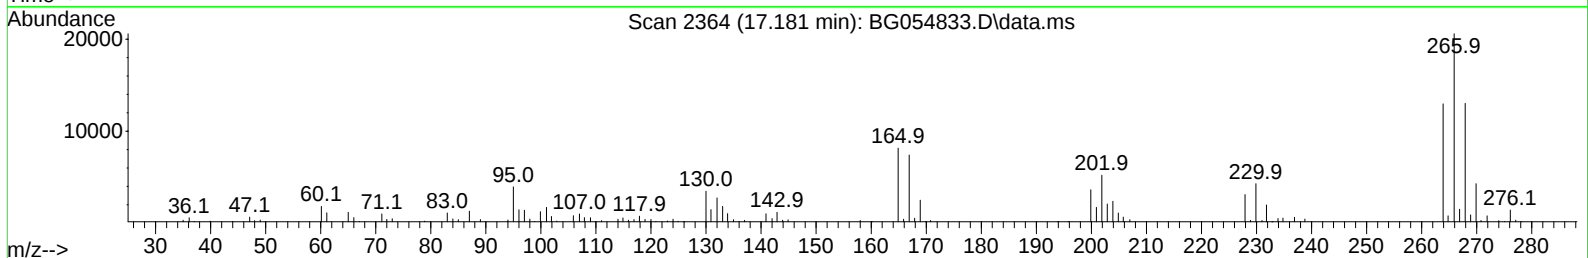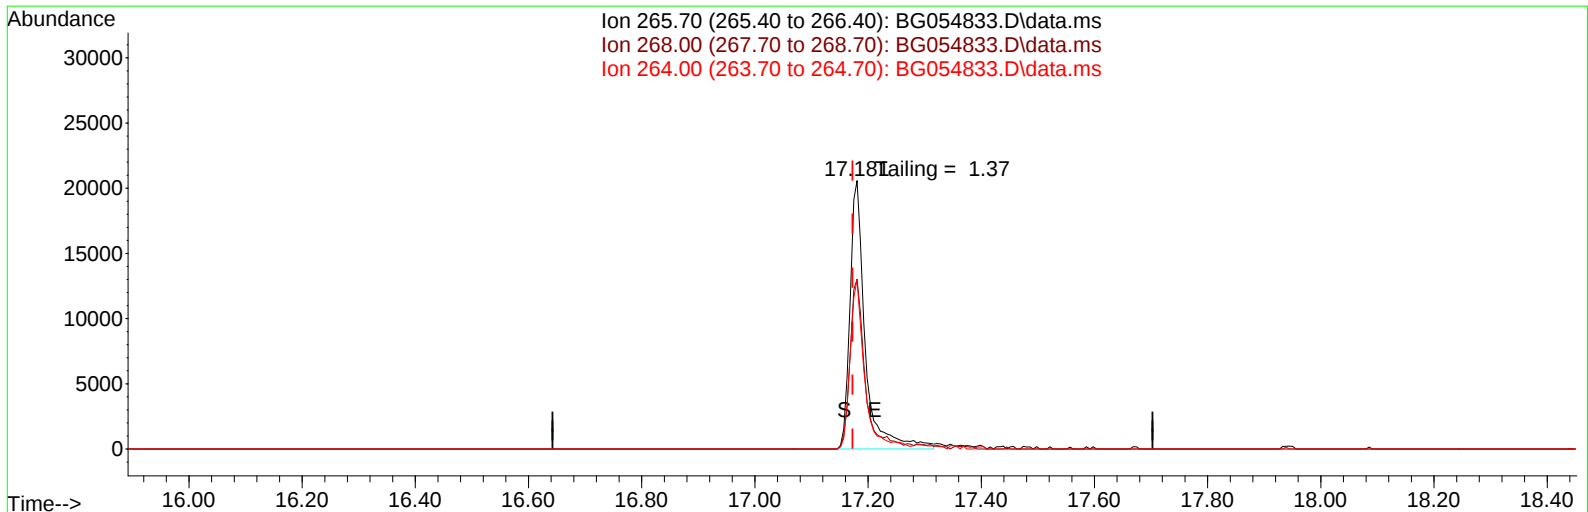

TIC: BG054833.D\data.ms

(70) Pentachlorophenol (C)

17.181min (+ 0.008) 16728.96 ng




response 39265

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	63.24
264.00	61.70	63.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090222\
Data File : BG054833.D
Acq On : 2 Sep 2022 9:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Sep 03 02:36:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 25 17:50:55 2022
Response via : Initial Calibration

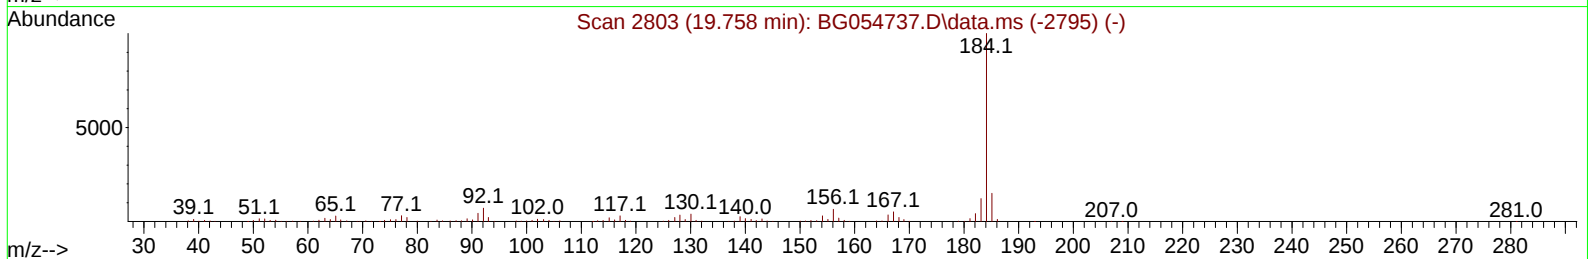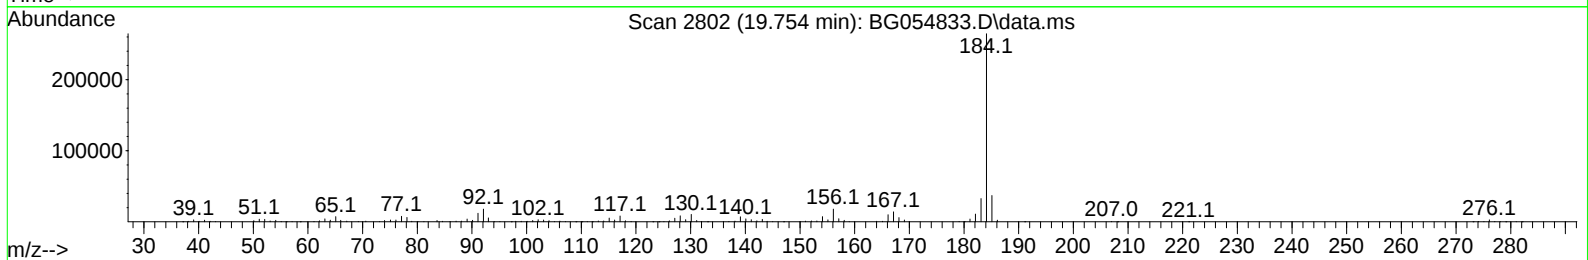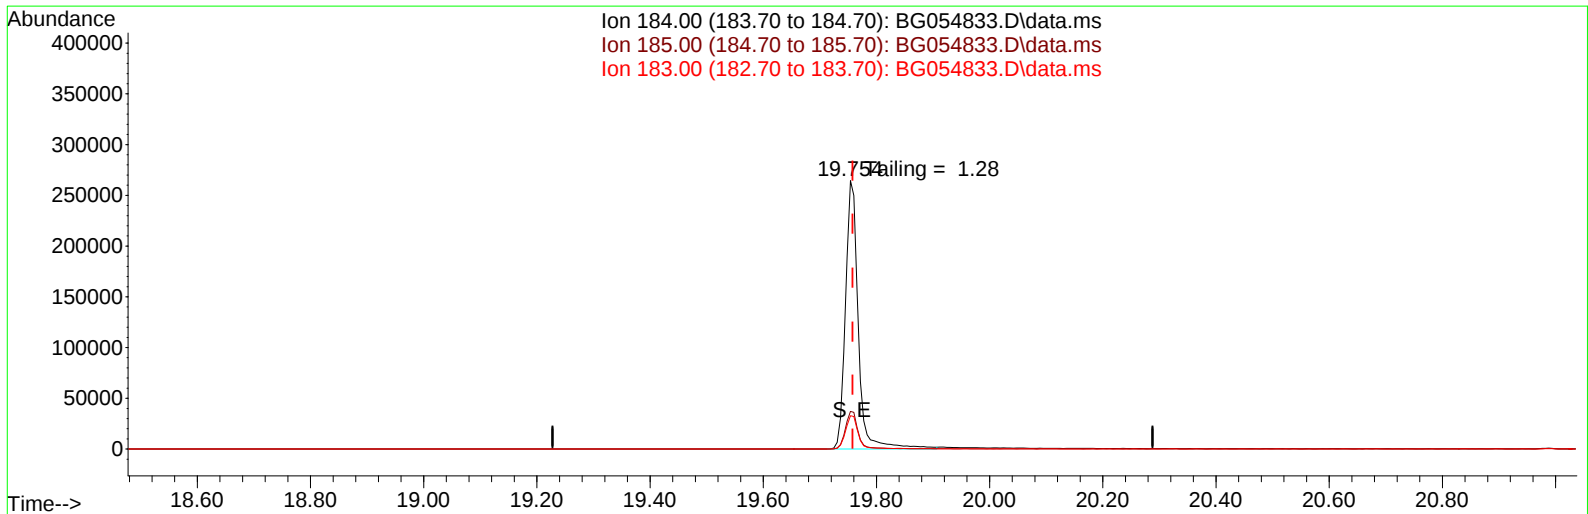

TIC: BG054833.D\data.ms

(77) Benzidine

19.754min (-0.004) 0.00 ng

response 417661

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.03
183.00	12.30	12.43
0.00	0.00	0.00