
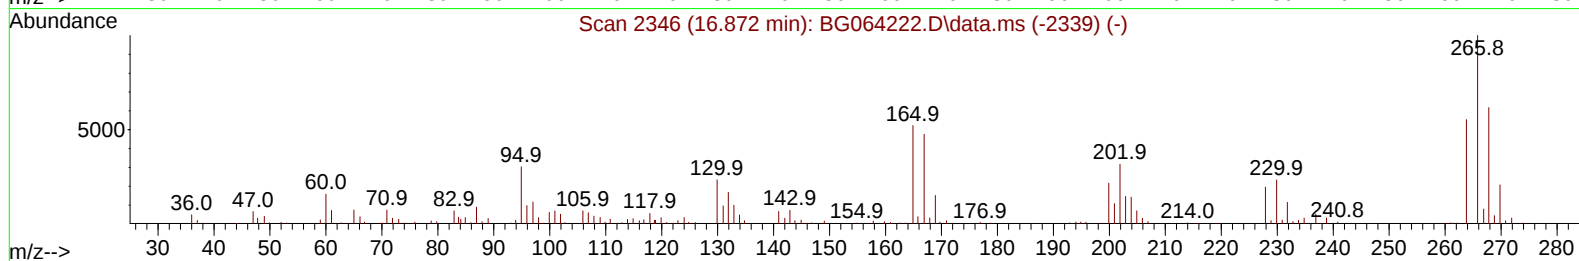
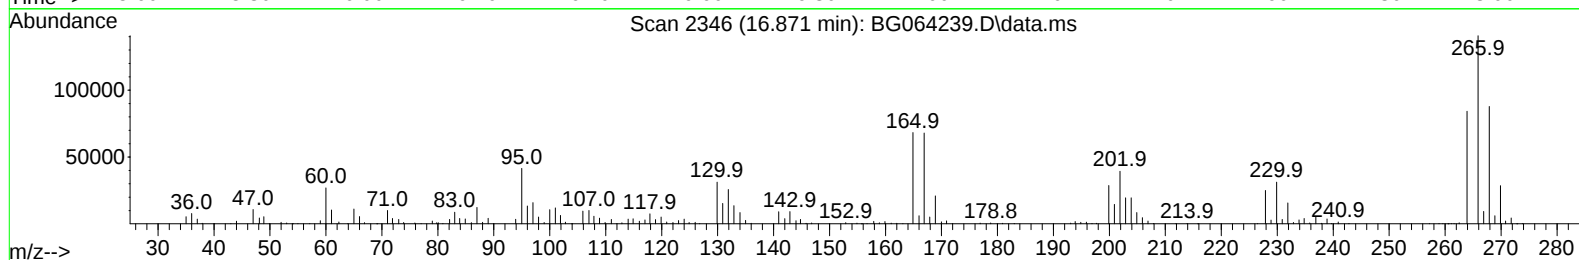


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090225\
Data File : BG064239.D
Acq On : 2 Sep 2025 9:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 02 12:14:30 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 28 17:41:58 2025
Response via : Initial Calibration

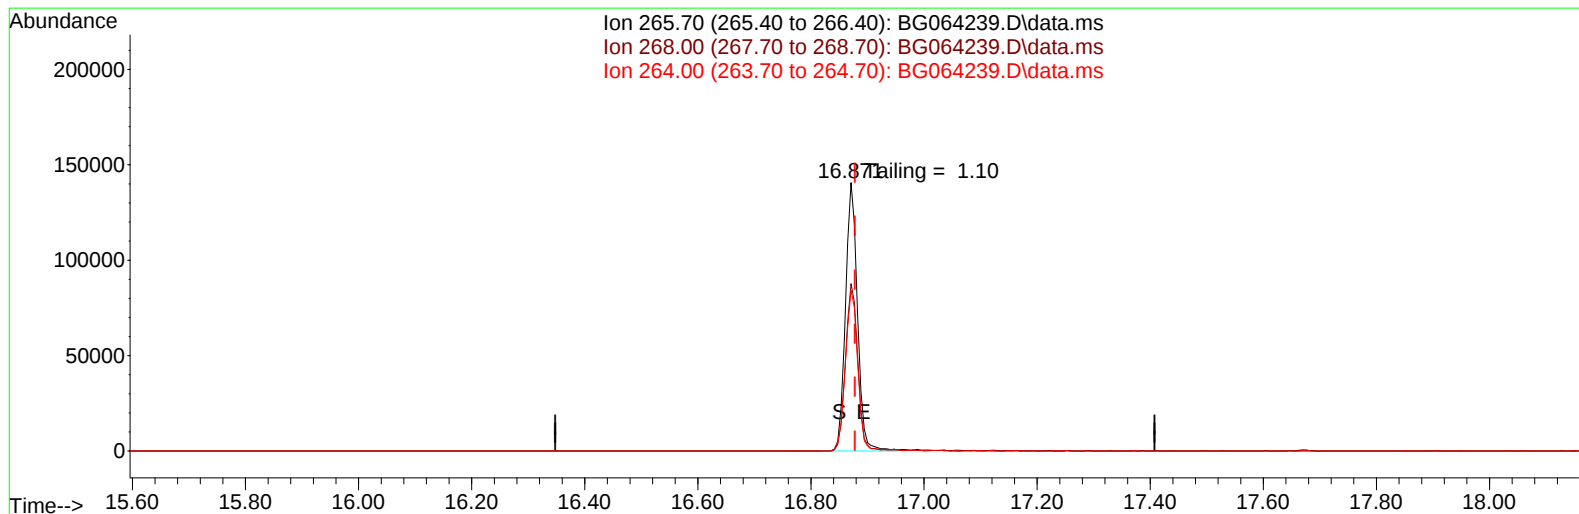

TIC: BG064239.D\data.ms

(70) Pentachlorophenol (C)




16.871min (-0.007) 208165.51 ng

response 206933

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	62.39
264.00	55.40	59.87
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090225\
Data File : BG064239.D
Acq On : 2 Sep 2025 9:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 02 12:14:30 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 28 17:41:58 2025
Response via : Initial Calibration

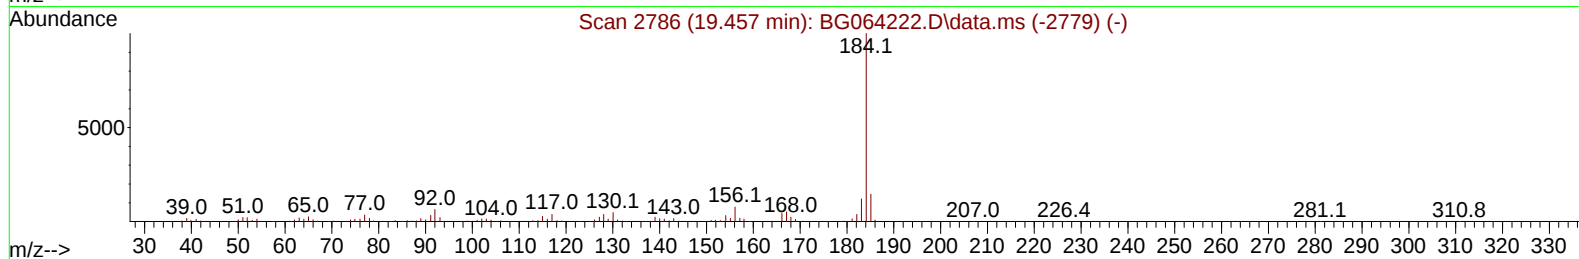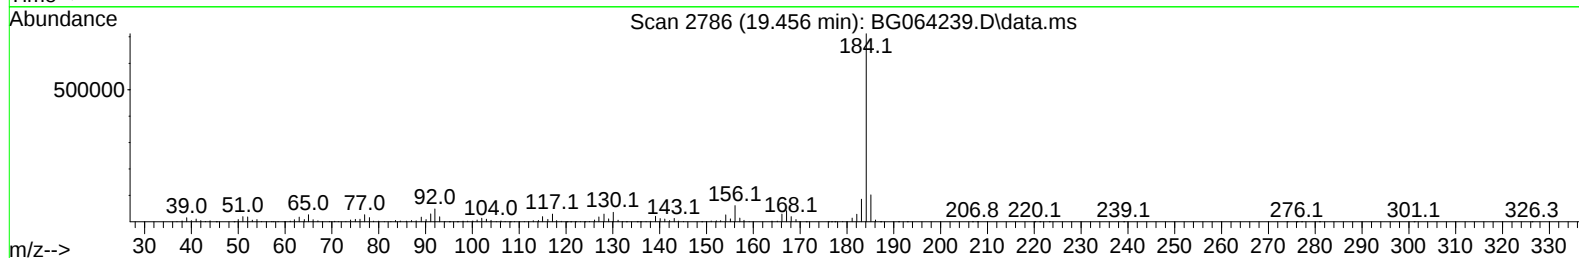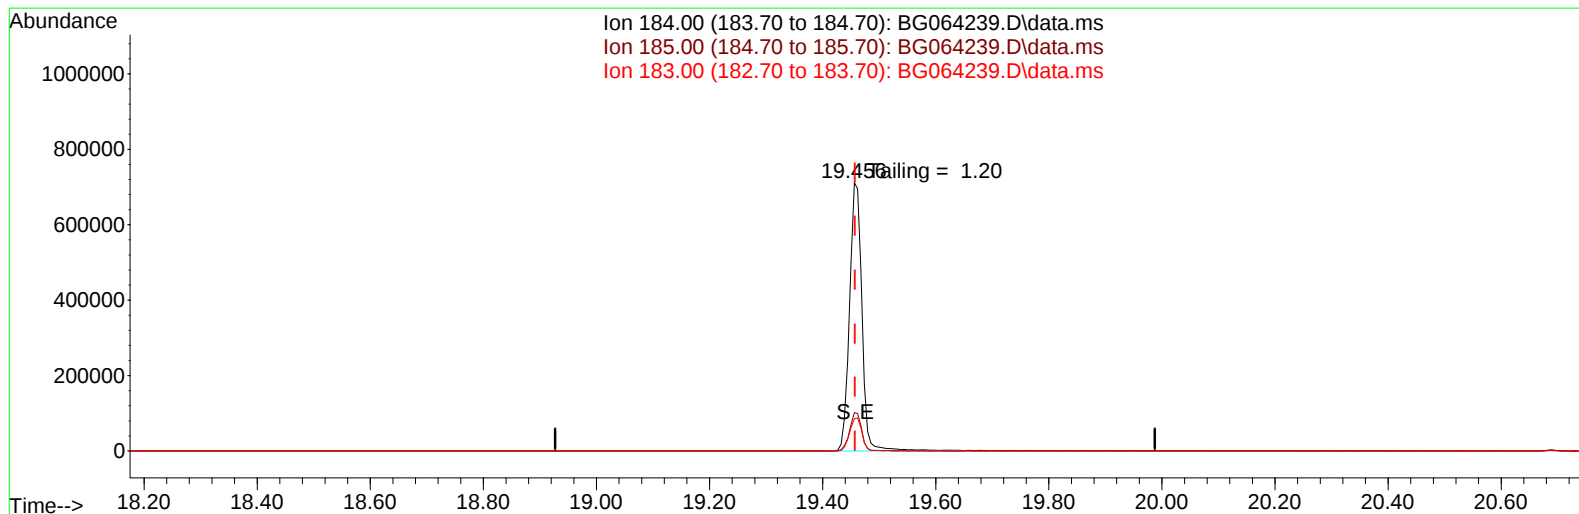

TIC: BG064239.D\data.ms

(77) Benzidine**19.456min (-0.001) 576729.23 ng****response 1079780**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.35
183.00	12.10	12.05
0.00	0.00	0.00