

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG090319\
 Data File : BG042686.D
 Acq On : 3 Sep 2019 13:22
 Operator : HP/JU
 Sample : PB122722BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB122722BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.556	413	420	434	rBV	431999	703336	24.15%	5.990%
2	7.160	686	693	703	rBV	432762	756989	25.99%	6.447%
3	7.530	748	756	766	rBV	479716	816978	28.05%	6.958%
4	7.994	826	835	845	rBV	92544	158498	5.44%	1.350%
5	8.323	883	891	900	rBV	393088	689162	23.66%	5.869%
6	9.164	1027	1034	1050	rBV	247509	475312	16.32%	4.048%
7	10.820	1308	1316	1335	rBV	101307	217737	7.48%	1.854%
8	13.276	1726	1734	1757	rBV	941259	1565129	53.74%	13.330%
9	14.657	1963	1969	1981	rBV	212982	365253	12.54%	3.111%
10	16.149	2216	2223	2248	rBV	714940	1313663	45.11%	11.188%
11	17.413	2431	2438	2452	rBV2	277691	483487	16.60%	4.118%
12	20.021	2876	2882	2896	rBV	2153326	2912188	100.00%	24.803%
13	21.684	3158	3165	3179	rBV	327089	610846	20.98%	5.202%
14	24.933	3704	3718	3736	rBV2	194582	672925	23.11%	5.731%


Sum of corrected areas: 11741503

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG090319\
Data File : BG042686.D
Acq On : 3 Sep 2019 13:22
Operator : HP/JU
Sample : PB122722BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB122722BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

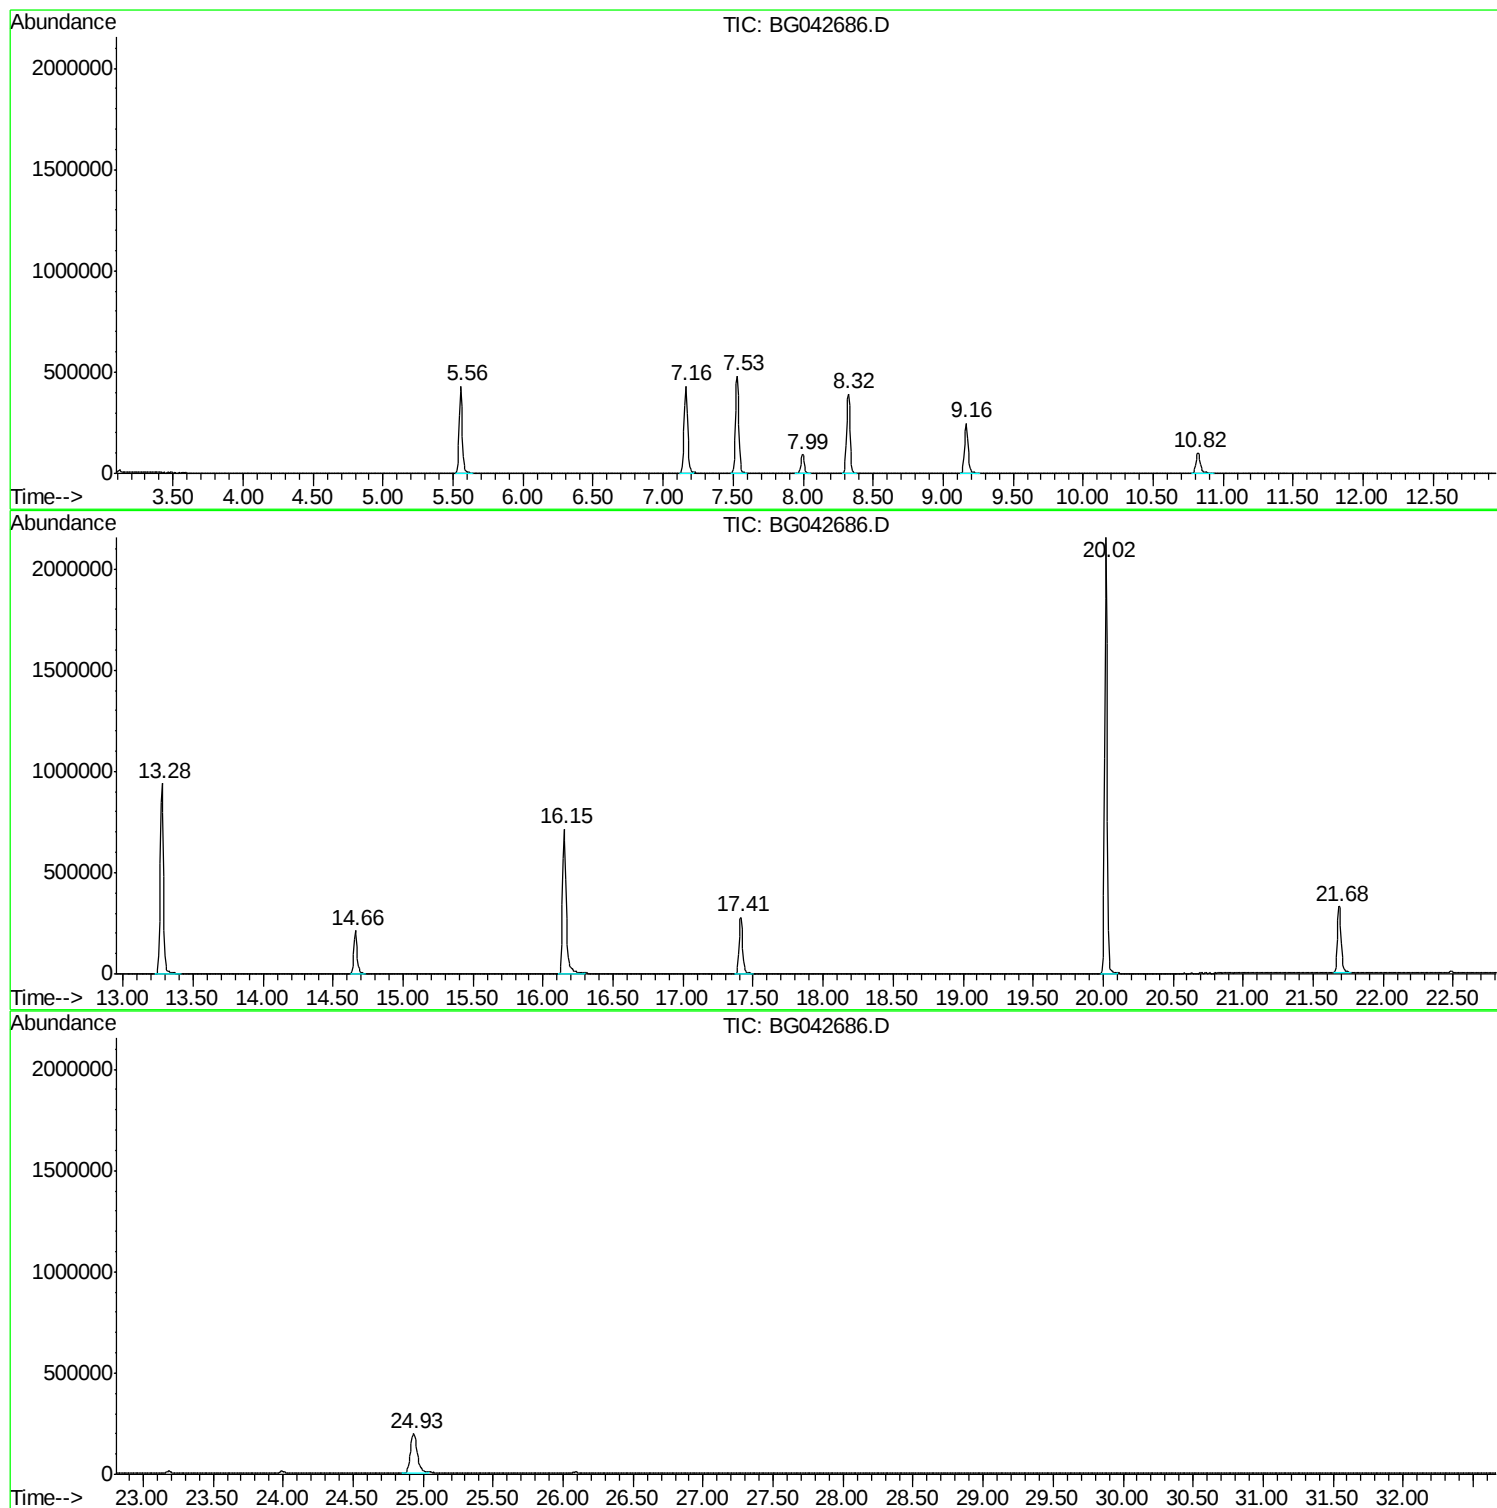

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG090319\
Data File : BG042686.D
Acq On : 3 Sep 2019 13:22
Operator : HP/JU
Sample : PB122722BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB122722BL









Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.53 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.53	103.09 ng	816978	1,4-Dichlorobenzene-d4	7.99

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	35
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	25
3		Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	16
4		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
5		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9

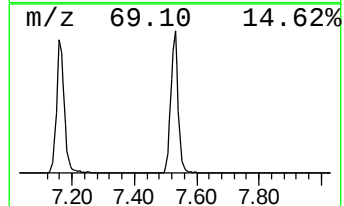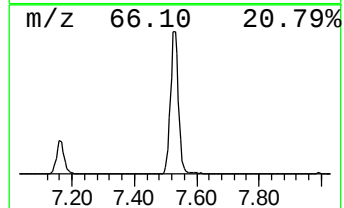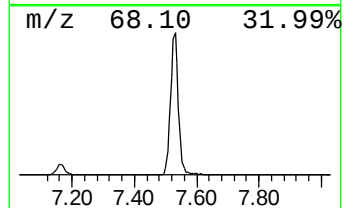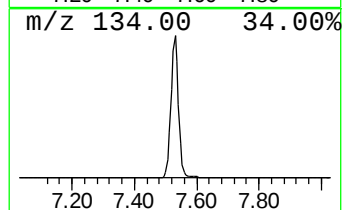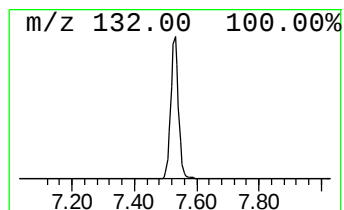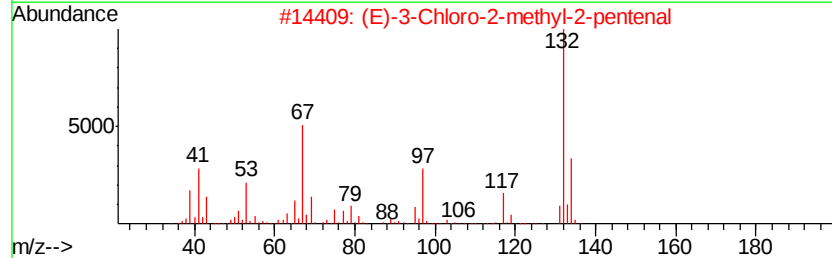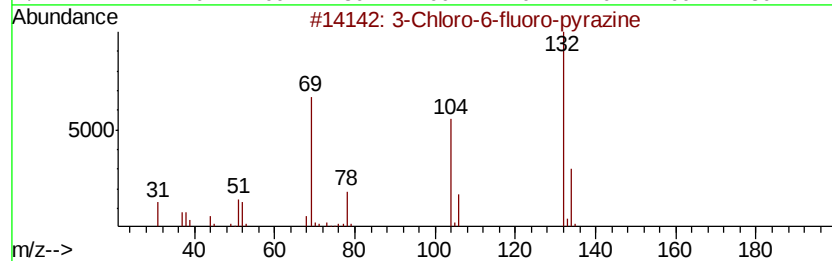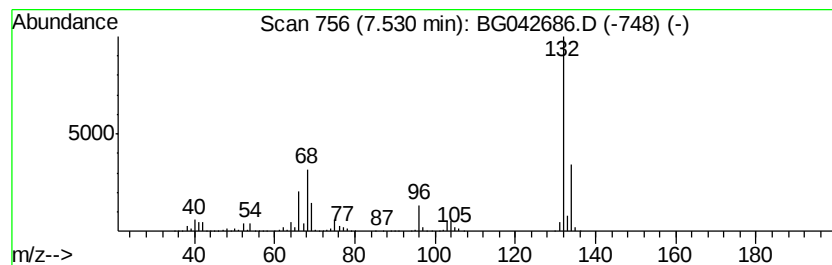

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG090319\
Data File : BG042686.D
Acq On : 3 Sep 2019 13:22
Operator : HP/JU
Sample : PB122722BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB122722BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.53	7.53	103.1	ng	816978	1	7.99	158498	20.0