


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG090319\
Data File : BG042682.D
Acq On : 3 Sep 2019 10:47
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082219.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Aug 22 14:29:15 2019

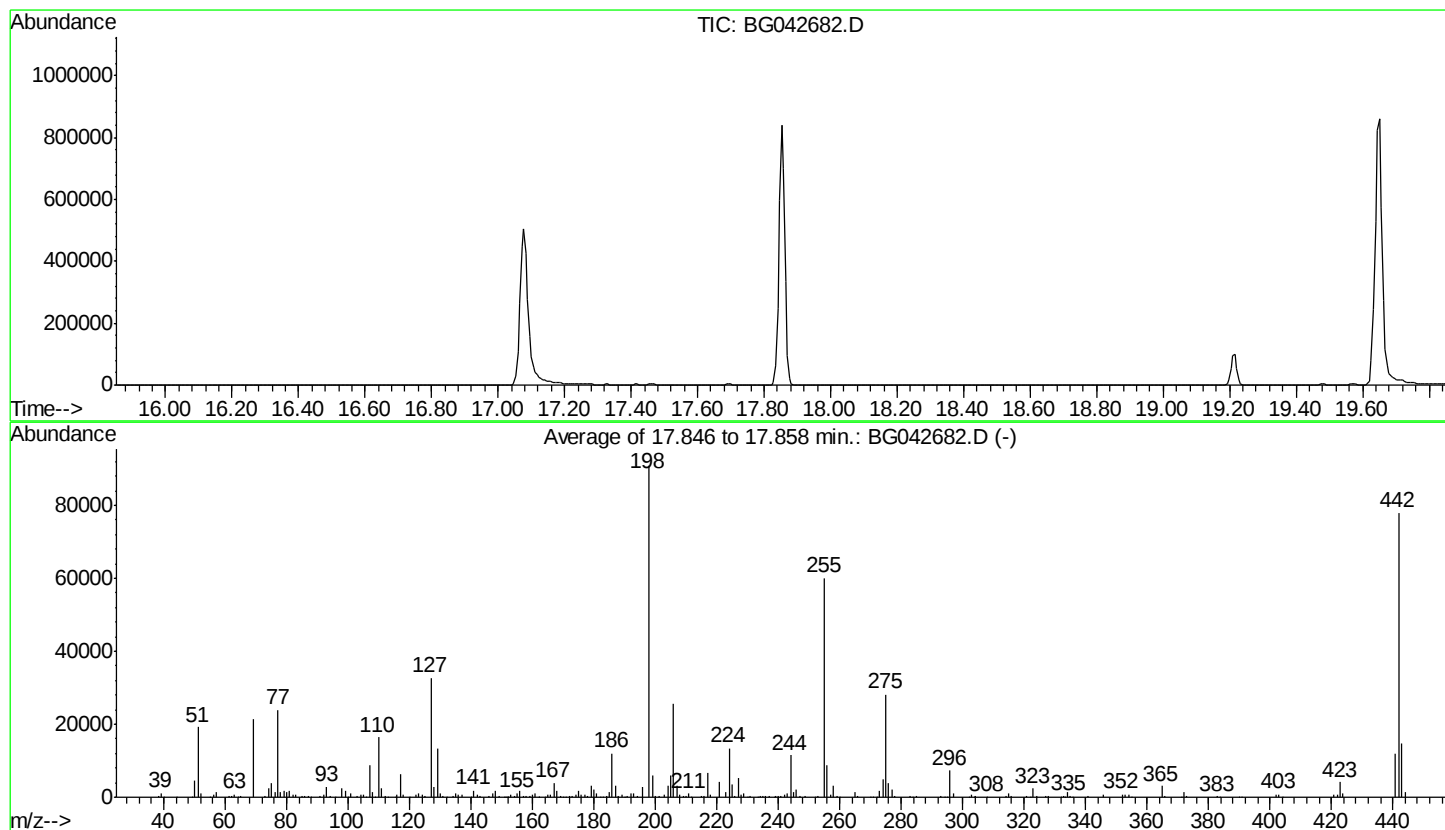

AutoFind: Scans 2512, 2513, 2514; Background Corrected with Scan 2505

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.1	19197	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	23.5	21386	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	35.9	32648	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	90850	PASS
199	198	5	9	6.7	6070	PASS
275	198	10	60	31.1	28218	PASS
365	198	1	100	3.4	3117	PASS
441	198	0.01	100	13.0	11829	PASS
442	198	50	100	85.8	77994	PASS
443	442	15	24	18.9	14764	PASS