
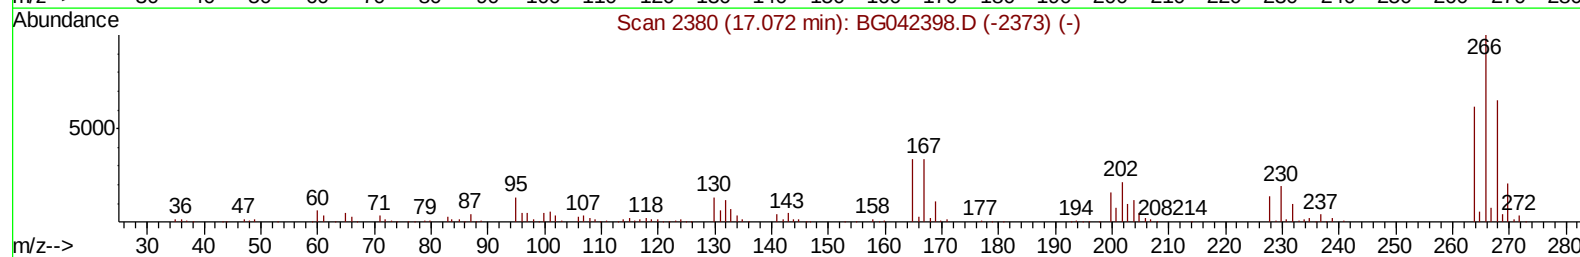
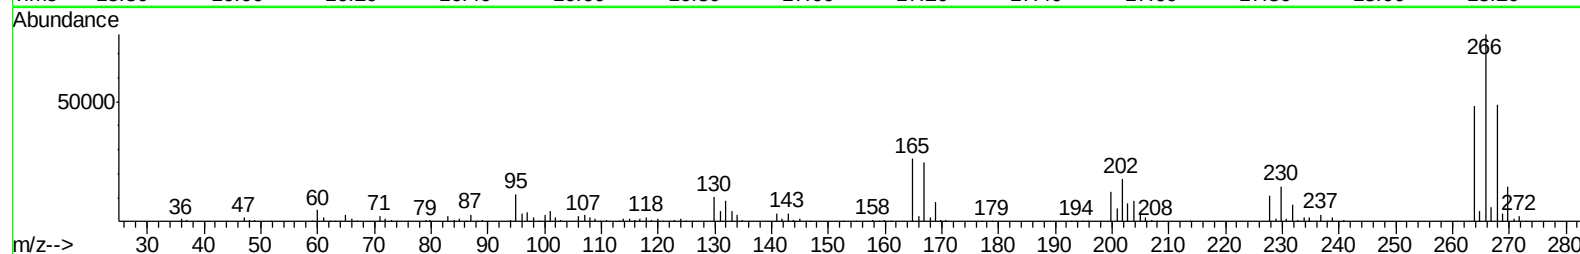


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG090419\
 Data File : BG042700.D
 Acq On : 4 Sep 2019 10:19
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 04 19:08:07 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082219.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 22 14:29:15 2019
 Response via : Initial Calibration

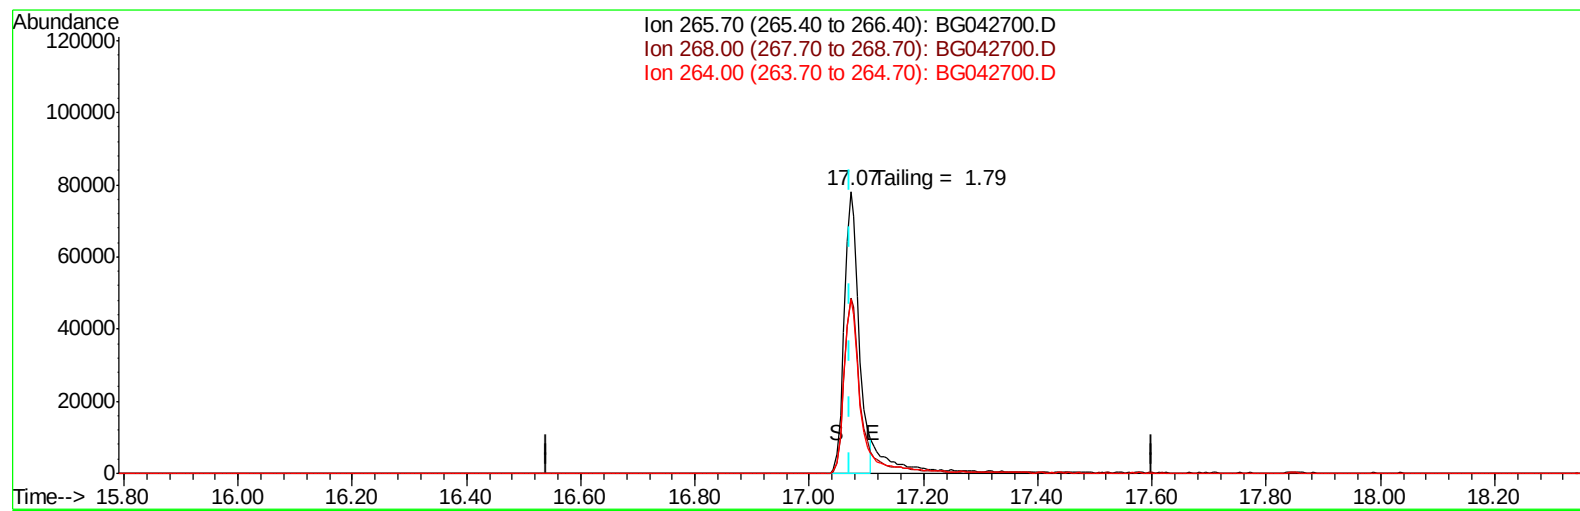

TIC: BG042700.D

(70) Pentachlorophenol (C)




17.072min (+0.000) 93468.41ng

response 158707

Ion	Exp%	Act%
265.70	100	100
268.00	65.10	62.46
264.00	61.80	61.90
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG090419\
 Data File : BG042700.D
 Acq On : 4 Sep 2019 10:19
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 04 19:08:07 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082219.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 22 14:29:15 2019
 Response via : Initial Calibration

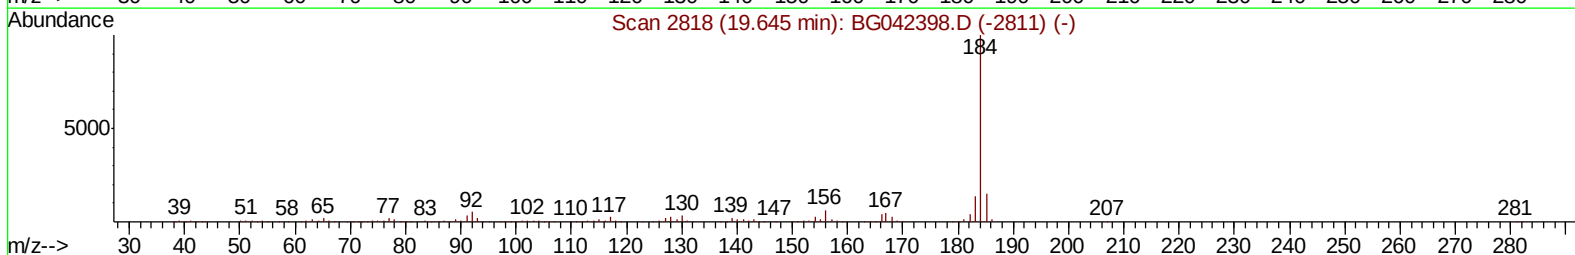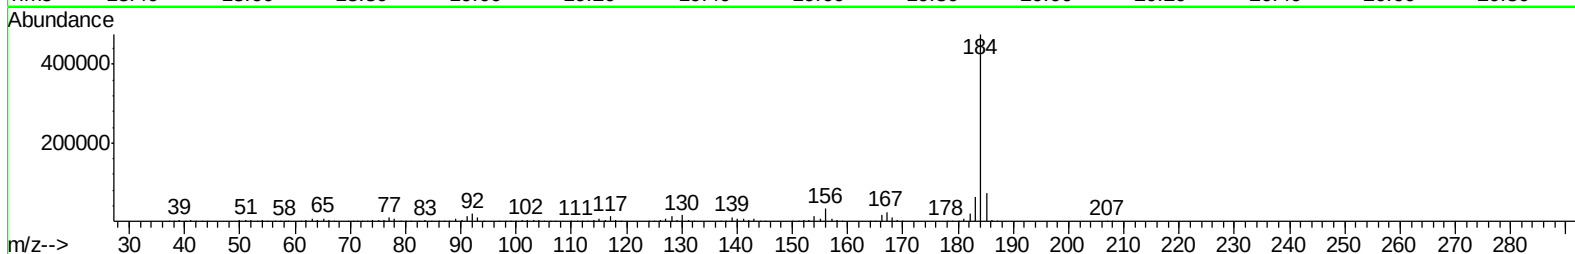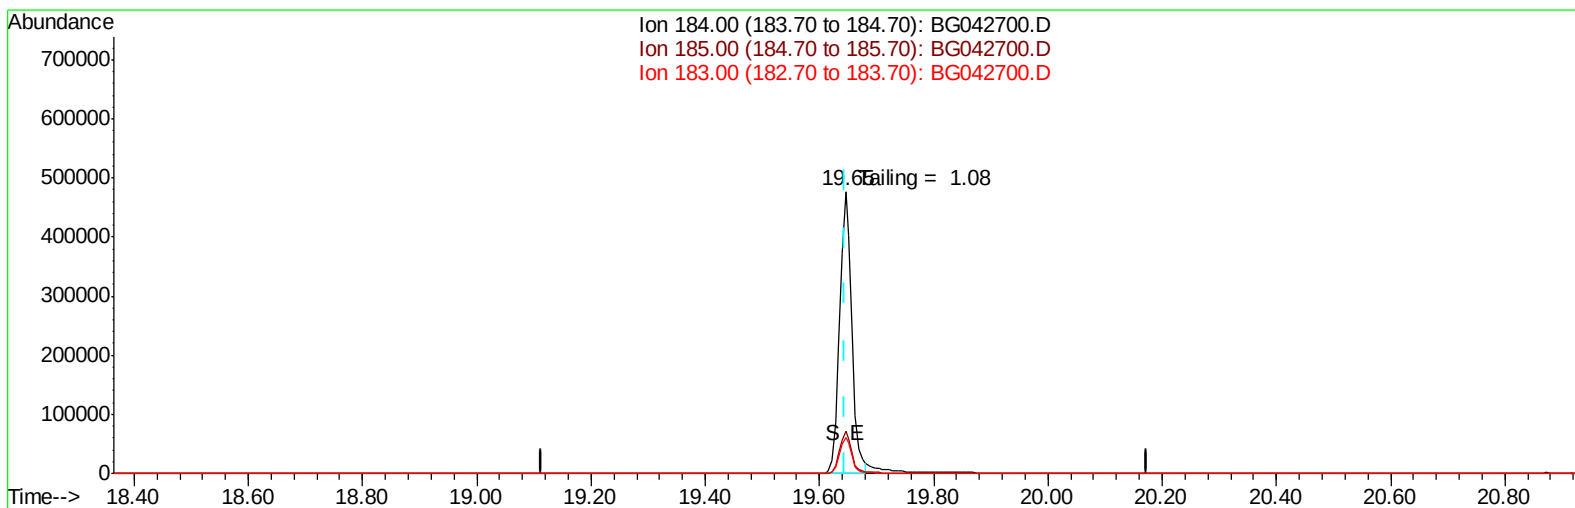

TIC: BG042700.D

(77) Benzidine

19.645min (+0.000) 46645.03ng

response 735533

Ion	Exp%	Act%
184.00	100	100
185.00	15.30	14.79
183.00	13.50	12.92
0.00	0.00	0.00