

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG090419\
 Data File : BG042706.D
 Acq On : 4 Sep 2019 14:08
 Operator : HP/JU
 Sample : PB122759BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB122759BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.555	413	420	435	rBV	432098	710074	25.36%	6.070%
2	7.165	686	694	708	rBV	424488	754160	26.93%	6.447%
3	7.529	748	756	773	rBV	466905	814032	29.07%	6.958%
4	7.999	828	836	846	rVB	108833	183698	6.56%	1.570%
5	8.323	883	891	902	rBV	397124	692939	24.75%	5.923%
6	9.169	1027	1035	1047	rBV	236682	458484	16.37%	3.919%
7	10.820	1309	1316	1334	rBV	117308	241906	8.64%	2.068%
8	13.276	1727	1734	1755	rBV	906649	1480379	52.87%	12.654%
9	14.662	1963	1970	1984	rBV	220323	397167	14.18%	3.395%
10	16.155	2217	2224	2250	rBV	661613	1223843	43.71%	10.461%
11	17.412	2431	2438	2454	rBV2	320761	532972	19.03%	4.556%
12	20.021	2876	2882	2897	rBV	2042750	2800213	100.00%	23.936%
13	21.689	3159	3166	3180	rBV	382372	688141	24.57%	5.882%
14	24.938	3708	3719	3742	rBV2	217925	720676	25.74%	6.160%


Sum of corrected areas: 11698684

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG090419\
Data File : BG042706.D
Acq On : 4 Sep 2019 14:08
Operator : HP/JU
Sample : PB122759BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB122759BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

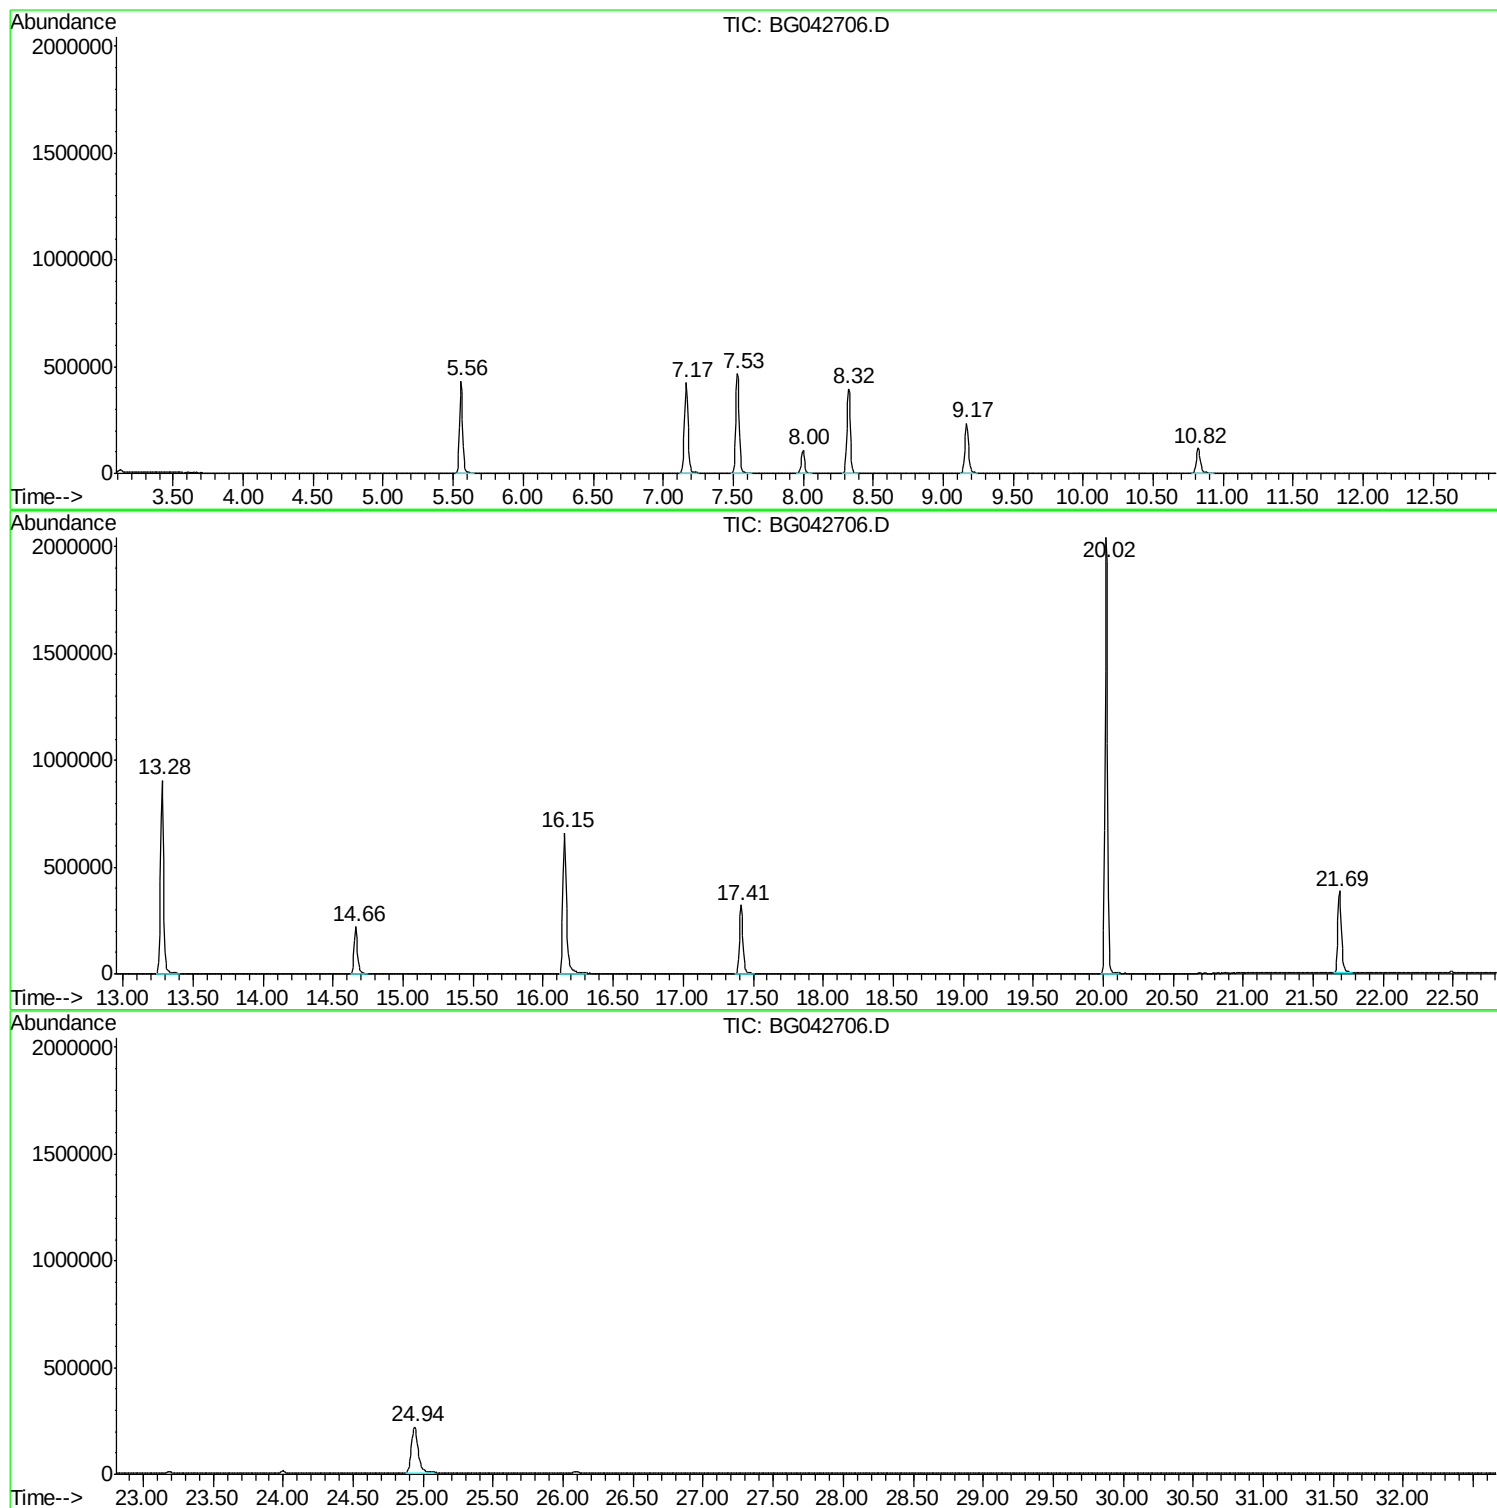

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG090419\
Data File : BG042706.D
Acq On : 4 Sep 2019 14:08
Operator : HP/JU
Sample : PB122759BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB122759BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.53 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.53	88.63 ng	814032	1,4-Dichlorobenzene-d4	8.00

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	38
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	25
3		Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	12
4		5-Aminoindole	132	C8H8N2	005192-03-0	12
5		2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	9

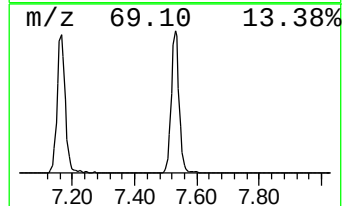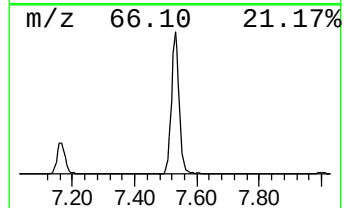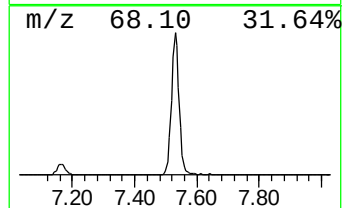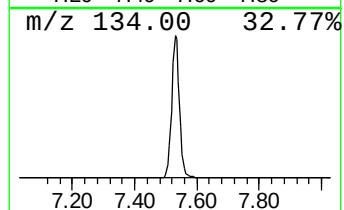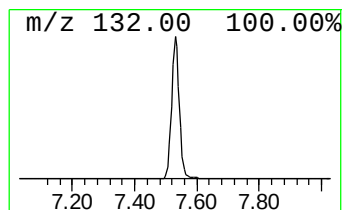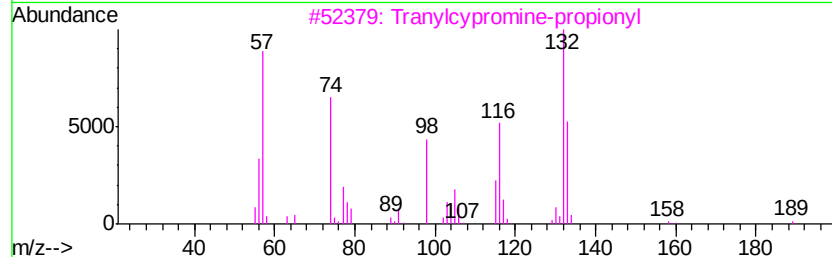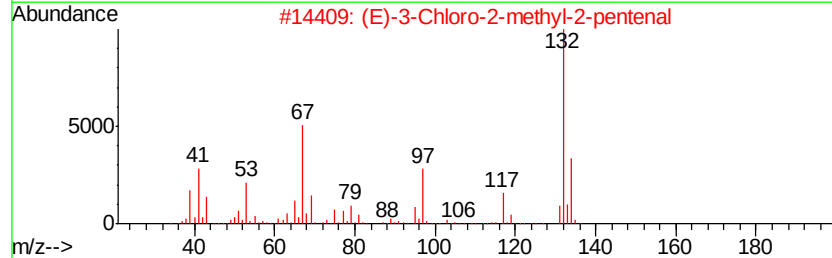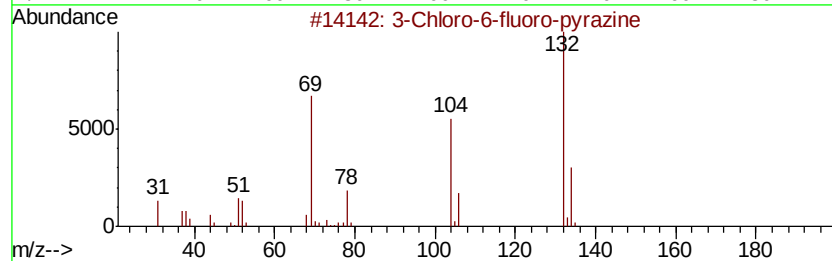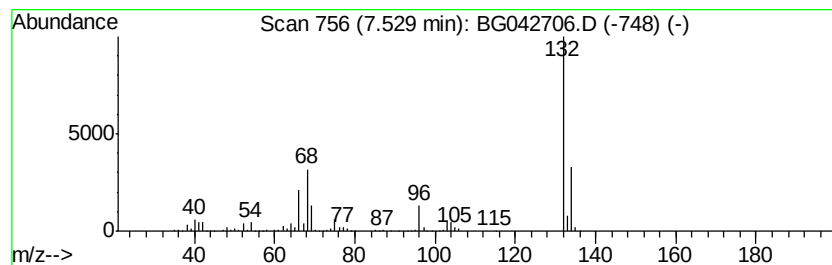

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG090419\
Data File : BG042706.D
Acq On : 4 Sep 2019 14:08
Operator : HP/JU
Sample : PB122759BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB122759BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.53	7.53	88.6	ng	814032	1	8.00	183698	20.0