
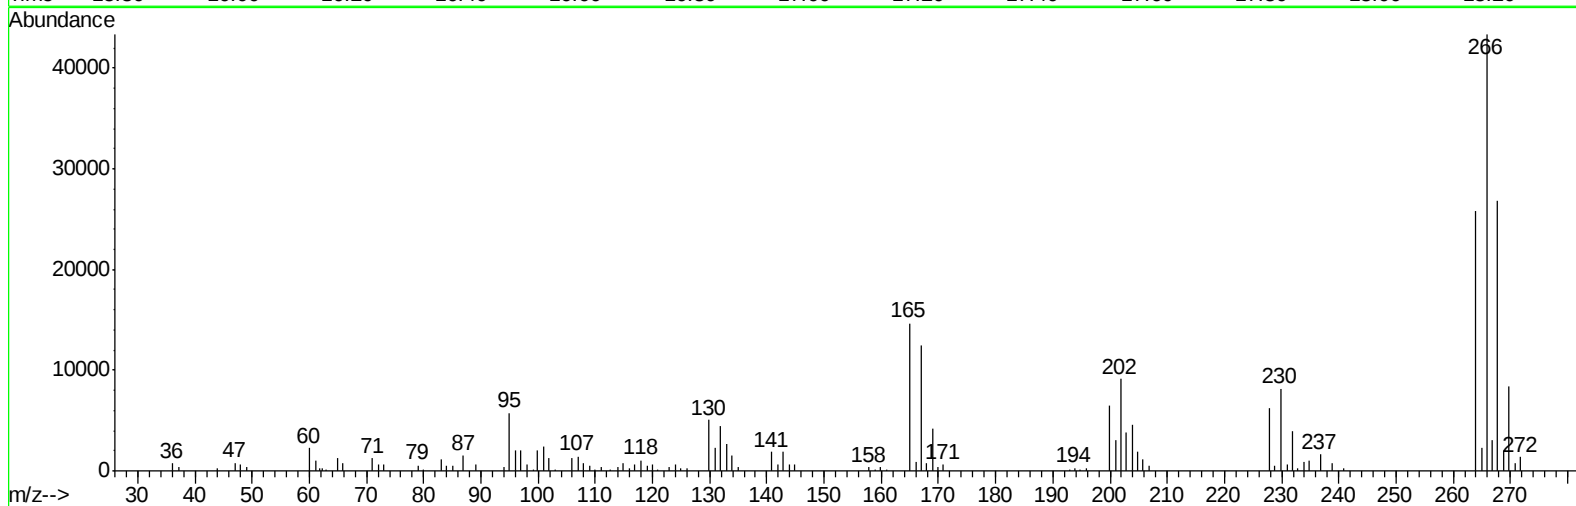


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG090519\  
Data File : BG042718.D  
Acq On : 5 Sep 2019 13:38  
Operator : HP/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 06 09:20:45 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082219.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Aug 22 14:29:15 2019  
Response via : Initial Calibration

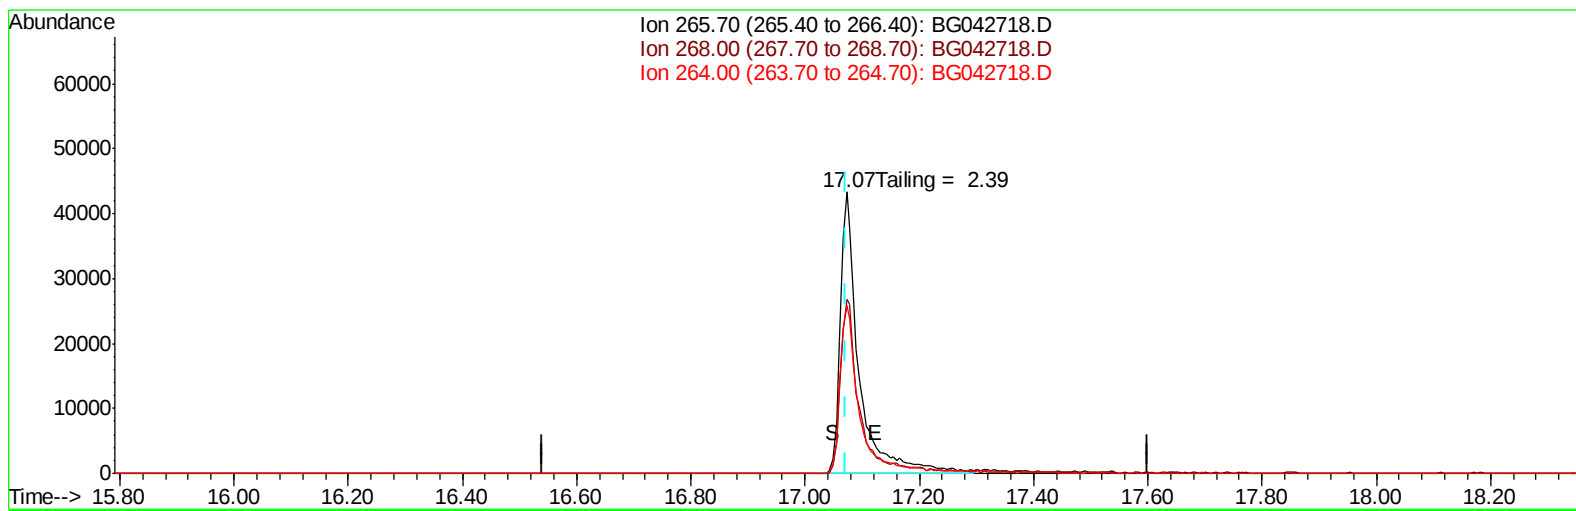

TIC: BG042718.D

(70) Pentachlorophenol (C)

17.072min (+0.000) 90072.21ng

response 97443

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 65.10 | 61.90 |
| 264.00 | 61.80 | 59.50 |
| 0.00   | 0.00  | 0.00  |