
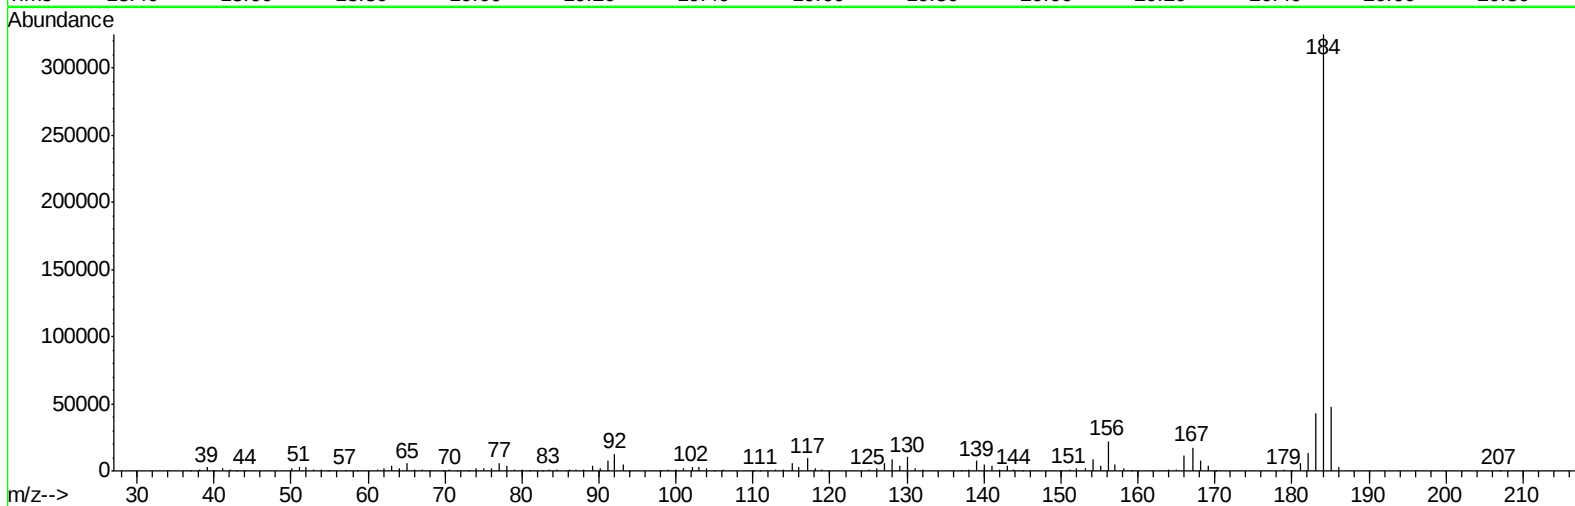


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG090519\
Data File : BG042718.D
Acq On : 5 Sep 2019 13:38
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 06 09:20:45 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 22 14:29:15 2019
Response via : Initial Calibration

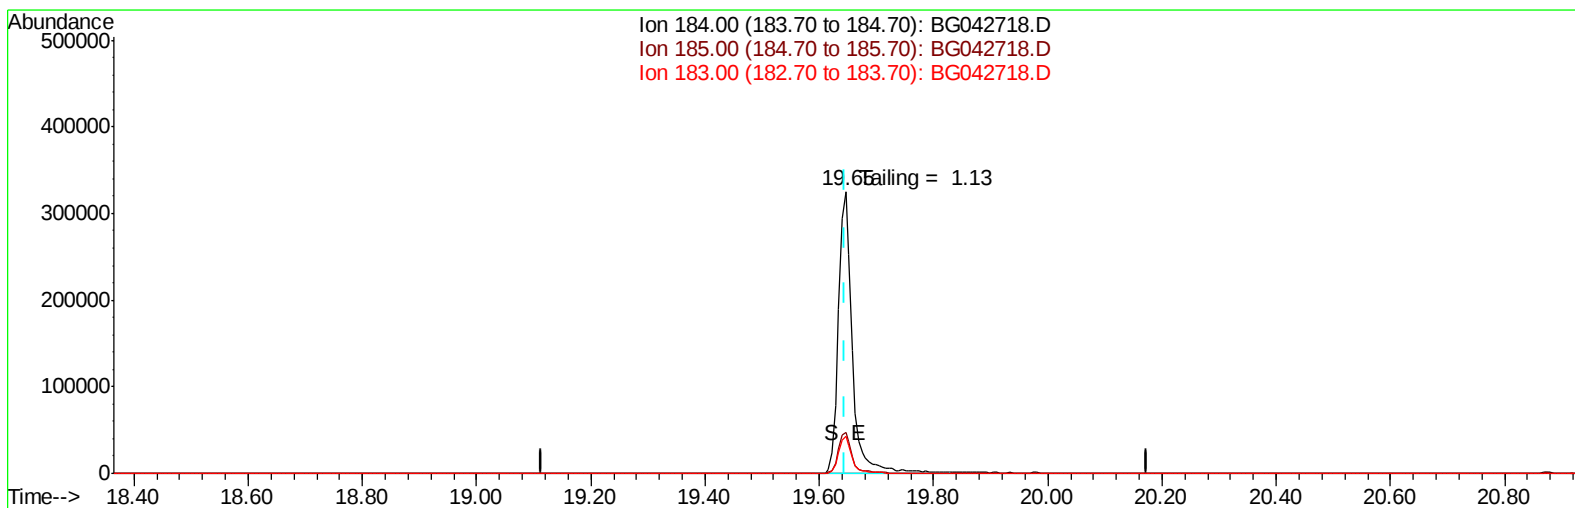

TIC: BG042718.D

(77) Benzidine



19.646min (+0.000) 86654.17ng

response 549055

Ion	Exp%	Act%
184.00	100	100
185.00	15.30	14.76
183.00	13.50	13.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG090519\
Data File : BG042718.D
Acq On : 5 Sep 2019 13:38
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 06 09:20:45 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 22 14:29:15 2019
Response via : Initial Calibration

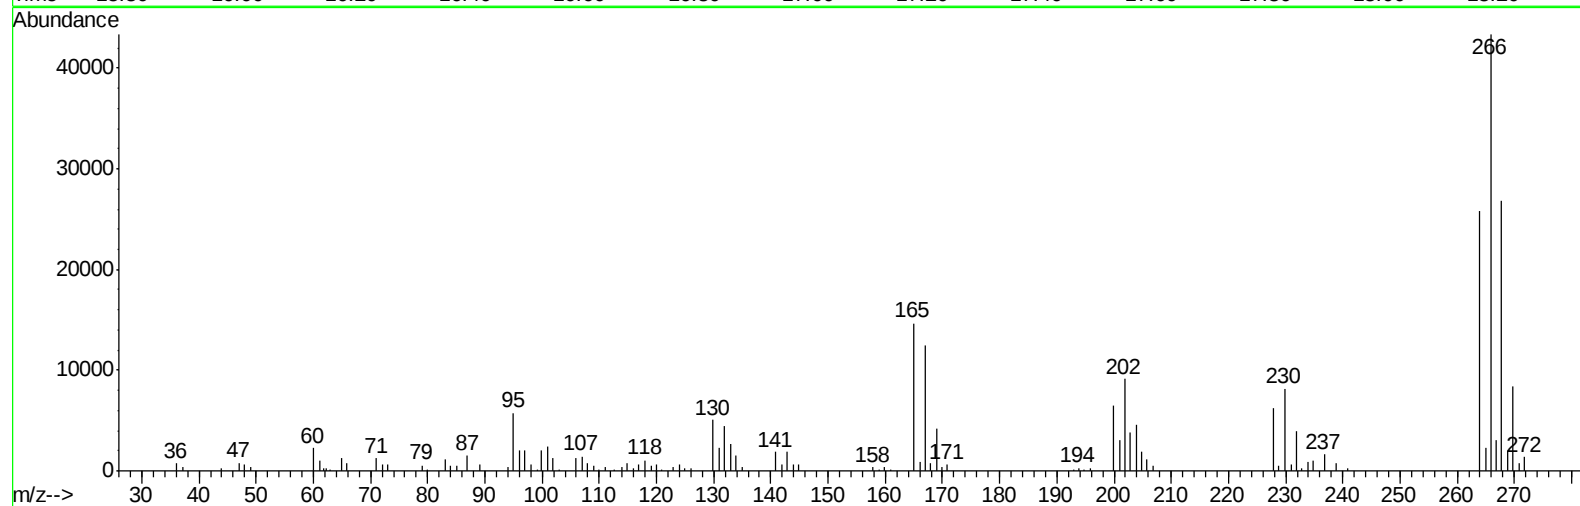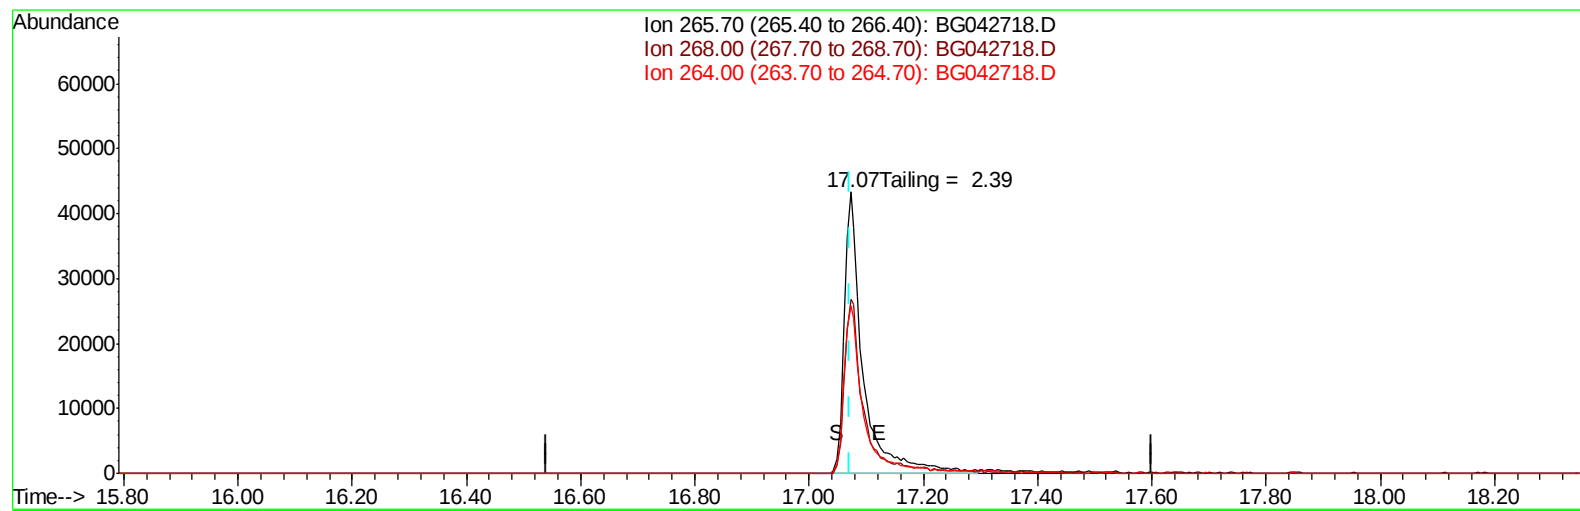

TIC: BG042718.D

(70) Pentachlorophenol (C)

17.072min (+0.000) 90072.21ng

response 97443

Ion	Exp%	Act%
265.70	100	100
268.00	65.10	61.90
264.00	61.80	59.50
0.00	0.00	0.00