
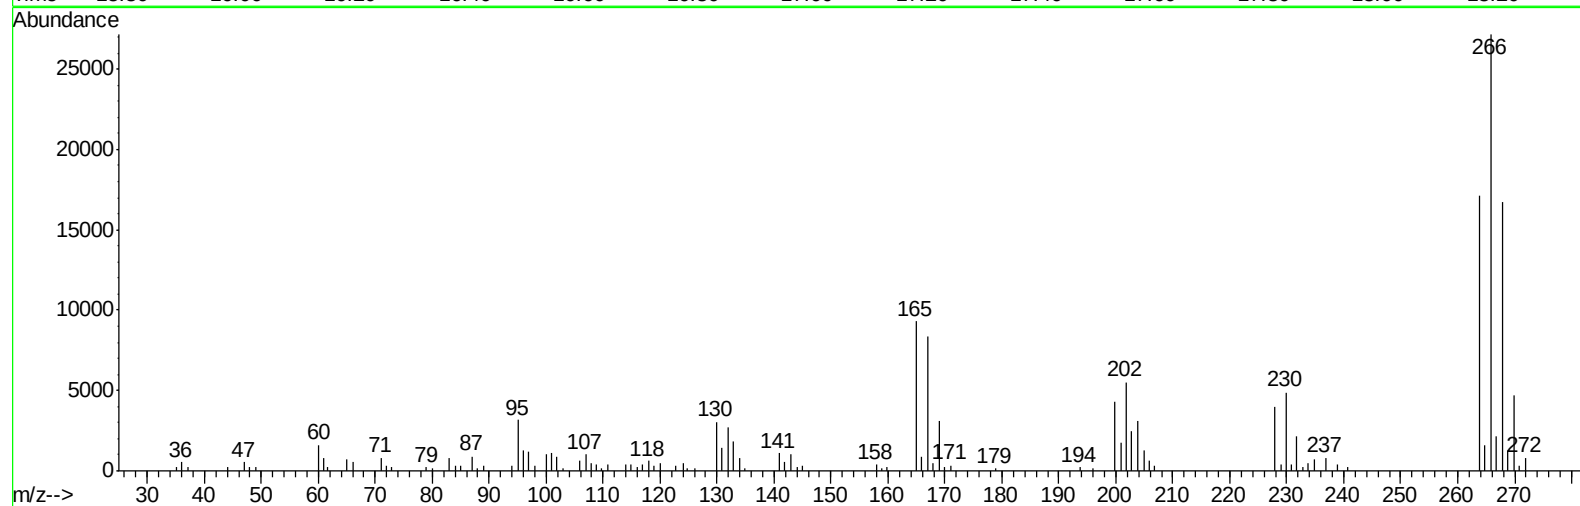


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG090519\
Data File : BG042736.D
Acq On : 6 Sep 2019 2:24
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 06 09:21:39 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 22 14:29:15 2019
Response via : Initial Calibration

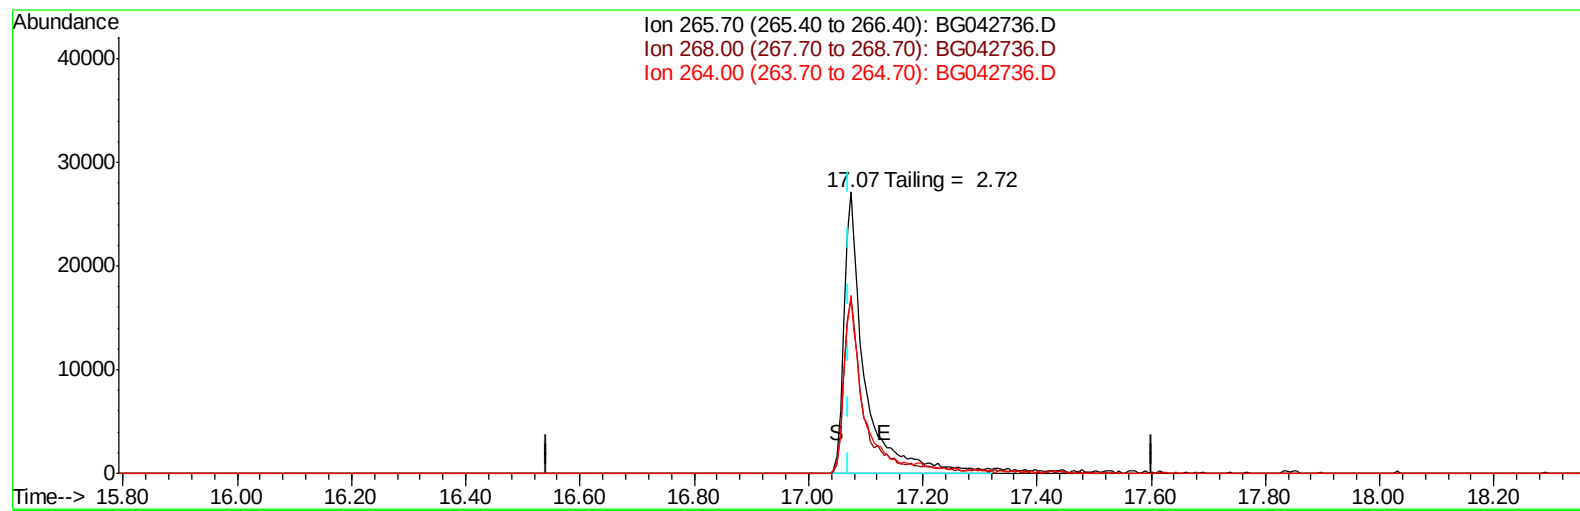

TIC: BG042736.D

(70) Pentachlorophenol (C)



17.073min (+0.002) 36214.21ng

response 66161

Ion	Exp%	Act%
265.70	100	100
268.00	65.10	61.62
264.00	61.80	63.06
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG090519\
Data File : BG042736.D
Acq On : 6 Sep 2019 2:24
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 06 09:21:39 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 22 14:29:15 2019
Response via : Initial Calibration

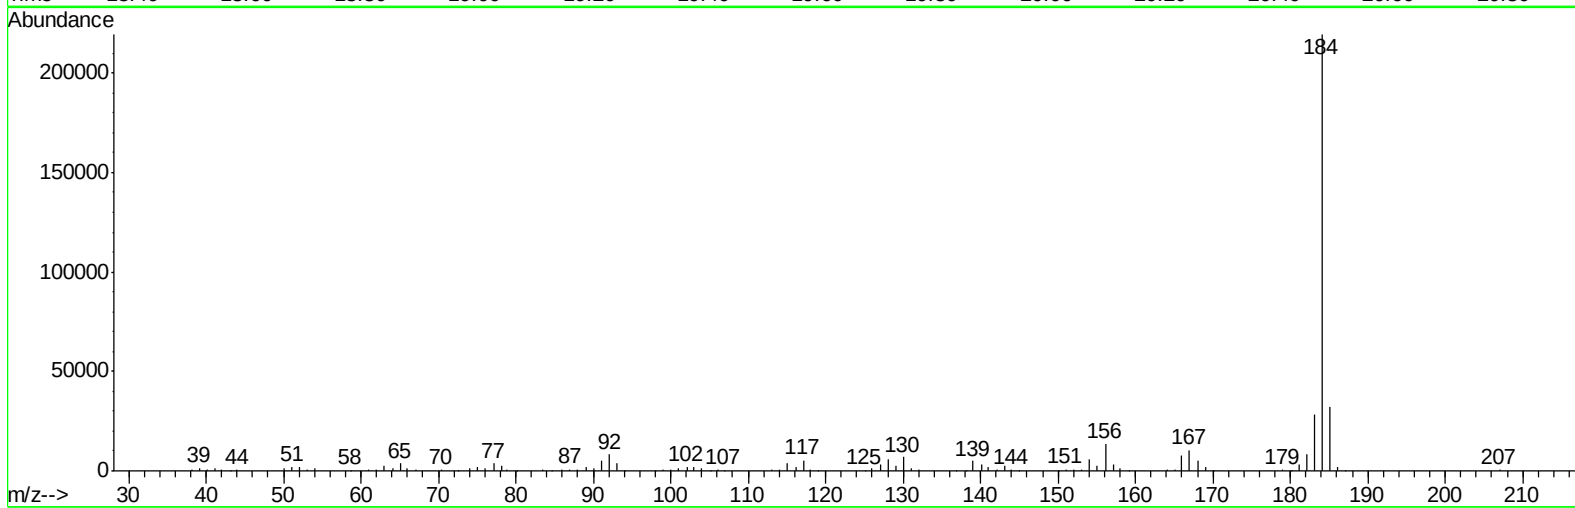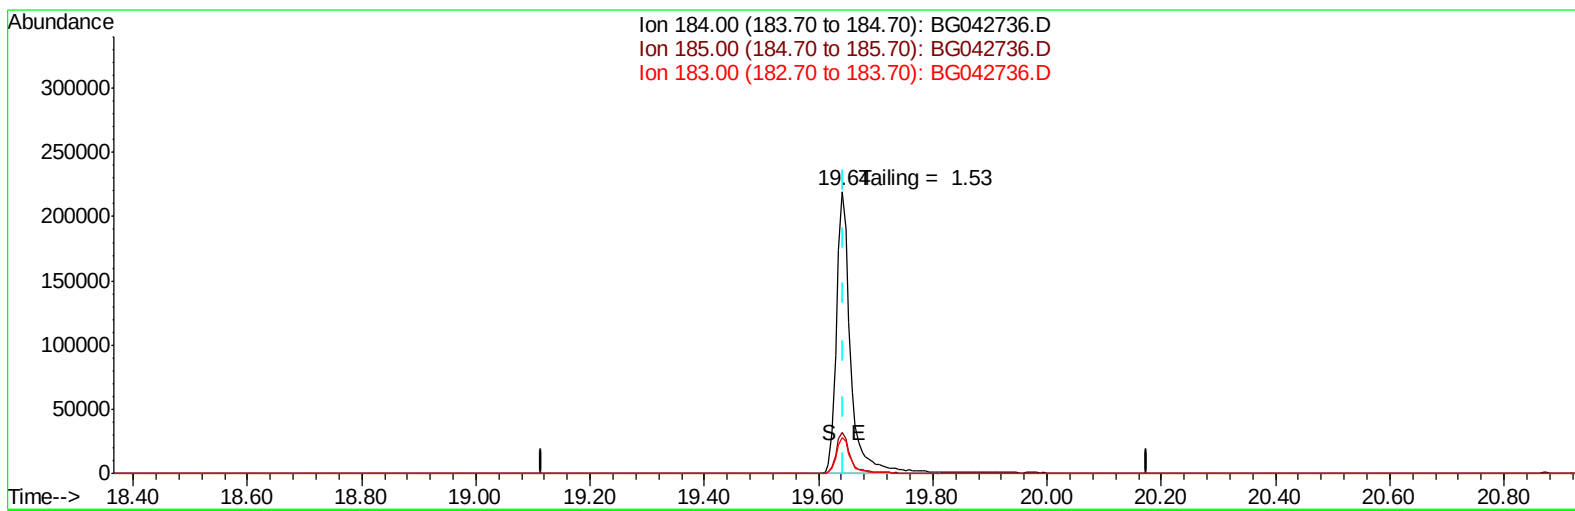

TIC: BG042736.D

(77) Benzidine

19.641min (-0.004) 107550.71ng

response 376190

Ion	Exp%	Act%
184.00	100	100
185.00	15.30	14.77
183.00	13.50	12.88
0.00	0.00	0.00