

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG090519\
 Data File : BG042732.D
 Acq On : 5 Sep 2019 22:35
 Operator : HP/JU
 Sample : K4695-20
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 T5-1-4-(0-2.5)

Quant Time: Sep 06 07:29:42 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082219.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 22 14:29:15 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.99	152	29230	20.00	ng	-0.01
21) Naphthalene-d8	10.82	136	103458	20.00	ng	0.00
39) Acenaphthene-d10	14.66	164	75175	20.00	ng	0.00
64) Phenanthrene-d10	17.41	188	187055	20.00	ng	0.00
76) Chrysene-d12	21.69	240	226286	20.00	ng	0.00
87) Perylene-d12	24.93	264	261819	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.56	112	181842	125.99	ng	0.00
7) Phenol-d6	7.16	99	213271	109.40	ng	-0.01
23) Nitrobenzene-d5	9.16	82	147363	98.43	ng	-0.01
42) 2,4,6-Tribromophenol	16.16	330	171661	160.66	ng	0.00
45) 2-Fluorobiphenyl	13.28	172	493556	111.04	ng	0.00
79) Terphenyl-d14	20.02	244	1122522	107.24	ng	0.00


Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG090519\
Data File : BG042732.D
Acq On : 5 Sep 2019 22:35
Operator : HP/JU
Sample : K4695-20
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
T5-1-4-(0-2.5)

Quant Time: Sep 06 07:29:42 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 22 14:29:15 2019
Response via : Initial Calibration

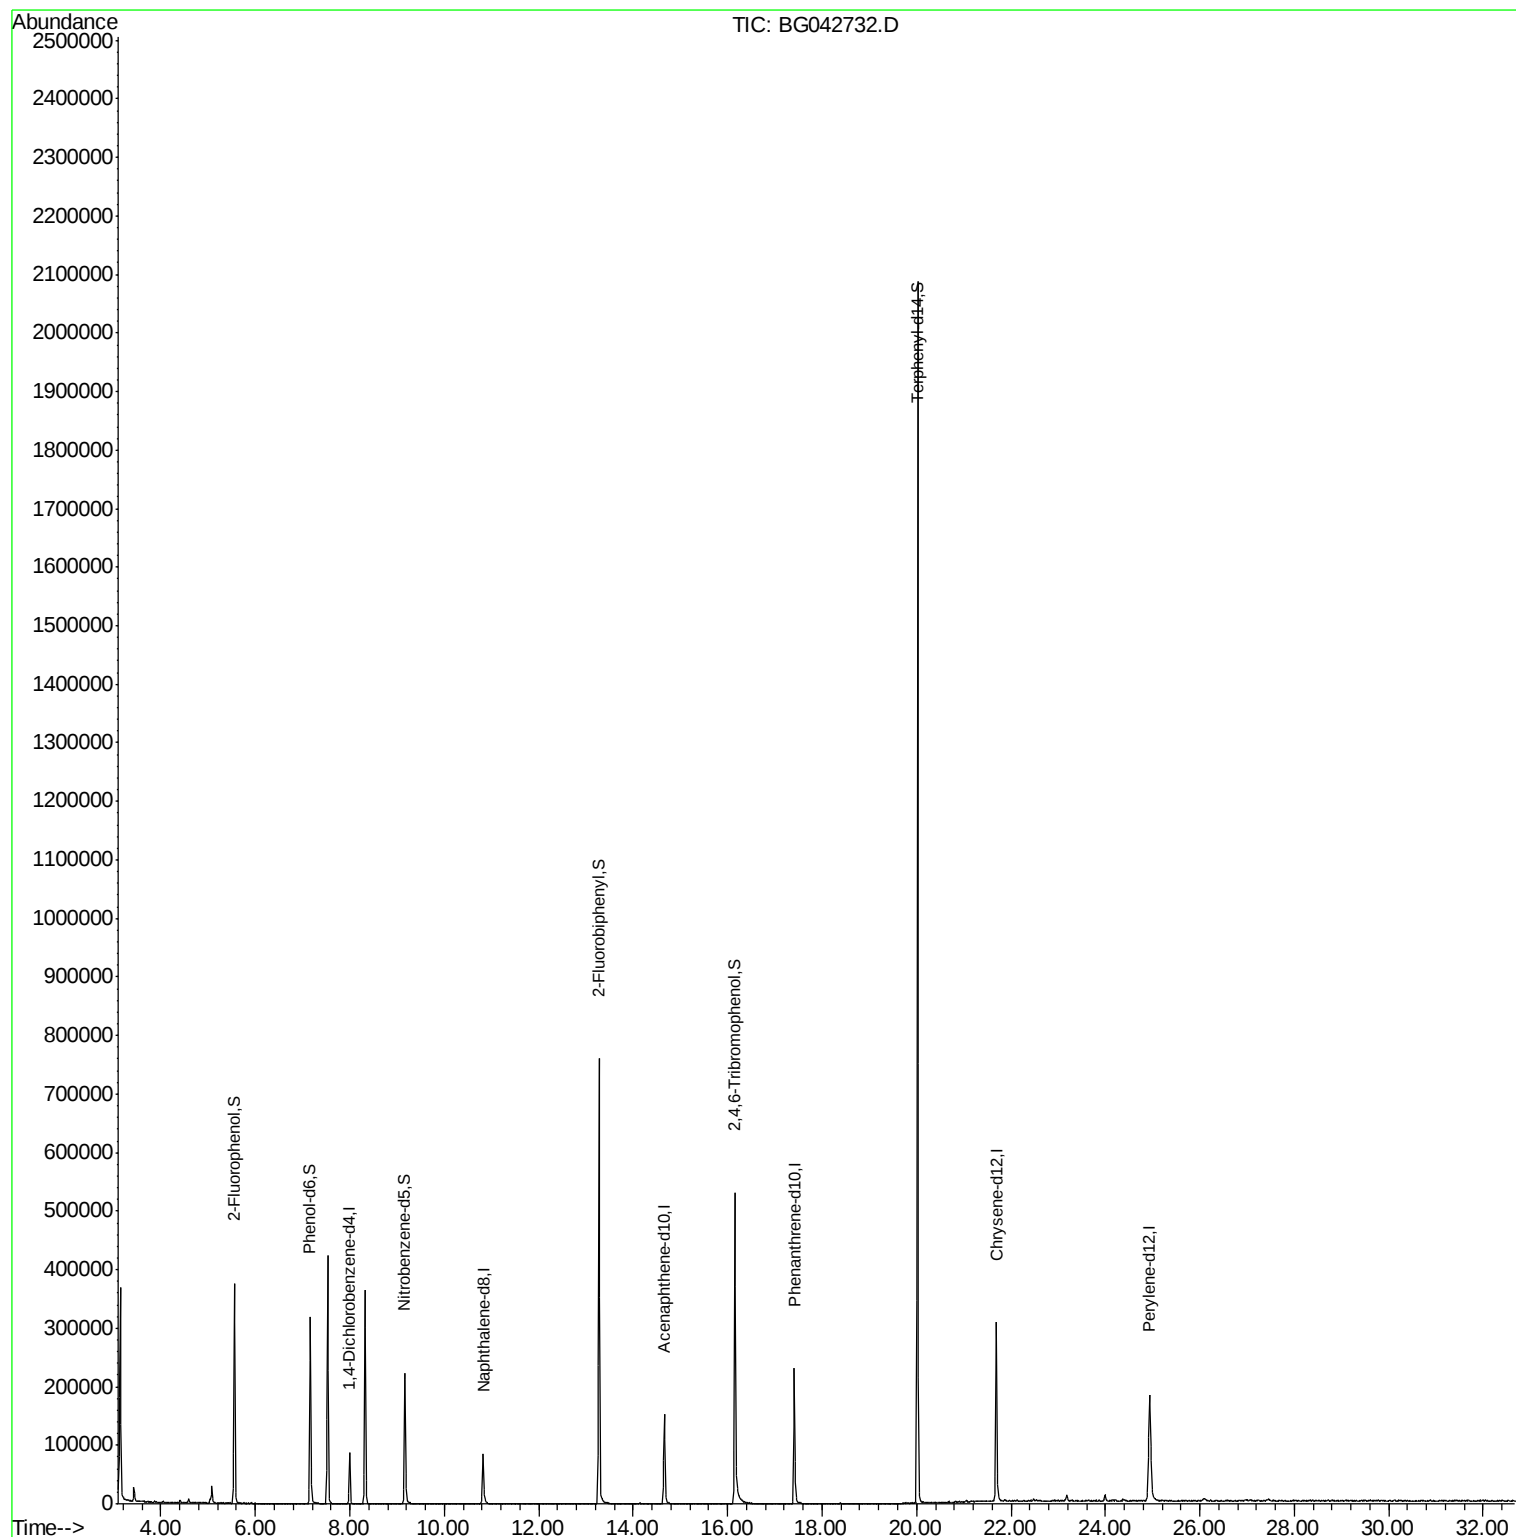




#1



1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 7.99 min Scan# 835
 Delta R.T. -0.01 min
 Lab File: BG042732.D
 Acq: 5 Sep 2019 22:35

Instrument :
 BNA_G
 ClientSampleId :
 T5-1-4-(0-2.5)

Tot Ion	Ratio	Lower	Upper
152	100		
150	159.7	125.4	188.0
115	49.9	38.5	57.7

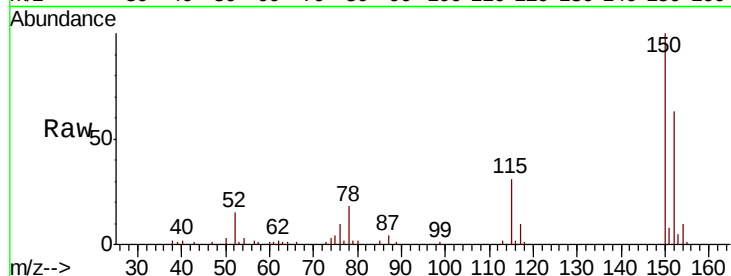


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

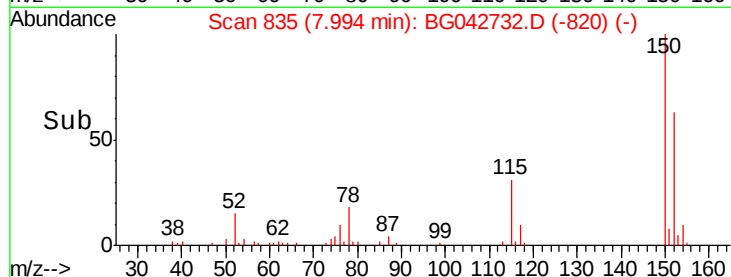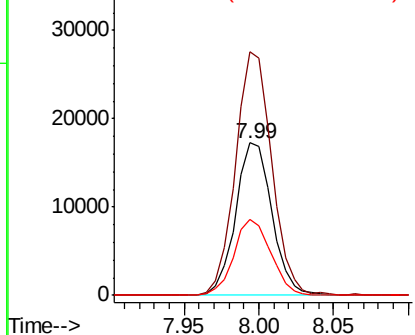



#5

2-Fluorophenol
 Concen: 125.995 ng
 RT: 5.56 min Scan# 420
 Delta R.T. -0.01 min
 Lab File: BG042732.D
 Acq: 5 Sep 2019 22:35

Tgt Ion	Ratio	Lower	Upper
112	100		
64	52.8	42.8	64.2
63	28.4	22.7	34.1

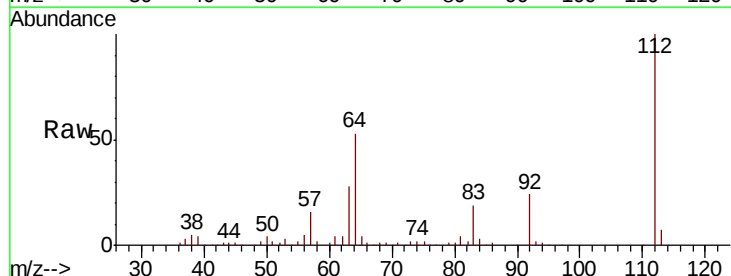

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BG
 Ion 63.00 (62.70 to 63.70): BG

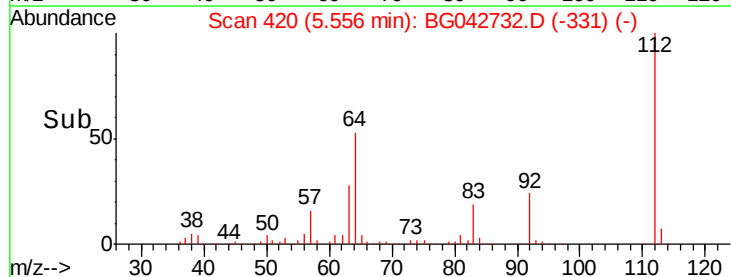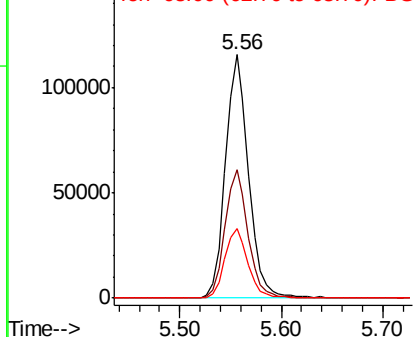



#7

Phenol-d6

Concen: 109.398 ng

RT: 7.16 min Scan# 693

Delta R.T. -0.01 min

Lab File: BG042732.D

Acq: 5 Sep 2019 22:35

Instrument :

BNA_G

ClientSampleId :

T5-1-4-(0-2.5)


Tot Ion: 99 Resp: 213271

Ion Ratio Lower Upper




99 100

42 15.3 12.0 18.0

71 35.4 26.3 39.5

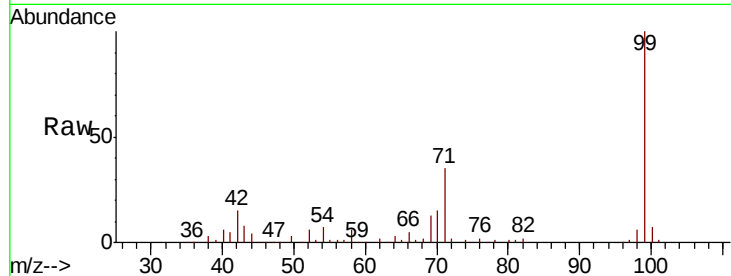

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

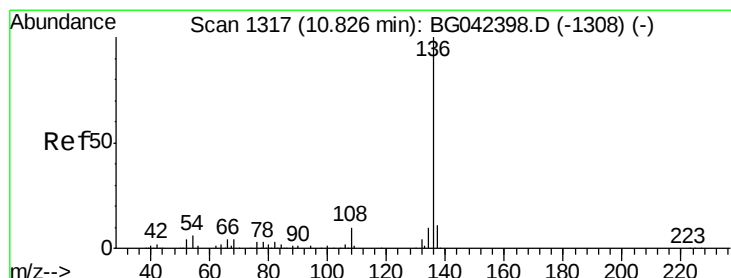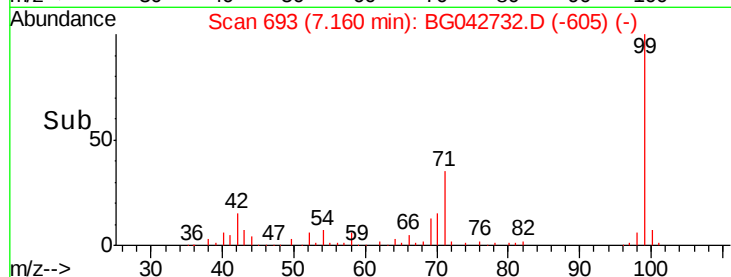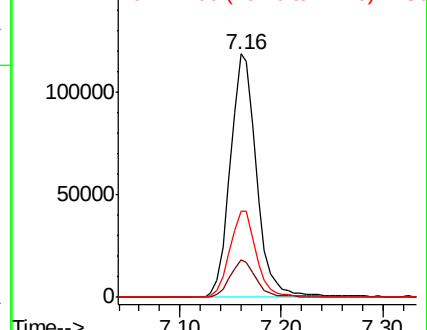

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.82 min Scan# 1316

Delta R.T. -0.01 min

Lab File: BG042732.D

Acq: 5 Sep 2019 22:35

Tgt Ion: 136 Resp: 103458


Ion Ratio Lower Upper

136 100



137 10.7 8.7 13.1


54 5.3 4.9 7.3

68 2.9 3.6 5.4#

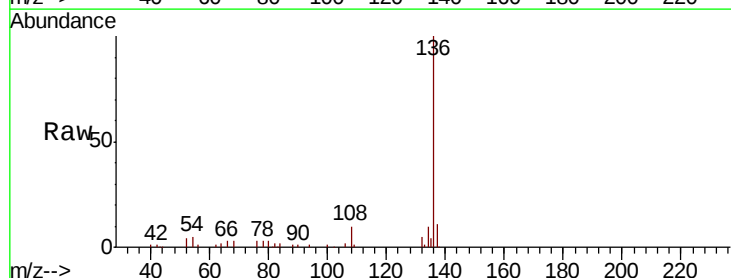

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

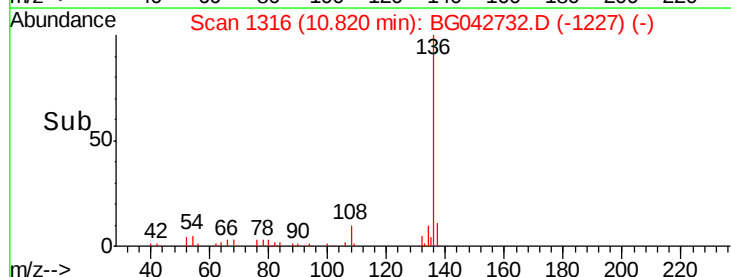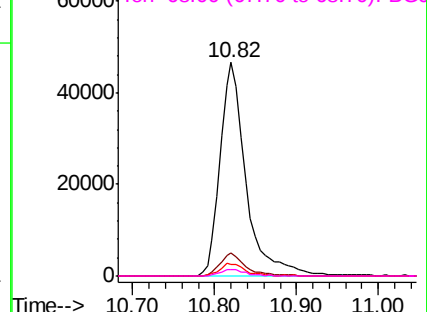


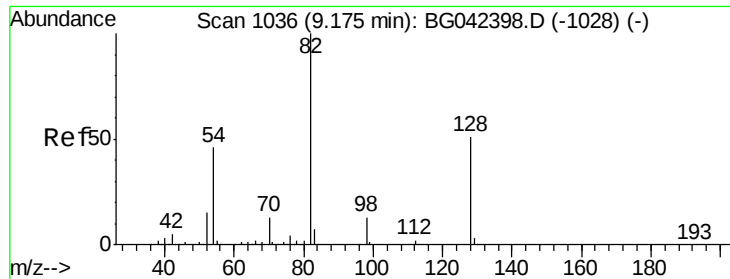

#23
Nitrobenzene-d5
Concen: 98.430 ng
RT: 9.16 min Scan# 1034
Delta R.T. -0.01 min
Lab File: BG042732.D
Acq: 5 Sep 2019 22:35

Instrument :
BNA_G
ClientSampleId :
T5-1-4-(0-2.5)

Tot Ion	82.00	Resp	147363
Ion Ratio	Lower	Upper	
82	100		
128	52.5	40.7	61.1
54	50.1	36.3	54.5


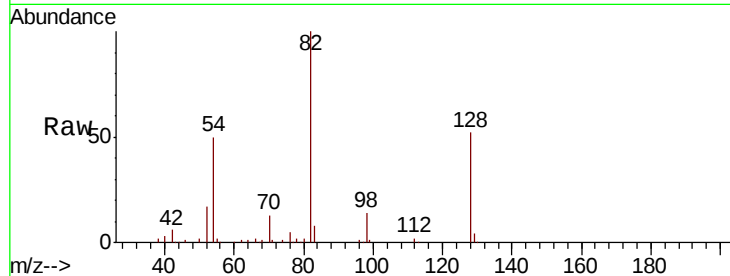


Abundance

Ion 82.00 (81.70 to 82.70): BGC


Ion 128.00 (127.70 to 128.70): BGC

Ion 54.00 (53.70 to 54.70): BGC

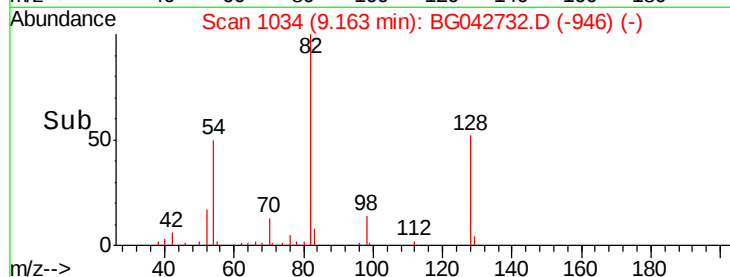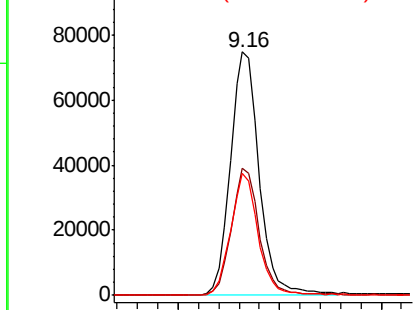

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.66 min Scan# 1969
Delta R.T. -0.01 min
Lab File: BG042732.D
Acq: 5 Sep 2019 22:35

Tgt Ion	164.00	Resp	75175
Ion Ratio	Lower	Upper	
164	100		
162	96.2	79.9	119.9
160	43.8	34.3	51.5


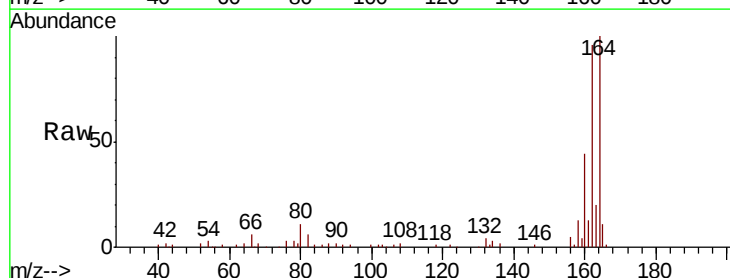



Abundance

Ion 164.00 (163.70 to 164.70): BGC

Ion 162.00 (161.70 to 162.70): BGC

Ion 160.00 (159.70 to 160.70): BGC

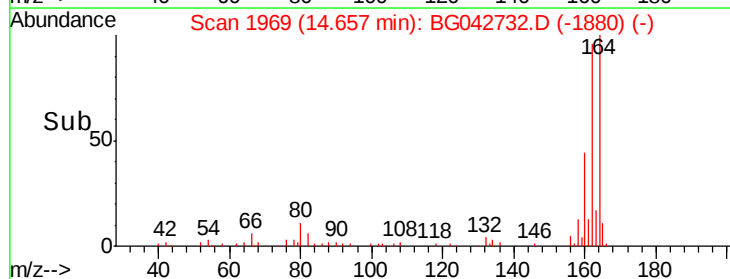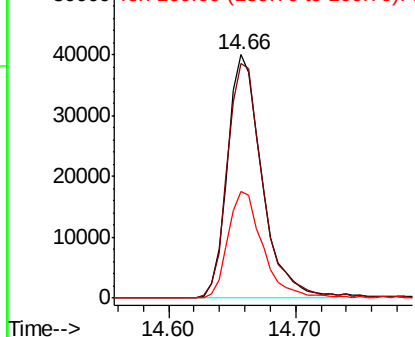

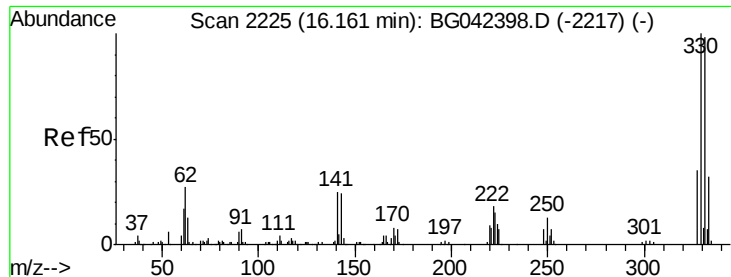

#42

2,4,6-Tribromophenol

Concen: 160.658 ng

RT: 16.16 min Scan# 2224

Delta R.T. -0.01 min

Lab File: BG042732.D

Acq: 5 Sep 2019 22:35

Instrument :

BNA_G

ClientSampleId :

T5-1-4-(0-2.5)


Tot Ion:330 Resp: 171661

Ion Ratio Lower Upper

330 100

332 95.5 77.4 116.0




141 26.4 21.4 32.0

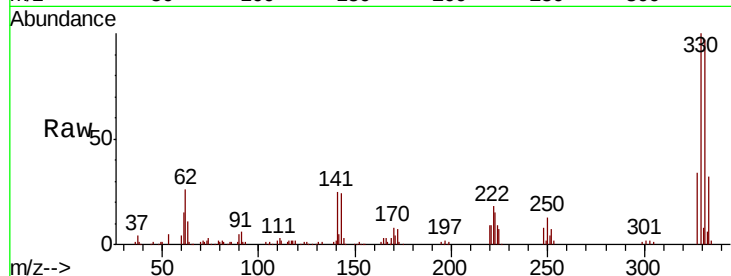

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

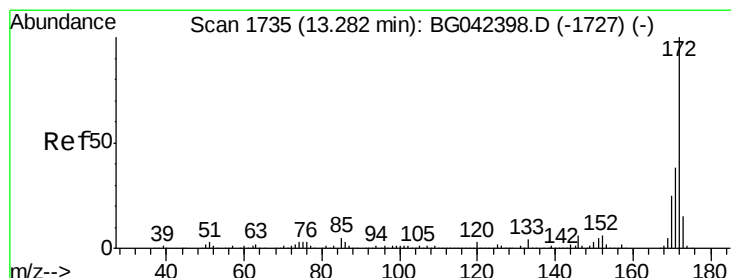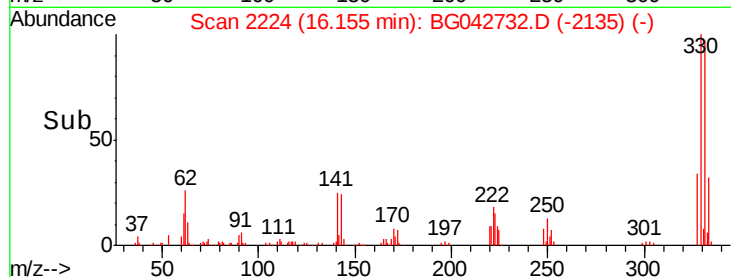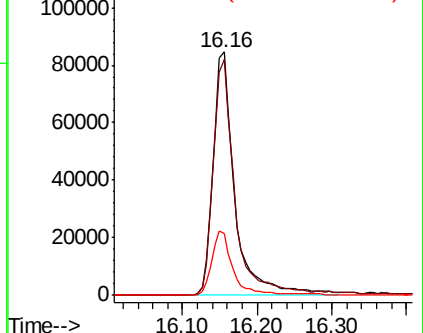

#45

2-Fluorobiphenyl

Concen: 111.040 ng

RT: 13.28 min Scan# 1734

Delta R.T. -0.01 min

Lab File: BG042732.D

Acq: 5 Sep 2019 22:35


Tgt Ion:172 Resp: 493556

Ion Ratio Lower Upper

172 100

171 37.7 30.5 45.7



170 24.6 20.2 30.2

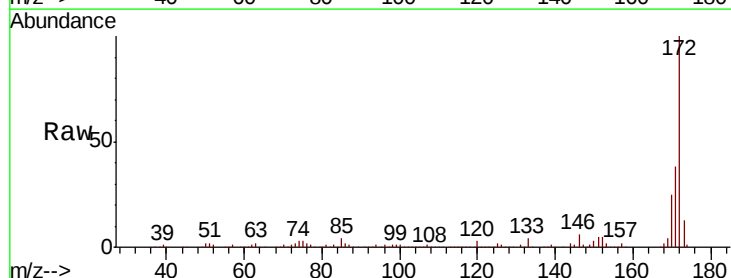

Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

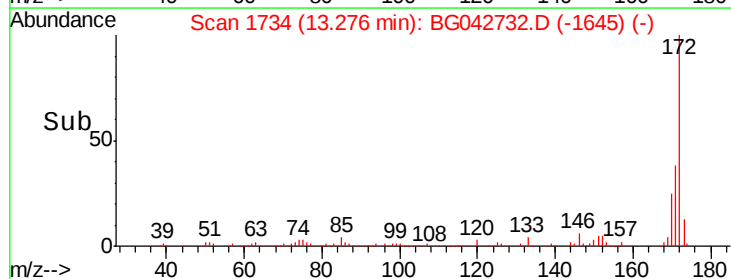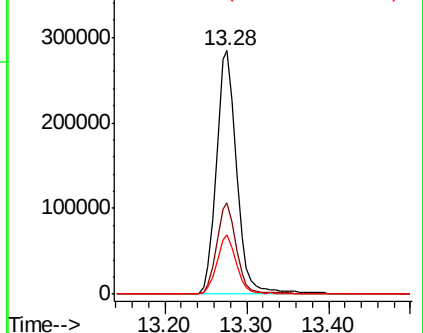



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.41 min Scan# 2438

Delta R.T. -0.01 min

Lab File: BG042732.D

Acq: 5 Sep 2019 22:35

Instrument :

BNA_G

ClientSampleId :

T5-1-4-(0-2.5)


Tot Ion:188 Resp: 187055

Ion Ratio Lower Upper

188 100

94 4.8 4.5 6.7




80 4.8 4.9 7.3#

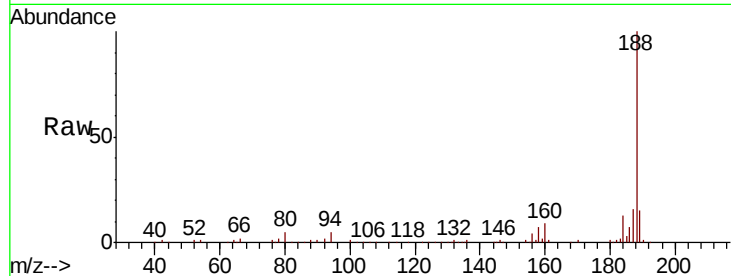

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BG

Ion 80.00 (79.70 to 80.70): BG

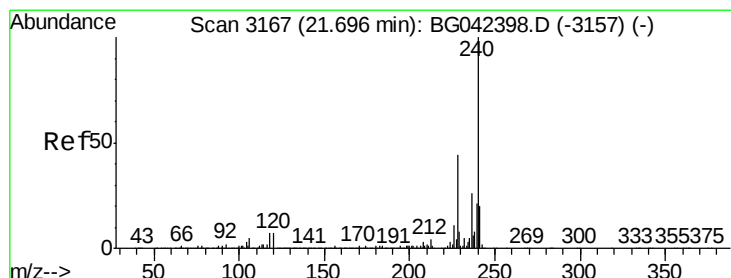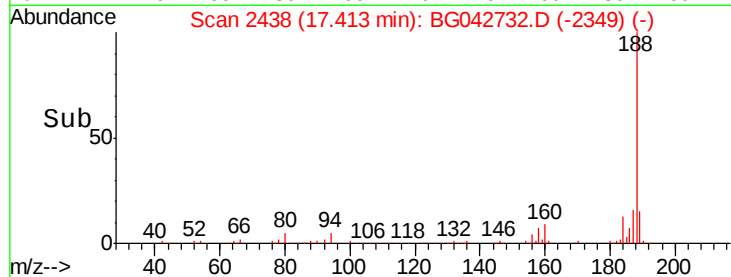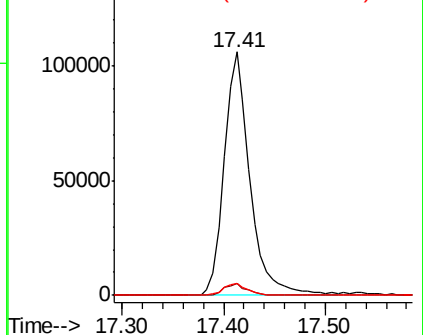

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.69 min Scan# 3166

Delta R.T. -0.01 min

Lab File: BG042732.D

Acq: 5 Sep 2019 22:35


Tgt Ion:240 Resp: 226286

Ion Ratio Lower Upper

240 100

120 5.6 5.7 8.5#



236 26.7 21.0 31.4

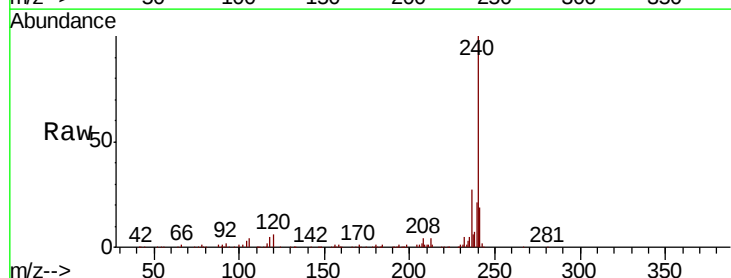

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

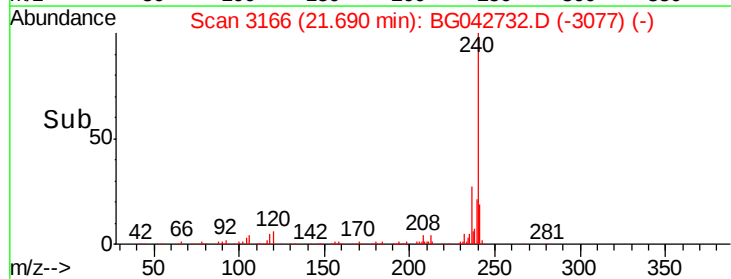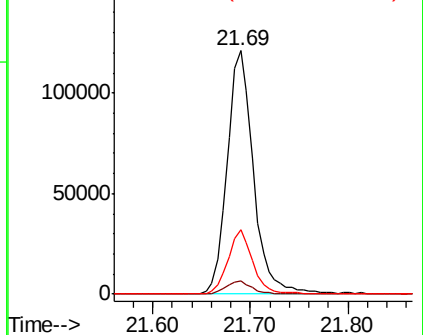



#79

Terphenyl-d14

Concen: 107.245 ng

RT: 20.02 min Scan# 2882

Delta R.T. -0.01 min

Lab File: BG042732.D

Acq: 5 Sep 2019 22:35

Instrument :

BNA_G

ClientSampleId :

T5-1-4-(0-2.5)


Tot Ion:244 Resp: 1122522

Ion Ratio Lower Upper

244 100

212 7.0 6.0 9.0




122 6.6 6.7 10.1#

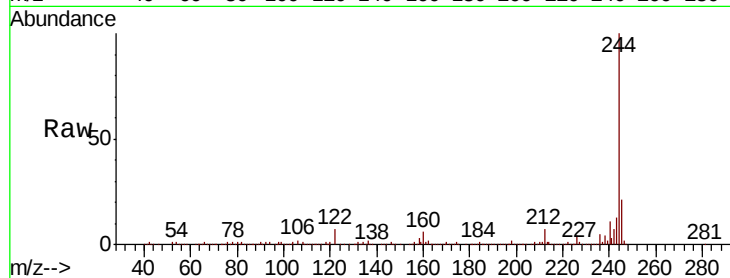

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

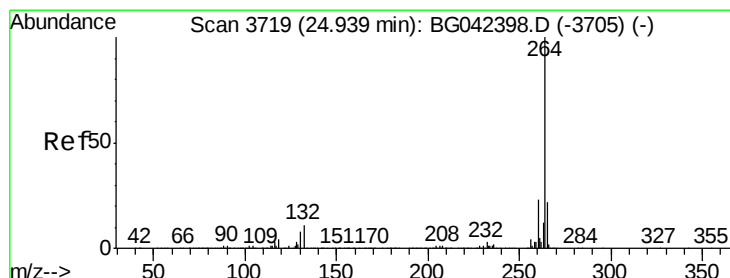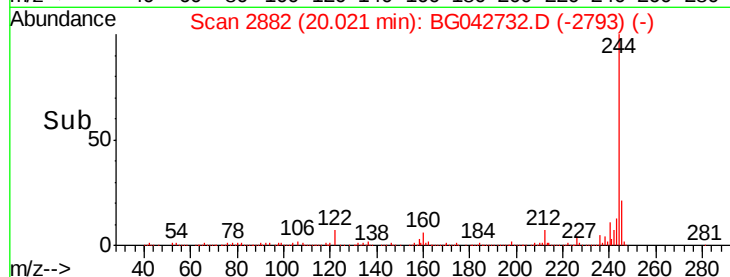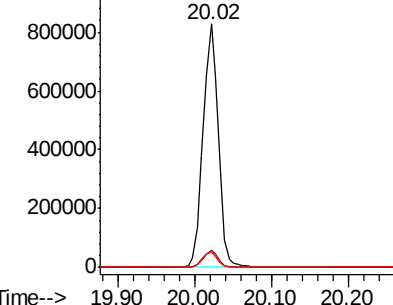

#87

Perylene-d12

Concen: 20.000 ng

RT: 24.93 min Scan# 3718

Delta R.T. -0.01 min

Lab File: BG042732.D

Acq: 5 Sep 2019 22:35


Tgt Ion:264 Resp: 261819

Ion Ratio Lower Upper

264 100

260 21.8 18.5 27.7

265 20.7 17.6 26.4

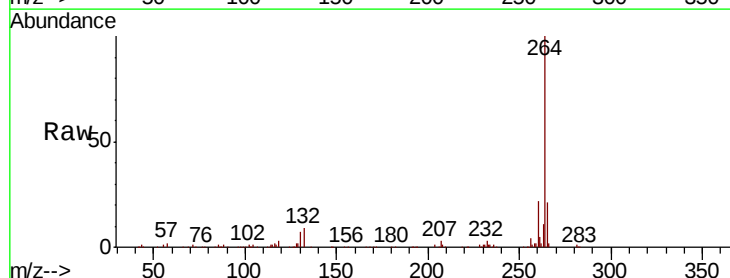

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

