


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG090519\
 Data File : BG042718.D
 Acq On : 5 Sep 2019 13:38
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 22 14:29:15 2019

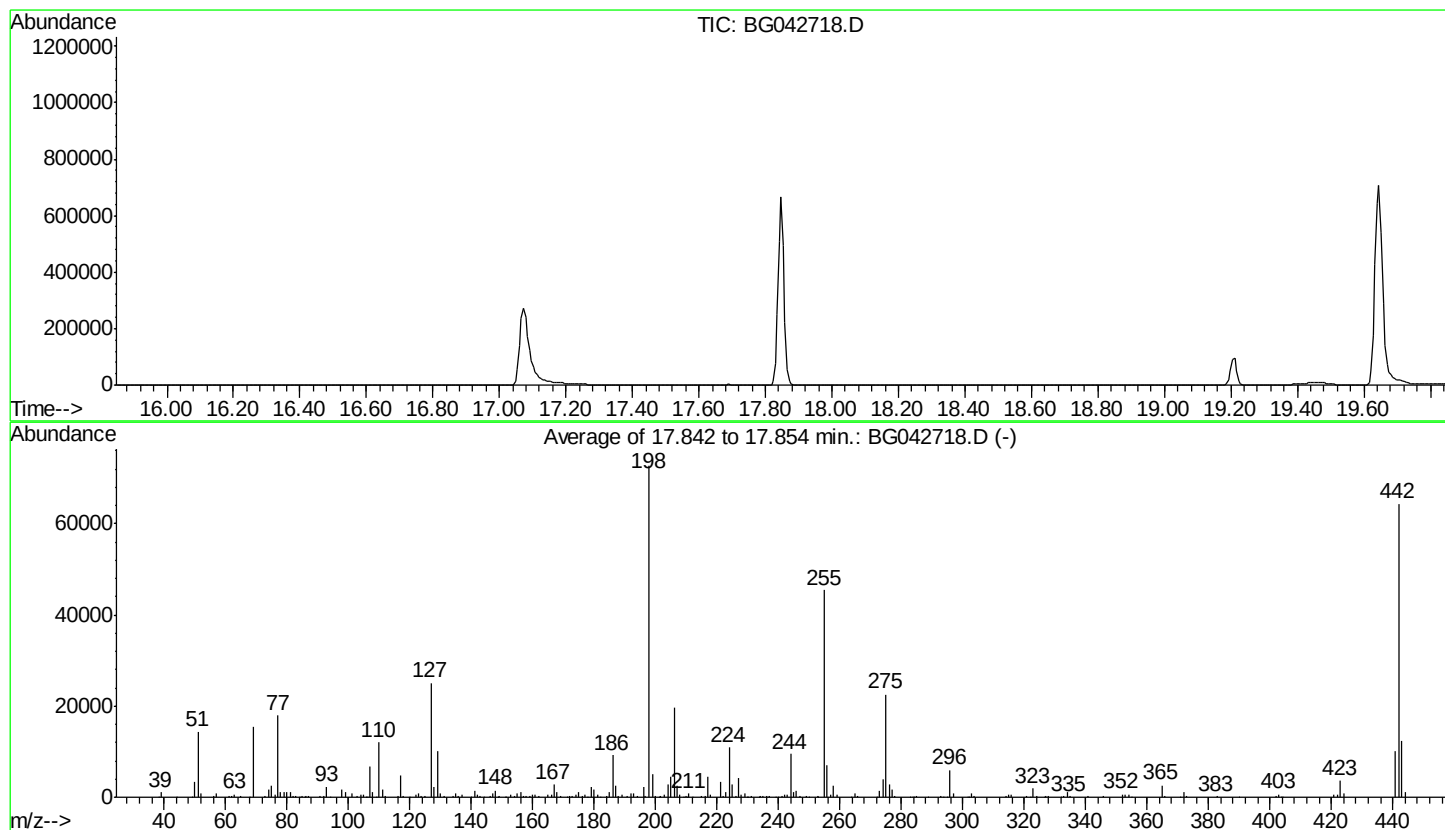

AutoFind: Scans 2511, 2512, 2513; Background Corrected with Scan 2504

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	19.8	14421	PASS
68	69	0.00	2	0.7	108	PASS
69	198	0.00	100	21.4	15586	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	34.4	25010	PASS
197	198	0.00	2	0.3	214	PASS
198	198	100	100	100.0	72746	PASS
199	198	5	9	7.0	5066	PASS
275	198	10	60	30.9	22501	PASS
365	198	1	100	3.5	2528	PASS
441	198	0.01	100	13.7	9997	PASS
442	198	50	100	88.5	64394	PASS
443	442	15	24	19.4	12496	PASS