
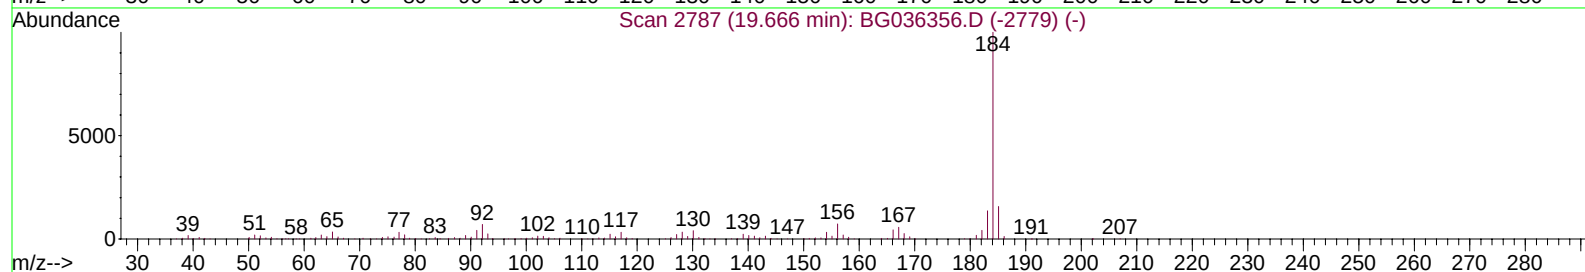
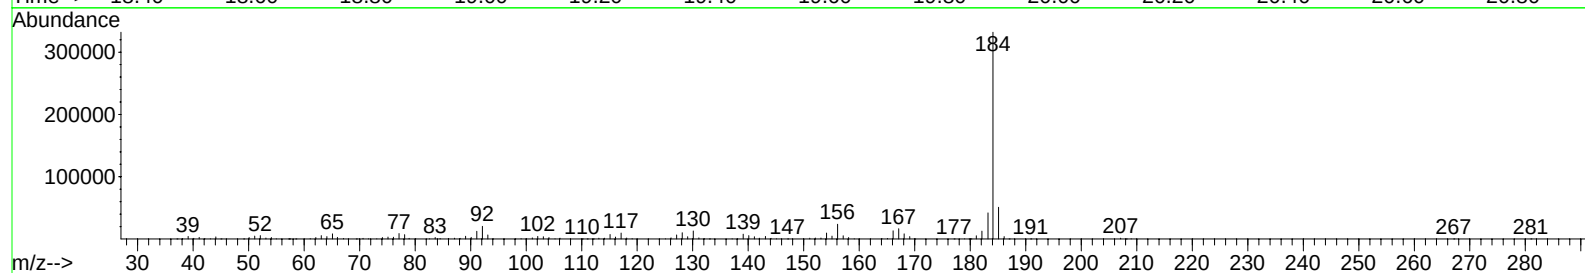


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG090618\
Data File : BG036569.D
Acq On : 6 Sep 2018 14:54
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 06 19:13:30 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 31 13:03:20 2018
Response via : Initial Calibration

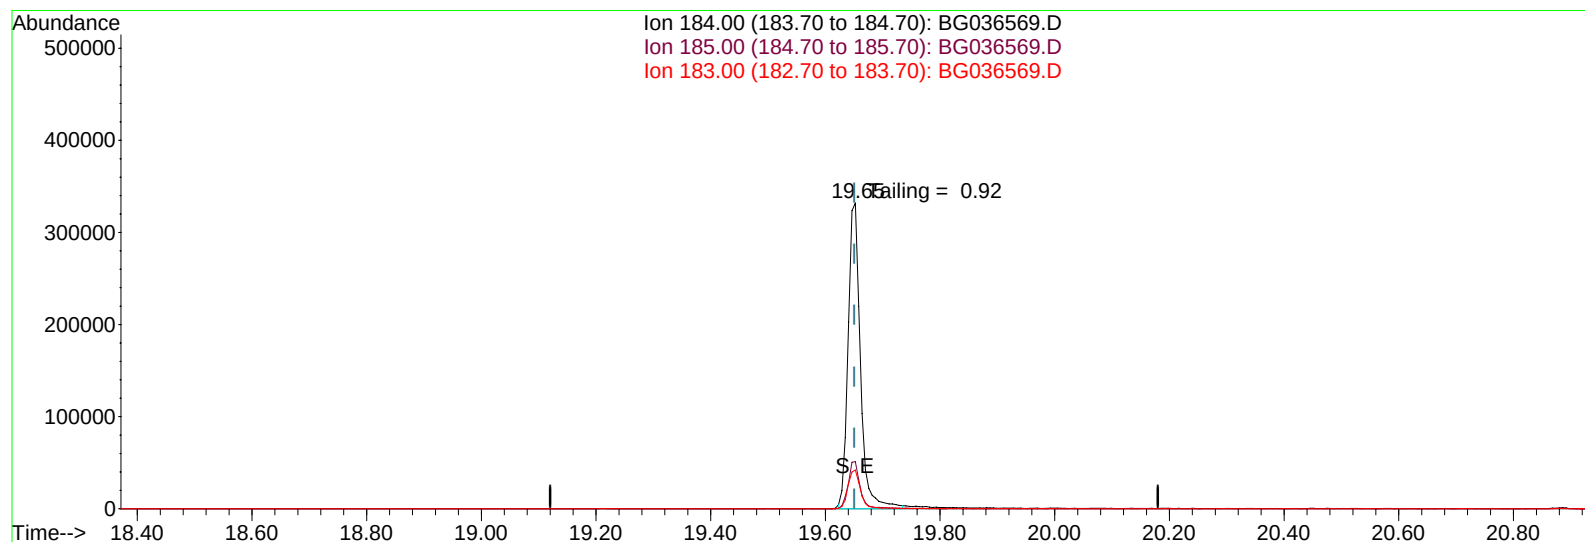

TIC: BG036569.D

(76) Benzidine




19.652min (+0.002) 10609.05ng

response 512453

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	15.37
183.00	13.60	12.69
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG090618\
Data File : BG036569.D
Acq On : 6 Sep 2018 14:54
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 06 19:13:30 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 31 13:03:20 2018
Response via : Initial Calibration

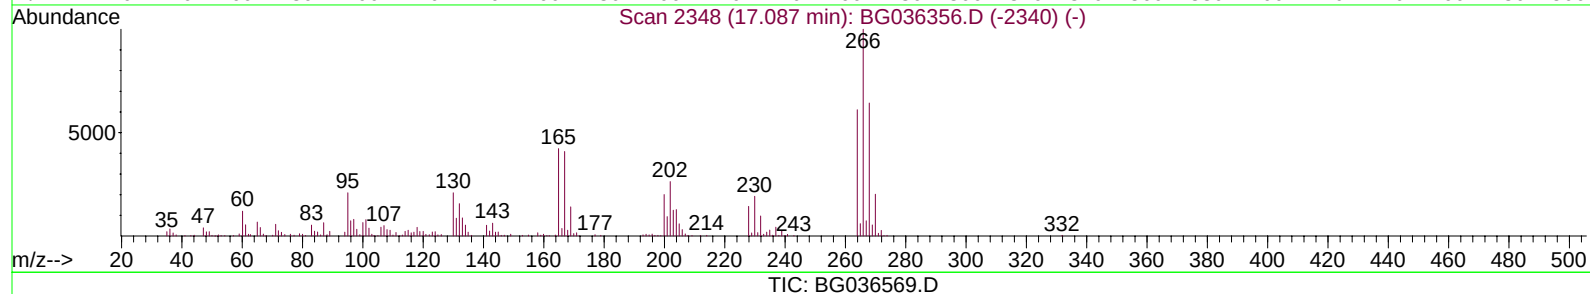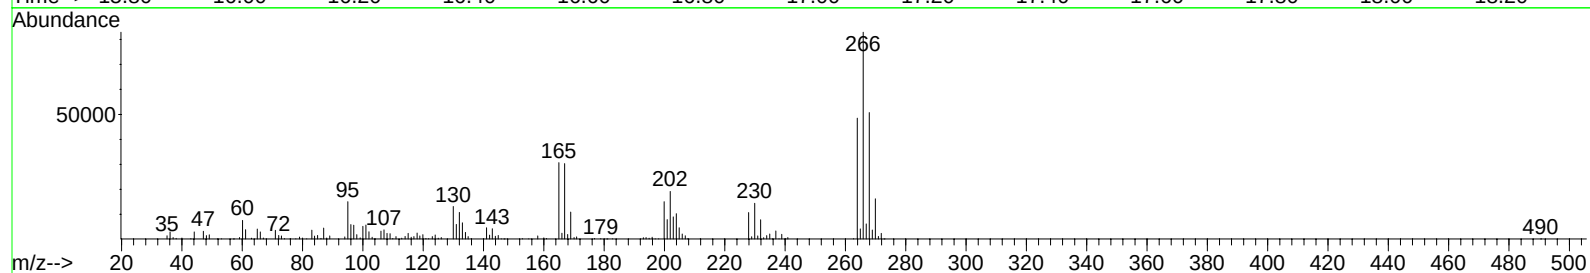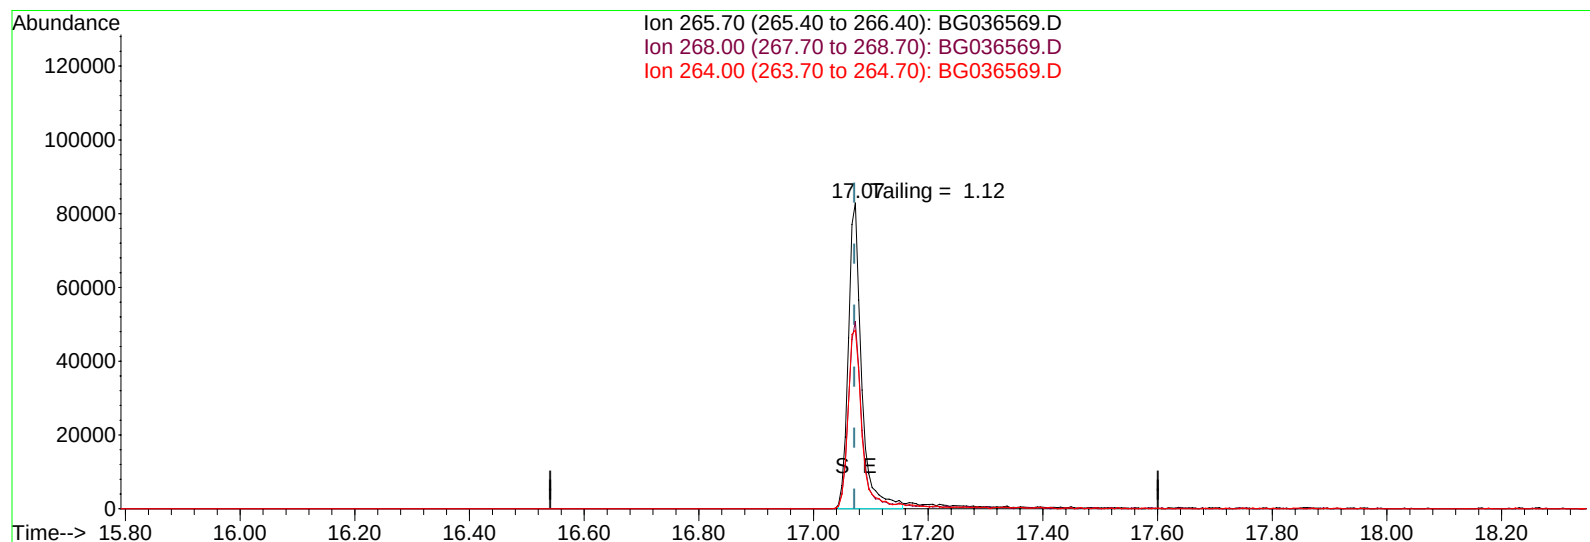

(69) Pentachlorophenol (C)

17.073min (+0.002) 13939.90ng

response 133951

Ion	Exp%	Act%
265.70	100	100
268.00	64.30	61.22
264.00	61.10	58.48
0.00	0.00	0.00