
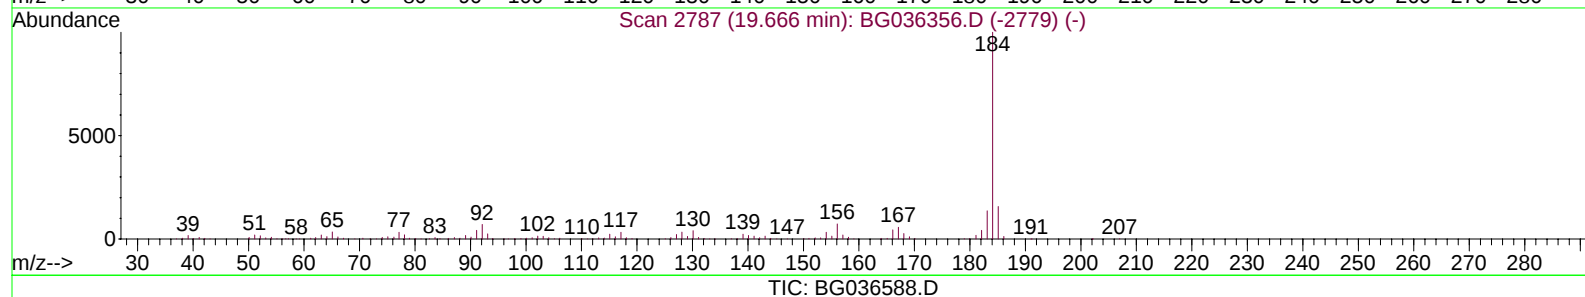
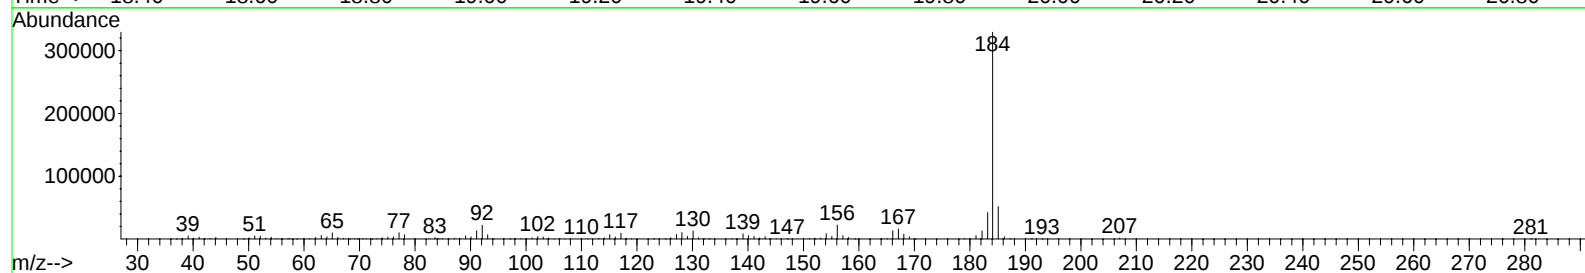


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG090618\
Data File : BG036588.D
Acq On : 7 Sep 2018 9:14
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 07 12:22:41 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 31 13:03:20 2018
Response via : Initial Calibration

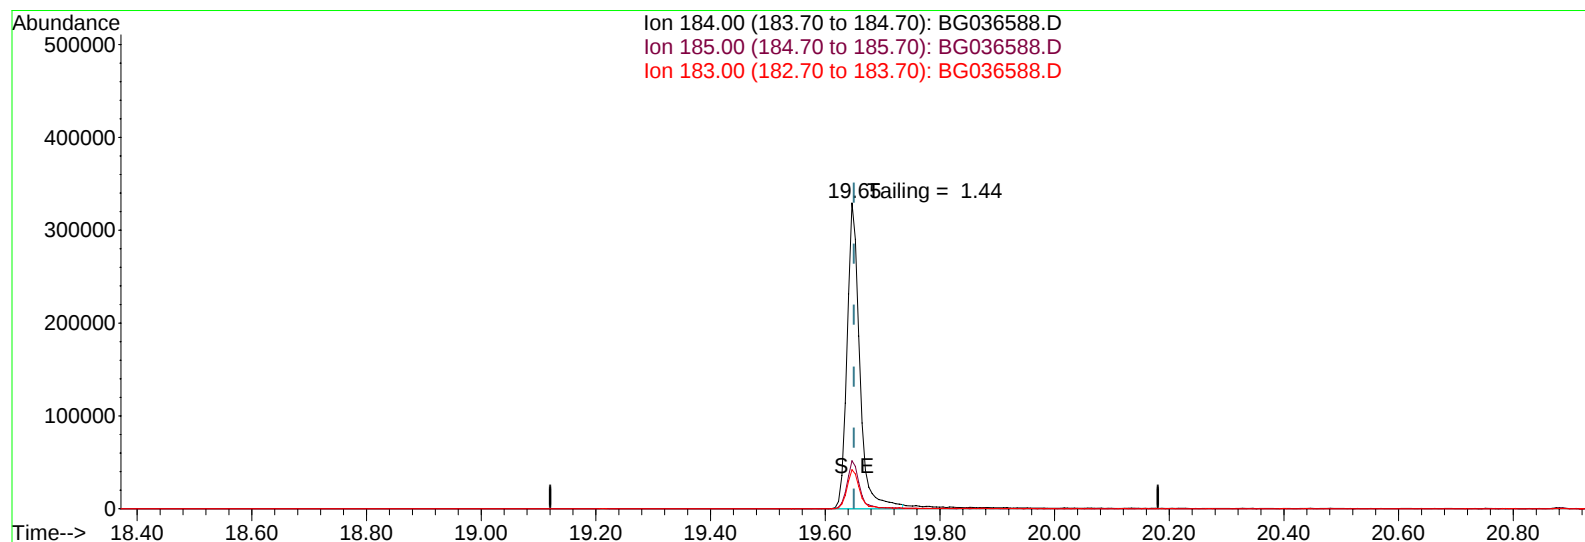

(76) Benzidine




19.647min (-0.003) 11270.87ng

response 512777

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	15.70
183.00	13.60	12.78
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG090618\
Data File : BG036588.D
Acq On : 7 Sep 2018 9:14
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 07 12:22:41 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 31 13:03:20 2018
Response via : Initial Calibration

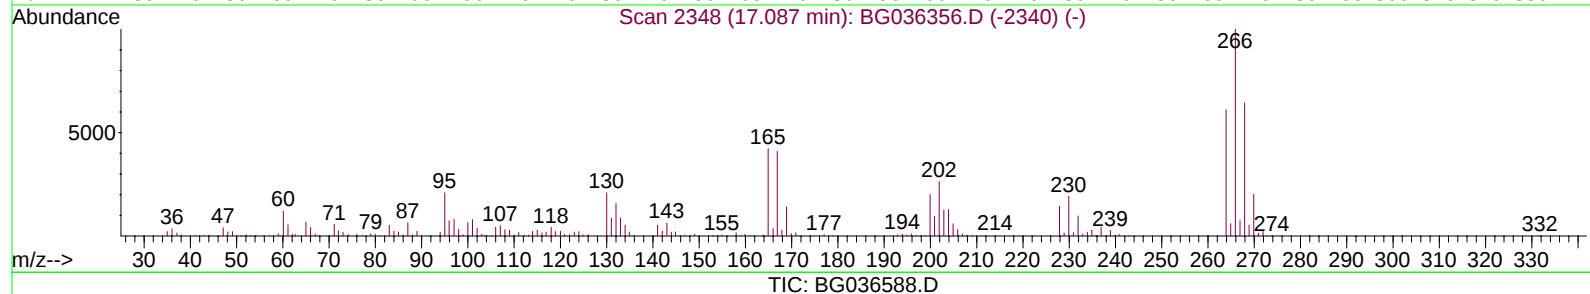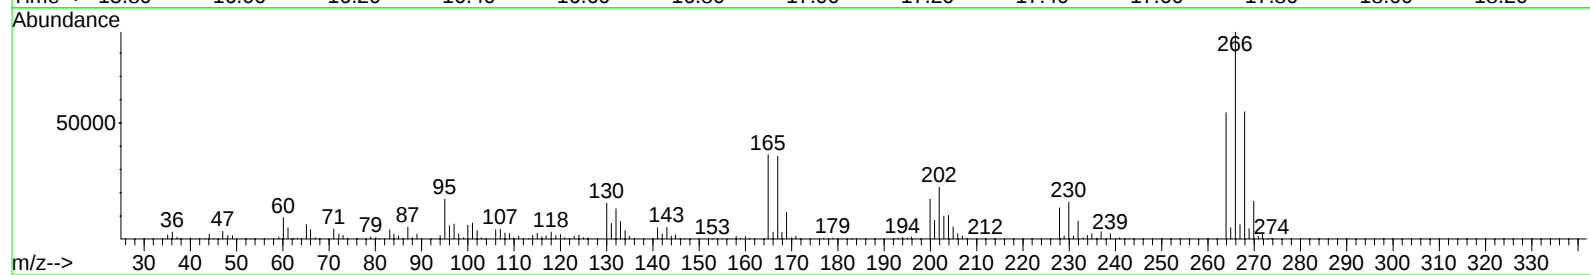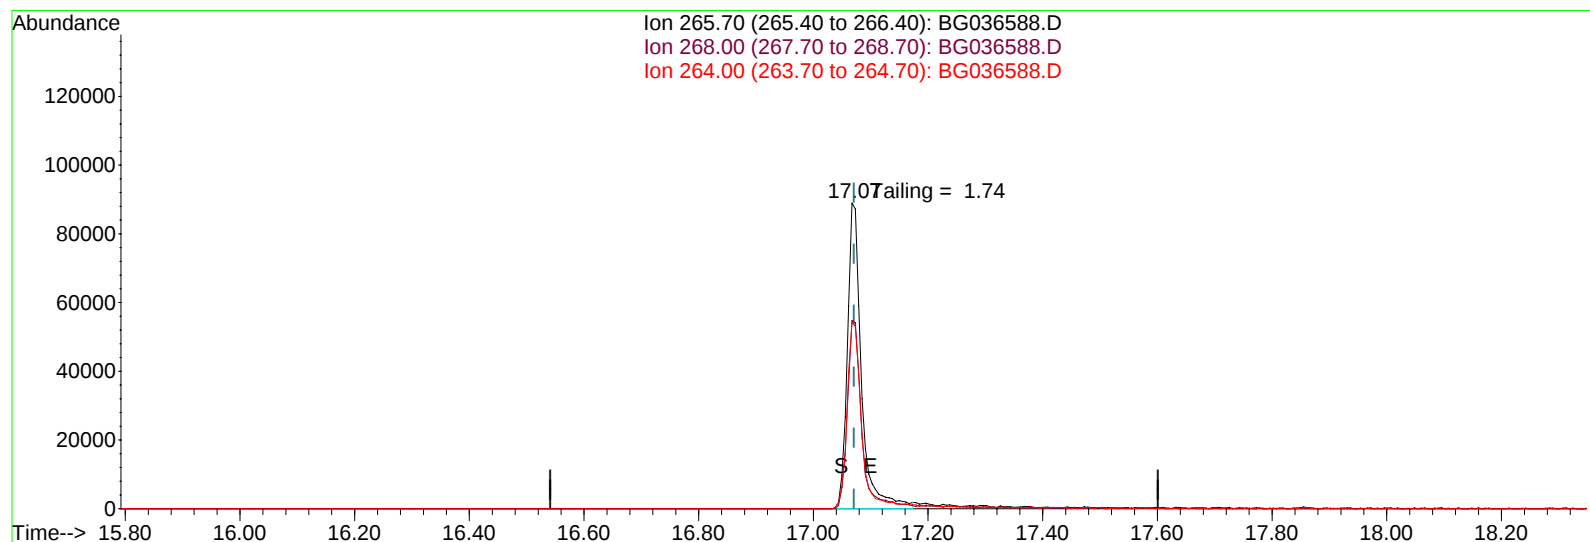

(69) Pentachlorophenol (C)

17.067min (-0.003) 15473.85ng

response 152594

Ion	Exp%	Act%
265.70	100	100
268.00	64.30	61.61
264.00	61.10	61.14
0.00	0.00	0.00