

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG090618\  
 Data File : BG036578.D  
 Acq On : 6 Sep 2018 20:46  
 Operator : JU/SJ  
 Sample : J4798-01  
 Misc :  
 ALS Vial : 10 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 090418-JETT-E-D-B

Integration Parameters: rteint.p  
 Integrator: RTE  
 Smoothing : ON  
 Sampling : 1  
 Start Thrs: 0.2  
 Stop Thrs : 0  
 Filtering: 5  
 Min Area: 3 % of largest Peak  
 Max Peaks: 100  
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG082318.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.162       | 313           | 319         | 326          | rVB      | 43613          | 64760         | 1.28%           | 0.296%        |
| 2         | 5.626       | 391           | 398         | 407          | rBV      | 398189         | 644913        | 12.78%          | 2.952%        |
| 3         | 7.207       | 659           | 667         | 676          | rBV      | 262043         | 462296        | 9.16%           | 2.116%        |
| 4         | 7.588       | 724           | 732         | 740          | rBV      | 697215         | 1227504       | 24.32%          | 5.618%        |
| 5         | 8.059       | 805           | 812         | 818          | rBV      | 206498         | 344556        | 6.83%           | 1.577%        |
| 6         | 8.382       | 859           | 867         | 876          | rVB      | 924423         | 1594277       | 31.58%          | 7.297%        |
| 7         | 9.216       | 999           | 1009        | 1021         | rBV      | 820253         | 1480953       | 29.34%          | 6.779%        |
| 8         | 10.861      | 1282          | 1289        | 1297         | rBV      | 287929         | 510682        | 10.12%          | 2.337%        |
| 9         | 13.305      | 1698          | 1705        | 1722         | rBV      | 2269404        | 3504713       | 69.43%          | 16.042%       |
| 10        | 14.128      | 1838          | 1845        | 1851         | rBV      | 209801         | 300621        | 5.96%           | 1.376%        |
| 11        | 14.680      | 1932          | 1939        | 1947         | rBV2     | 494183         | 794093        | 15.73%          | 3.635%        |
| 12        | 15.967      | 2152          | 2158        | 2164         | rBV      | 124374         | 166157        | 3.29%           | 0.761%        |
| 13        | 16.167      | 2185          | 2192        | 2212         | rBV      | 1235180        | 1899434       | 37.63%          | 8.694%        |
| 14        | 17.424      | 2399          | 2406        | 2414         | rBV2     | 648903         | 1021158       | 20.23%          | 4.674%        |
| 15        | 18.305      | 2549          | 2556        | 2563         | rBV2     | 58475          | 94044         | 1.86%           | 0.430%        |
| 16        | 20.033      | 2843          | 2850        | 2859         | rBV      | 3704302        | 5048114       | 100.00%         | 23.106%       |
| 17        | 21.690      | 3125          | 3132        | 3141         | rBV2     | 668685         | 1166710       | 23.11%          | 5.340%        |
| 18        | 23.188      | 3381          | 3387        | 3397         | rVB2     | 43325          | 84457         | 1.67%           | 0.387%        |
| 19        | 23.993      | 3518          | 3524        | 3532         | rVB2     | 52442          | 109301        | 2.17%           | 0.500%        |
| 20        | 24.898      | 3668          | 3678        | 3695         | rBV      | 355614         | 1156408       | 22.91%          | 5.293%        |
| 21        | 26.073      | 3870          | 3878        | 3888         | rVB4     | 33551          | 105190        | 2.08%           | 0.481%        |
| 22        | 27.430      | 4101          | 4109        | 4119         | rVB5     | 21361          | 67268         | 1.33%           | 0.308%        |


Sum of corrected areas: 21847609

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG090618\  
Data File : BG036578.D  
Acq On : 6 Sep 2018 20:46  
Operator : JU/SJ  
Sample : J4798-01  
Misc :  
ALS Vial : 10 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
090418-JETT-E-D-B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L  
TIC Integration Parameters: LSCINT.P

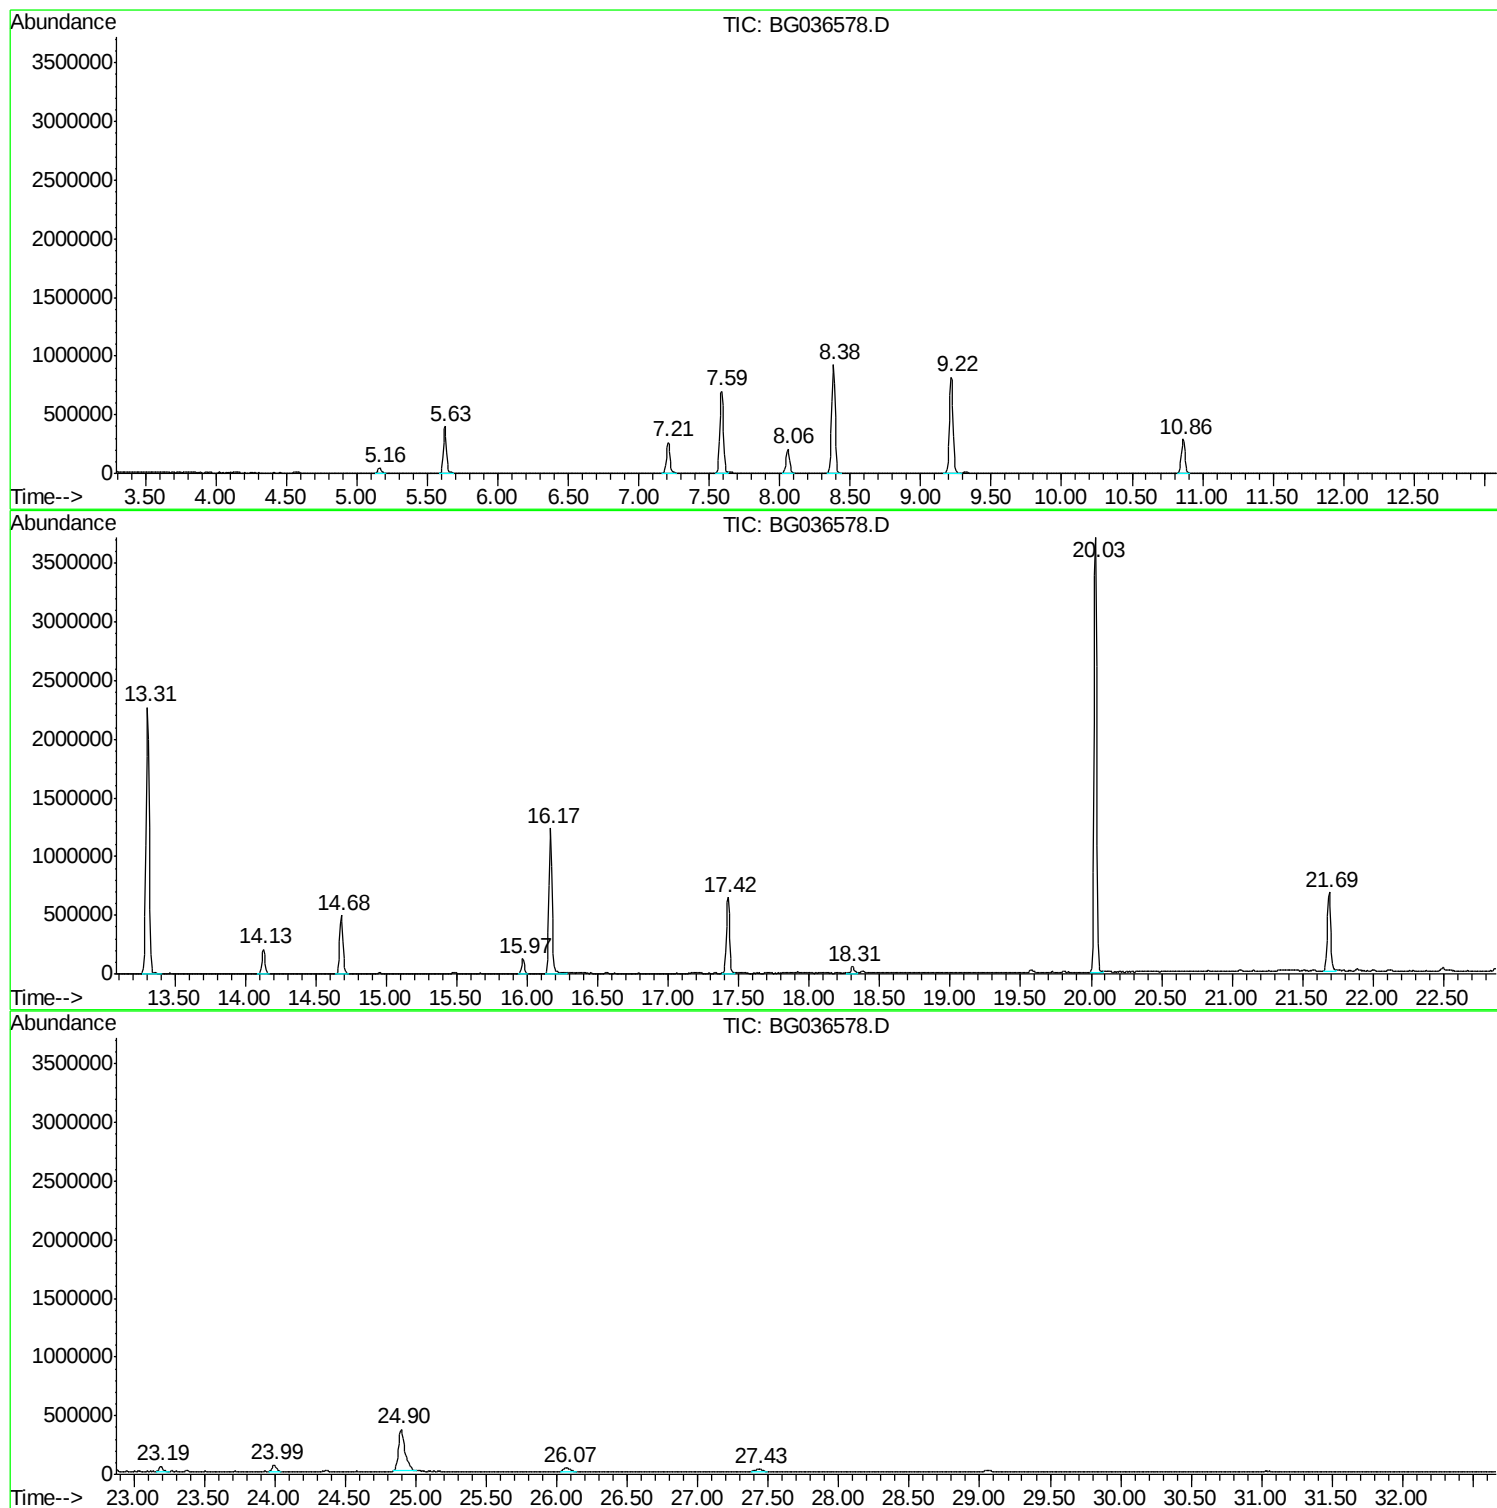

Data\_Path : Z:\SVOASRV\HPCHEM1\BNA\_G\DATA\BG090618\  
Data\_File : BG036578.D  
Acq\_On : 6-Sep-2018 20:466  
Operator : JU/SJJ  
Sample : J4798-011  
Misc :  
ALS\_Vial : 10 Sample\_Multiplier: 11

Instrument :  
BNA\_G  
ClientSampleId :  
090418-JETT-E-D-B

Quant\_Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG082318.MM  
Quant\_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC\_Library : C:\Database\NIST11.LL  
TIC\_Integration\_Parameters: LSCINT.PP

| TIC Top Hit name | RT | EstConc | Units | Response | Internal Standard |
|------------------|----|---------|-------|----------|-------------------|
|                  |    |         |       | #        | RT Resp Conc      |

No Library Search Compounds Detected

\*\*\*\*\*