


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG090618\
 Data File : BG036569.D
 Acq On : 6 Sep 2018 14:54
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 31 13:03:20 2018

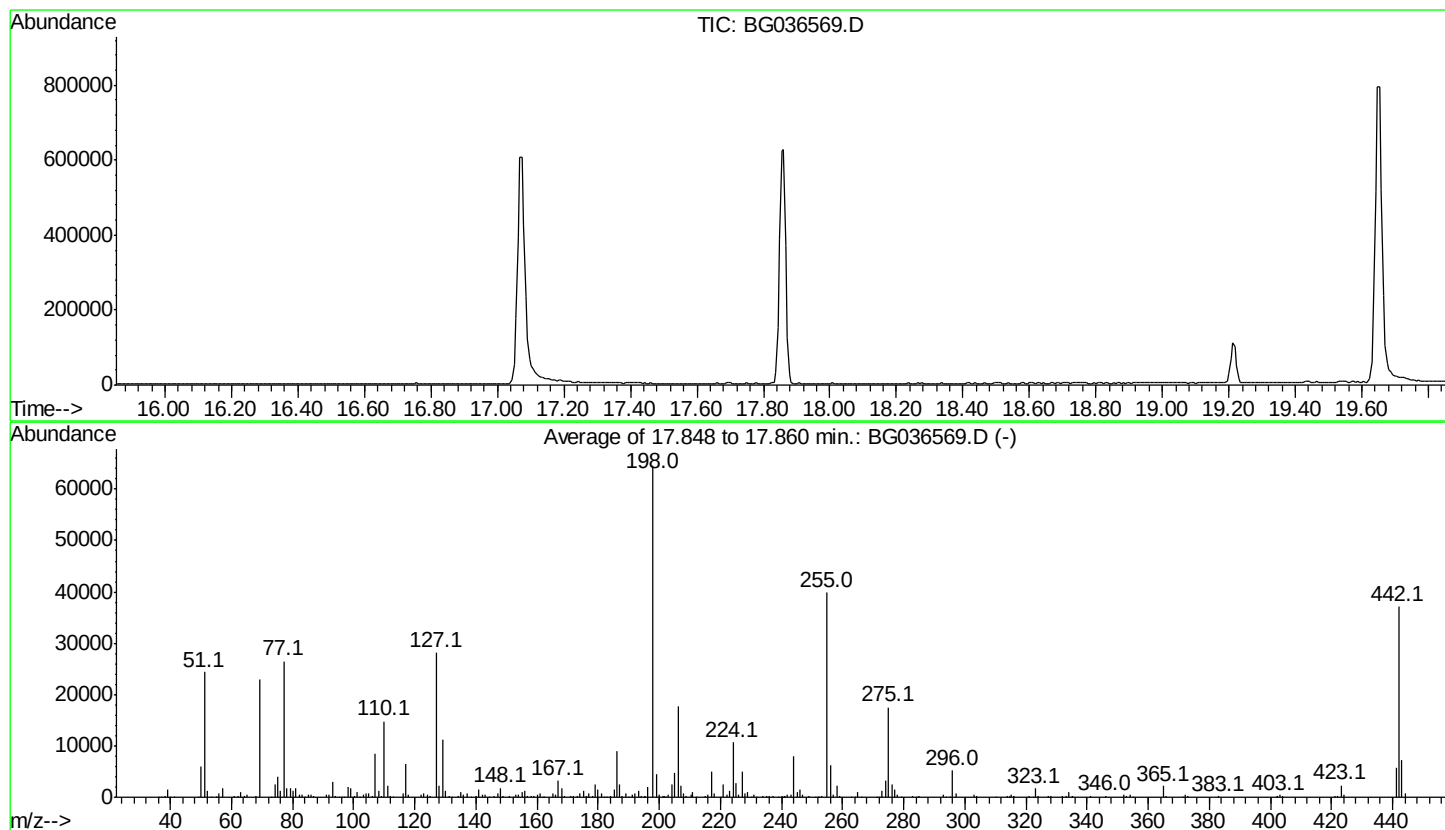

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.7	24333	PASS
68	69	0.00	2	1.3	298	PASS
69	198	0.00	100	35.5	22896	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.5	28061	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	64581	PASS
199	198	5	9	6.9	4447	PASS
275	198	10	60	27.1	17507	PASS
365	198	1	100	3.4	2190	PASS
441	198	0.01	100	8.7	5644	PASS
442	198	50	100	57.4	37090	PASS
443	442	15	24	19.6	7286	PASS