
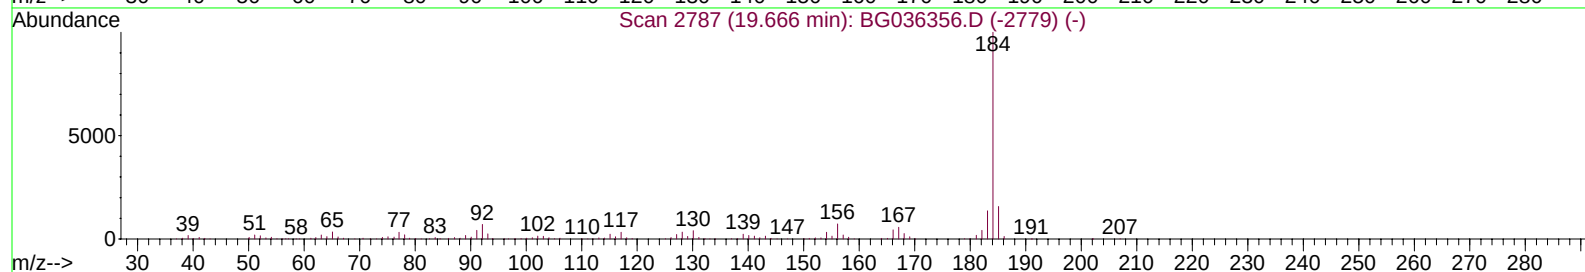
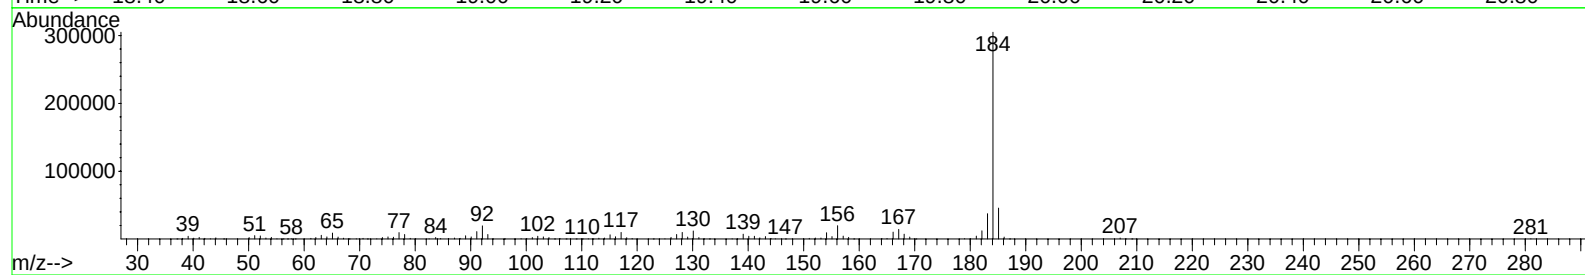


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG090718\
Data File : BG036593.D
Acq On : 7 Sep 2018 12:29
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 07 18:08:22 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 31 13:03:20 2018
Response via : Initial Calibration

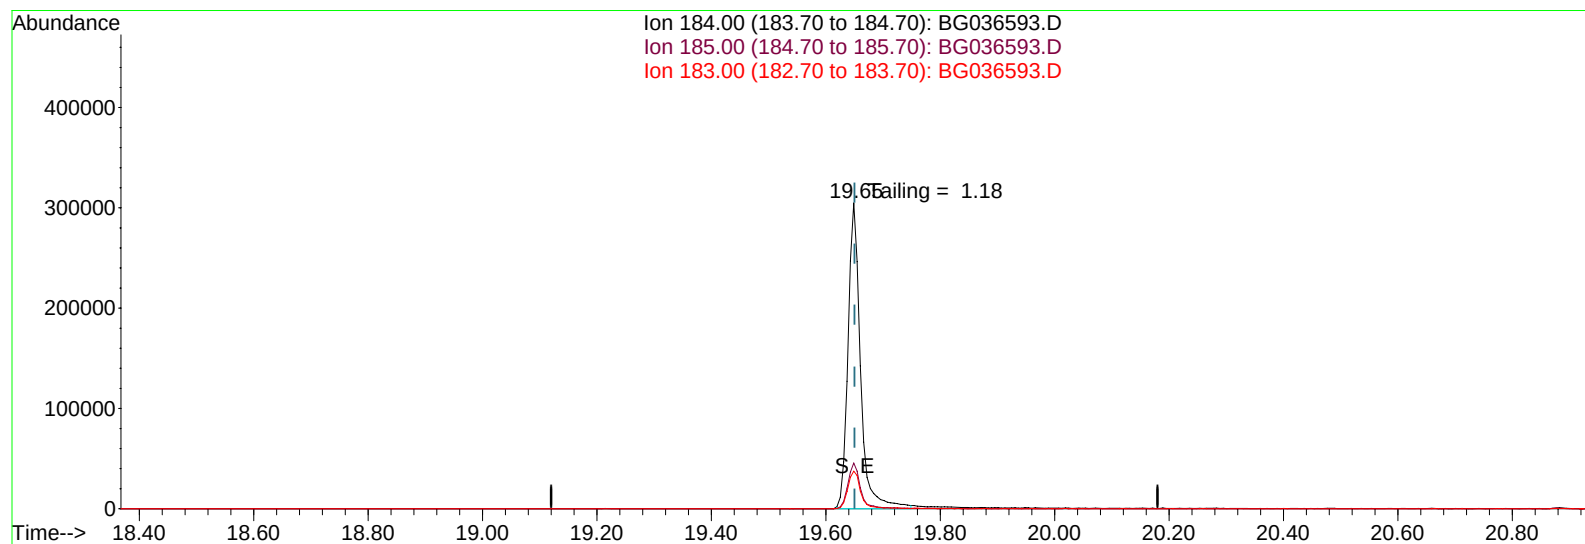

TIC: BG036593.D

(76) Benzidine




19.649min (-0.001) 9118.11ng

response 472726

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.98
183.00	13.60	12.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG090718\
Data File : BG036593.D
Acq On : 7 Sep 2018 12:29
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 07 18:08:22 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 31 13:03:20 2018
Response via : Initial Calibration

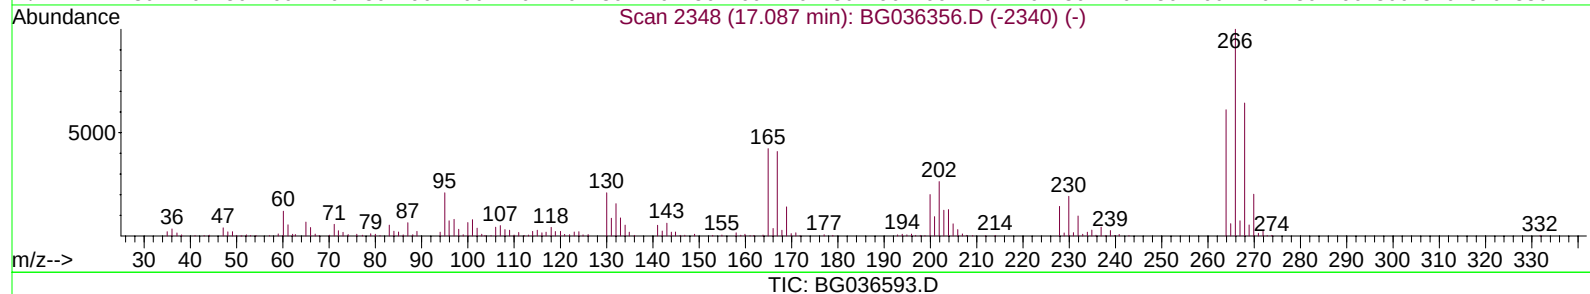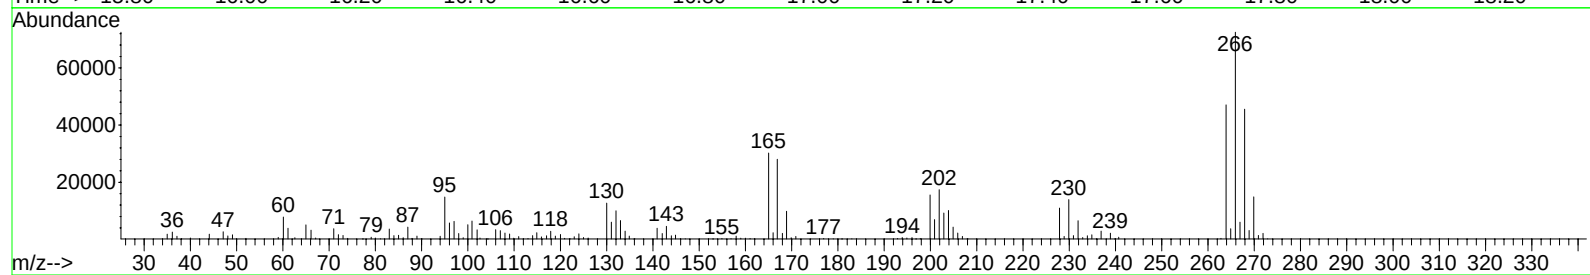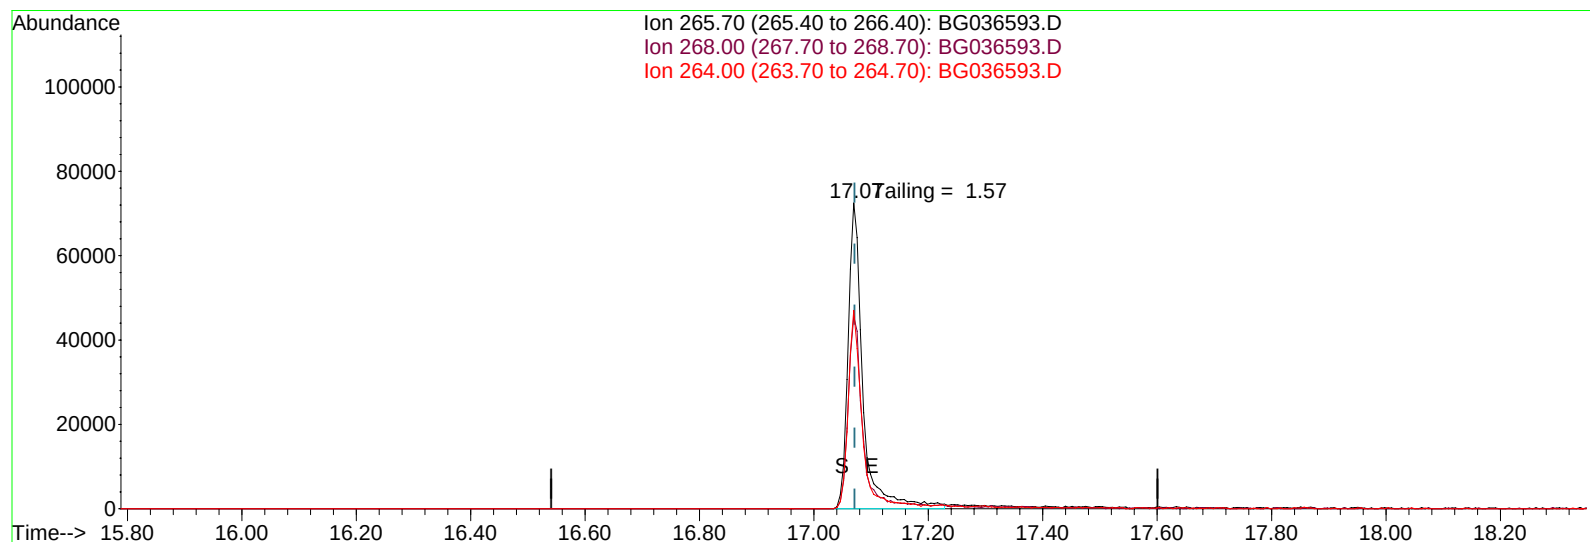

(69) Pentachlorophenol (C)

17.069min (-0.001) 13226.41ng

response 129032

Ion	Exp%	Act%
265.70	100	100
268.00	64.30	62.87
264.00	61.10	64.92
0.00	0.00	0.00