

Data File : BG036612.D

Acq On : 8 Sep 2018 1:28

Operator : JU/SJ

Sample : DFTPP

Misc :

ALS Vial : 1 Sample Multiplier: 1




Quant Time: Sep 08 04:41:14 2018

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082318.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Aug 31 13:03:20 2018

Response via : Initial Calibration

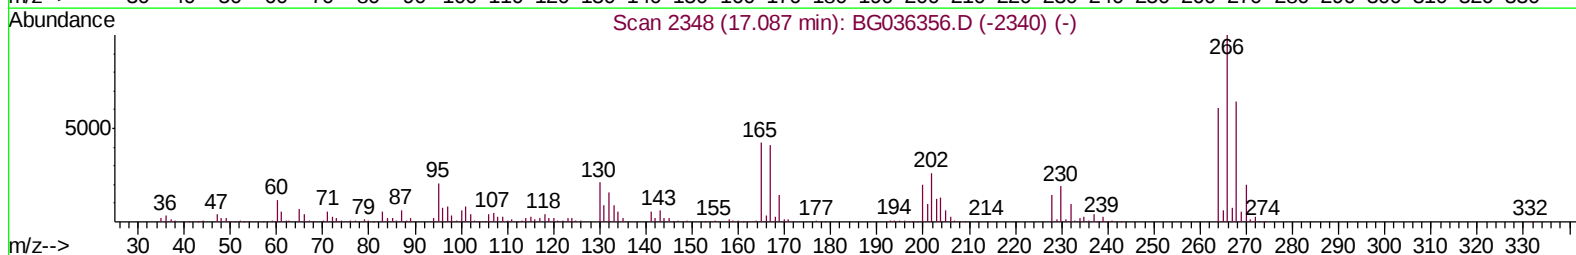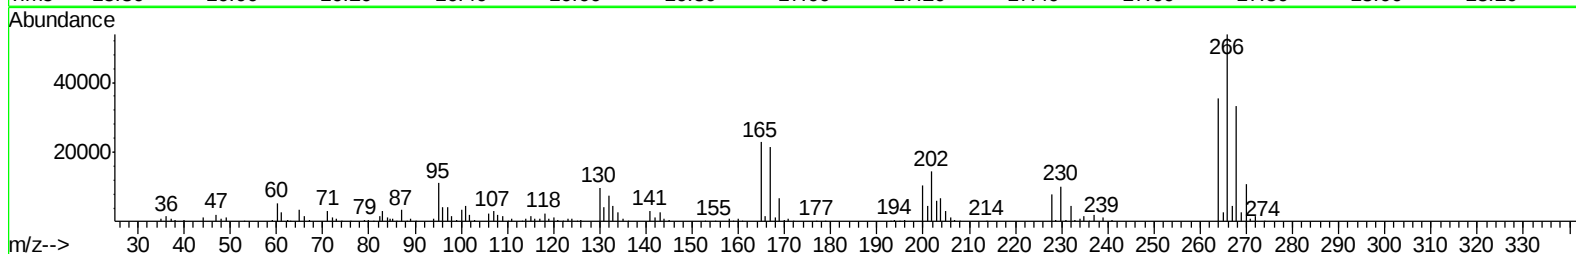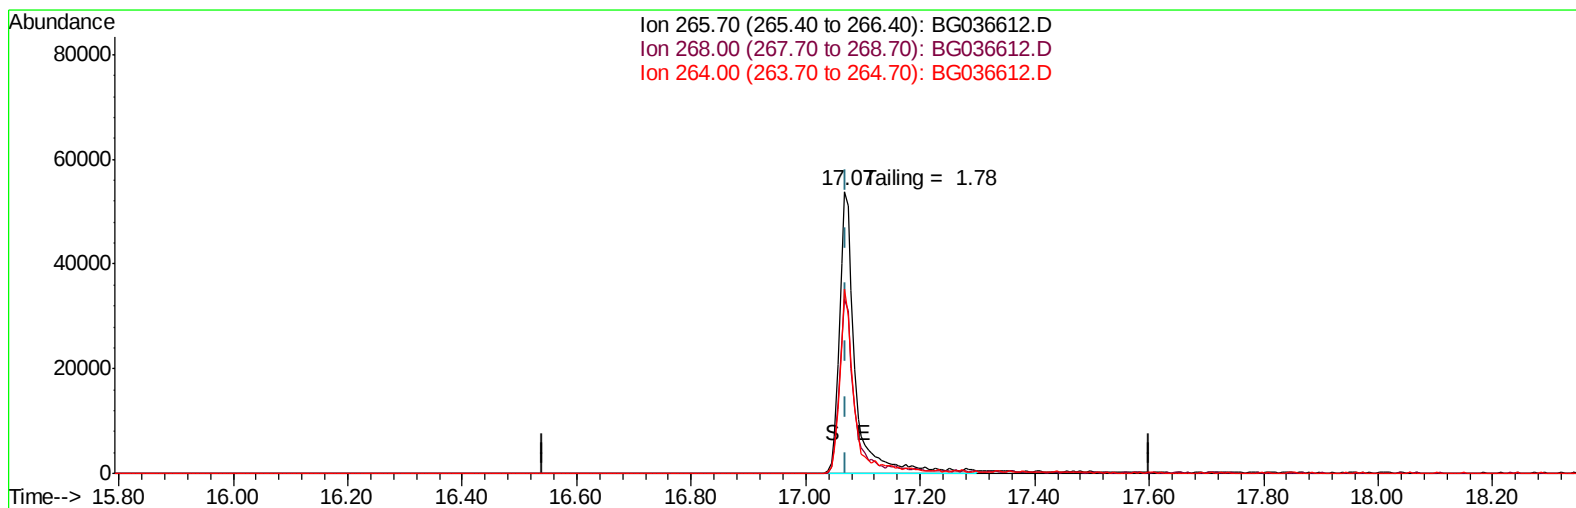

TIC: BG036612.D

(69) Pentachlorophenol (C)




17.068min (-0.003) 20663.02ng

response 98857

Ion	Exp%	Act%
265.70	100	100
268.00	64.30	61.61
264.00	61.10	65.57
0.00	0.00	0.00

Data File : BG036612.D
Acq On : 8 Sep 2018 1:28
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 08 04:41:14 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 31 13:03:20 2018
Response via : Initial Calibration

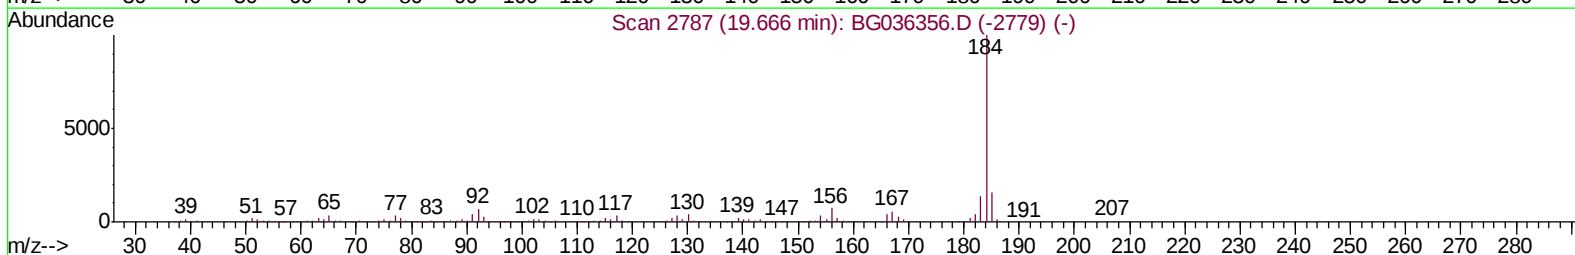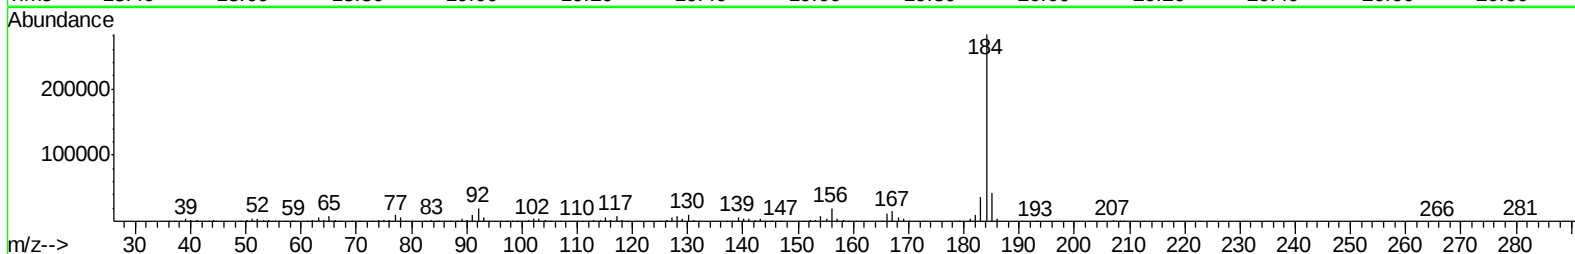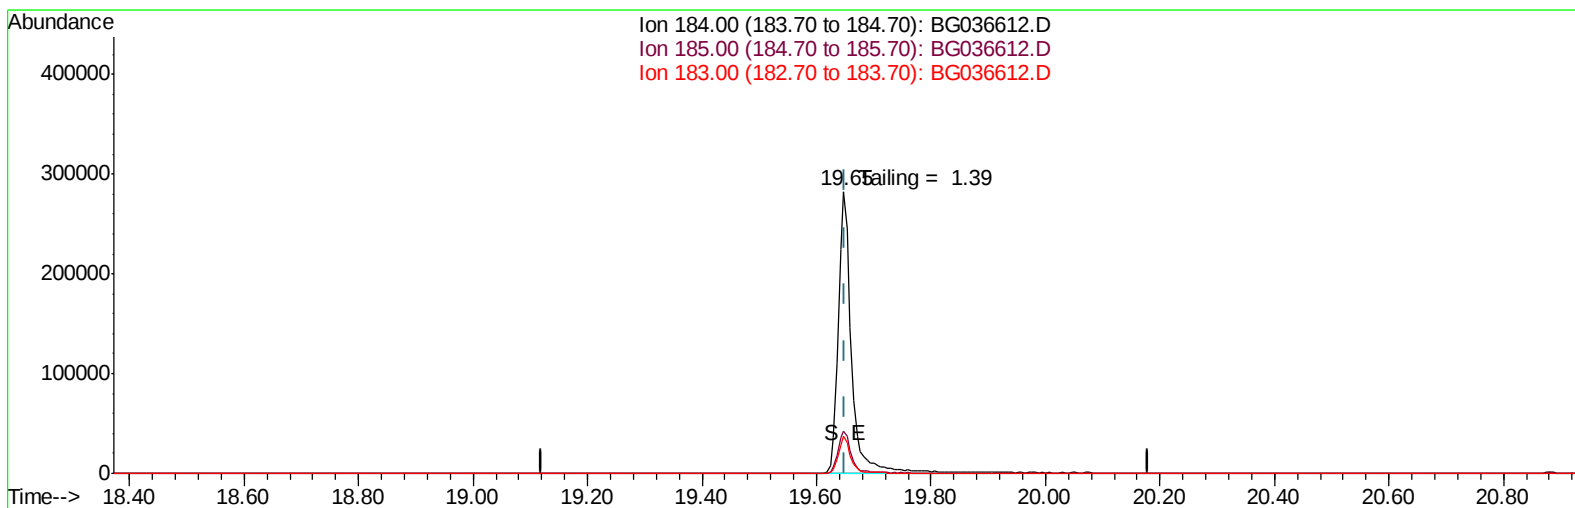

TIC: BG036612.D

(76) Benzidine

19.647min (-0.003) 29306.81ng

response 459094

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.90
183.00	13.60	13.14
0.00	0.00	0.00