

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG090718\
 Data File : BG036615.D
 Acq On : 8 Sep 2018 3:26
 Operator : JU/SJ
 Sample : J4798-18
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 090418-TIPC-E-U-M

Quant Time: Sep 08 04:34:35 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 31 13:03:20 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.06	152	58138	20.00	ng	0.00
21) Naphthalene-d8	10.86	136	251136	20.00	ng	0.00
38) Acenaphthene-d10	14.68	164	170611	20.00	ng	0.00
63) Phenanthrene-d10	17.42	188	429408	20.00	ng	0.00
75) Chrysene-d12	21.68	240	429398	20.00	ng	-0.01
86) Perylene-d12	24.90	264	413701	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.63	112	183663	50.11	ng	0.00
7) Phenol-d6	7.21	99	171334	32.65	ng	-0.01
23) Nitrobenzene-d5	9.22	82	518244	111.96	ng	0.00
41) 2,4,6-Tribromophenol	16.17	330	240998	118.38	ng	0.00
44) 2-Fluorobiphenyl	13.31	172	1183338	99.03	ng	0.00
78) Terphenyl-d14	20.03	244	1788820	97.37	ng	0.00
Target Compounds						Qvalue
49) Dimethylphthalate	14.13	163	65650	4.712	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG090718\
Data File : BG036615.D
Acq On : 8 Sep 2018 3:26
Operator : JU/SJ
Sample : J4798-18
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
090418-TIPC-E-U-M

Quant Time: Sep 08 04:34:35 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 31 13:03:20 2018
Response via : Initial Calibration

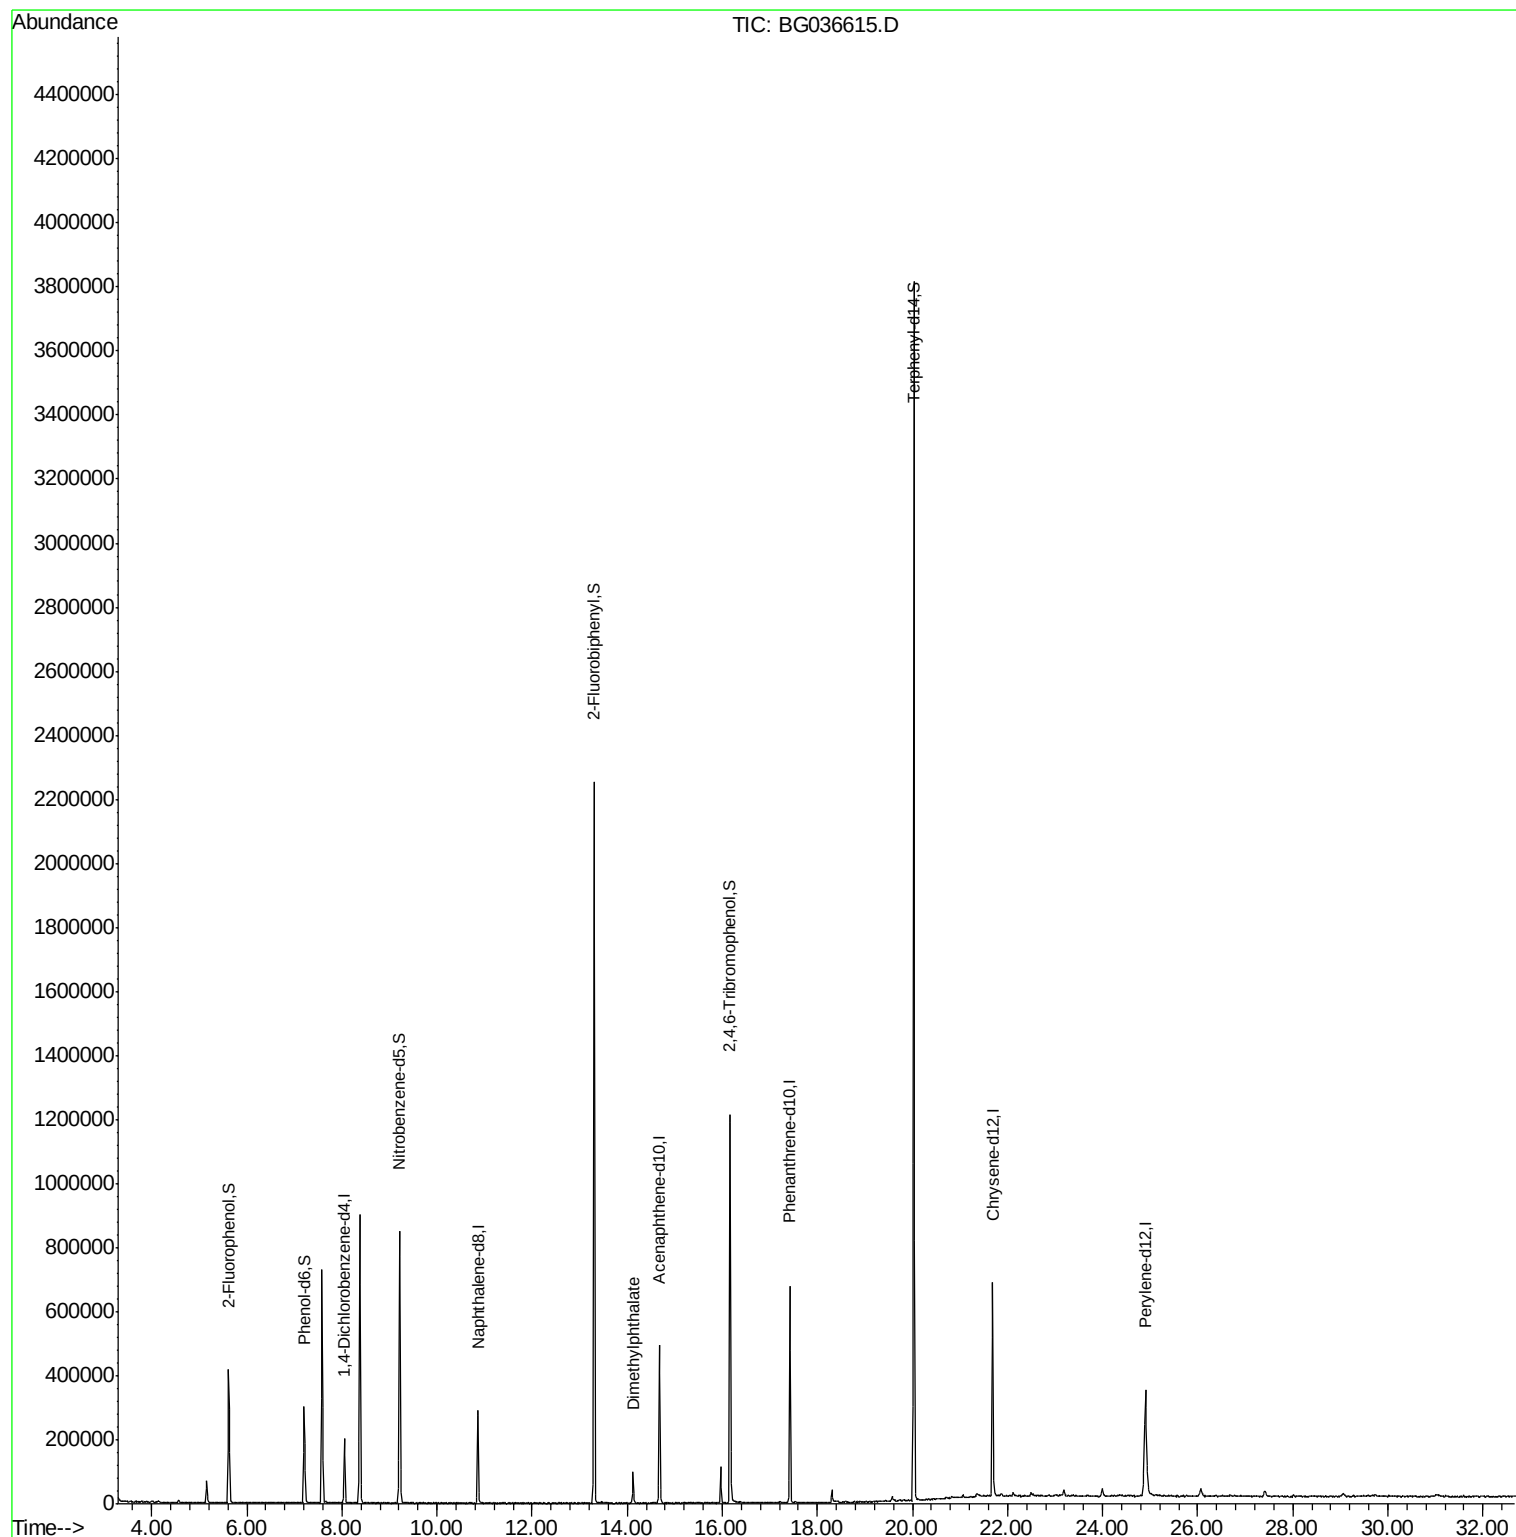

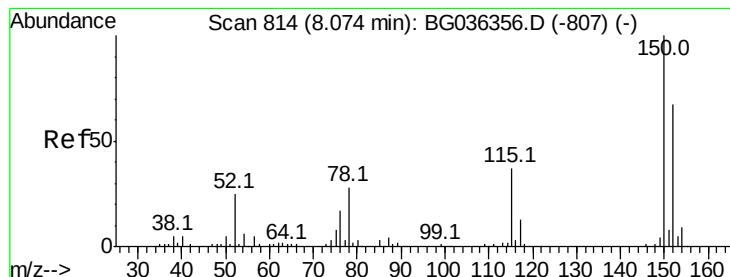

#1

1,4-Dichlorobenzene-d4

Concen: 20.000 ng

RT: 8.06 min Scan# 812

Delta R.T. -0.00 min

Lab File: BG036615.D

Acq: 8 Sep 2018 3:26

Instrument :

BNA_G

ClientSampleId :

090418-TIPC-E-U-M


Tot Ion:152 Resp: 58138

Ion Ratio Lower Upper

152 100

150 149.7 119.5 179.3




115 56.3 44.5 66.7

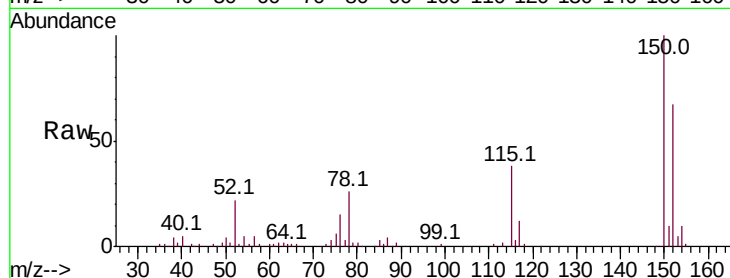

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

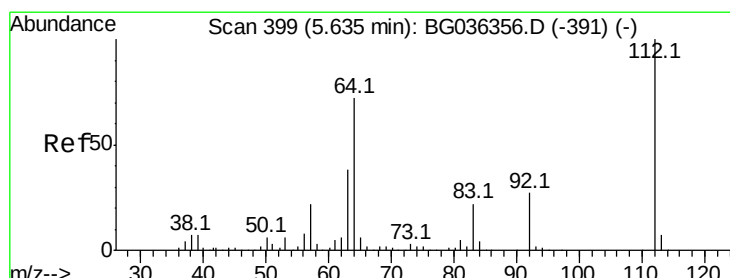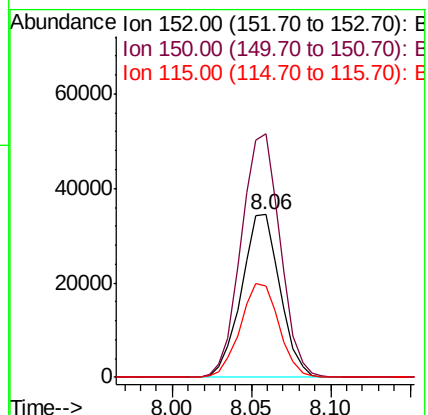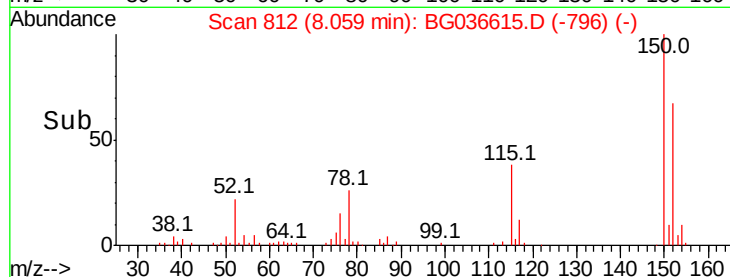

#5

2-Fluorophenol

Concen: 50.112 ng

RT: 5.63 min Scan# 398

Delta R.T. 0.00 min

Lab File: BG036615.D

Acq: 8 Sep 2018 3:26


Tgt Ion:112 Resp: 183663

Ion Ratio Lower Upper

112 100

64 67.4 57.2 85.8



63 35.9 30.8 46.2

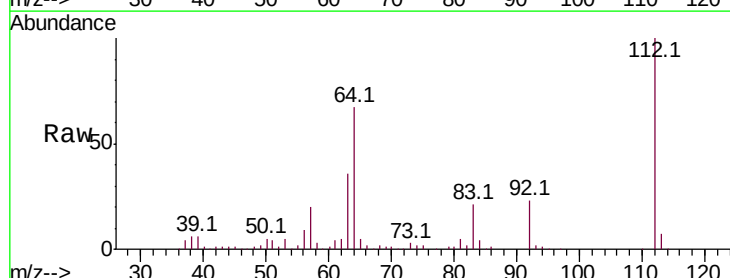


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BG

Ion 63.00 (62.70 to 63.70): BG

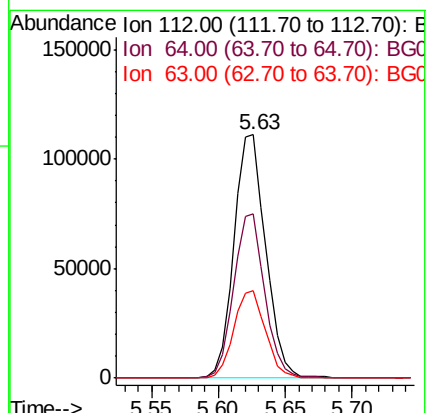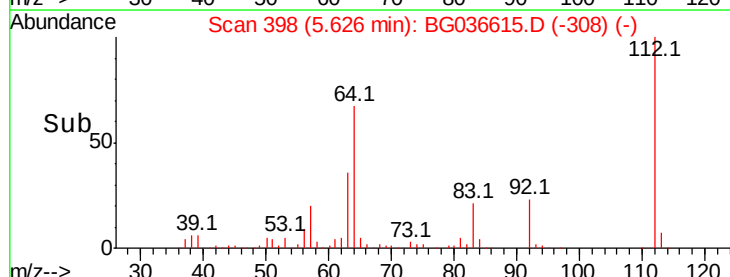

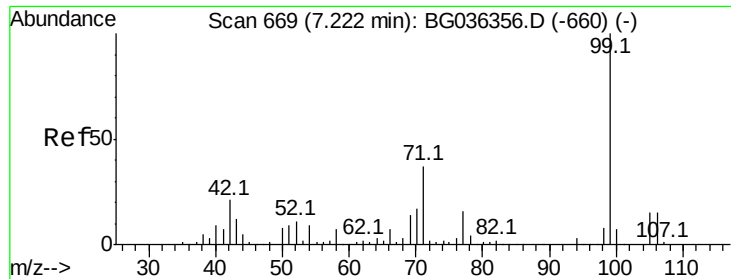

#7

Phenol-d6

Concen: 32.651 ng

RT: 7.21 min Scan# 667

Delta R.T. -0.01 min

Lab File: BG036615.D

Acq: 8 Sep 2018 3:26

Instrument :

BNA_G

ClientSampleId :

090418-TIPC-E-U-M


Tot Ion: 99 Resp: 171334

Ion Ratio Lower Upper




99 100

42 19.4 16.5 24.7

71 35.0 29.4 44.2

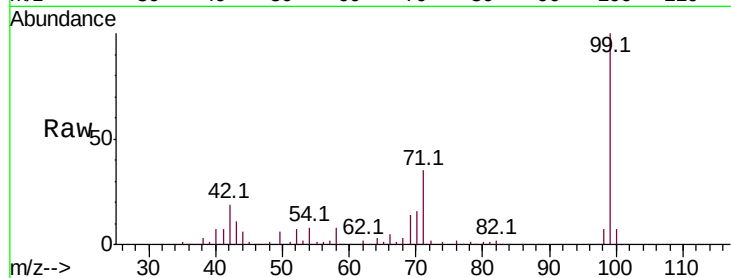

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

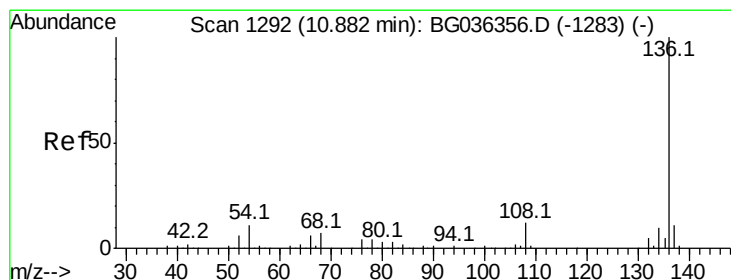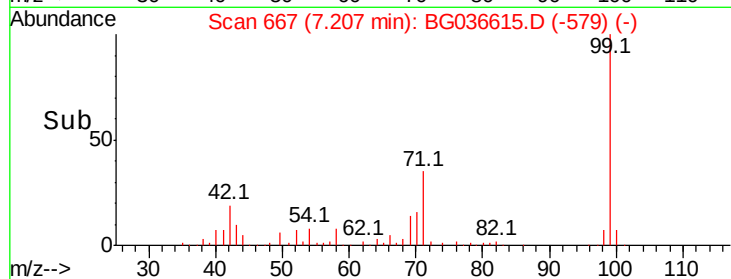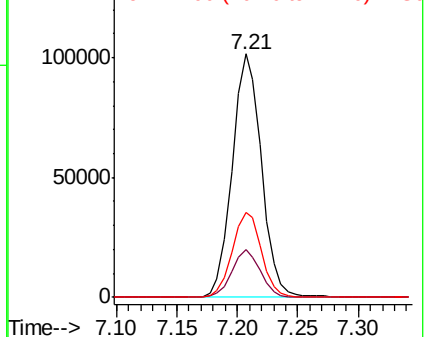

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.86 min Scan# 1289

Delta R.T. -0.00 min

Lab File: BG036615.D

Acq: 8 Sep 2018 3:26

Tgt Ion: 136 Resp: 251136


Ion Ratio Lower Upper

136 100



137 11.1 8.8 13.2


54 9.9 9.2 13.8

68 6.6 5.8 8.6

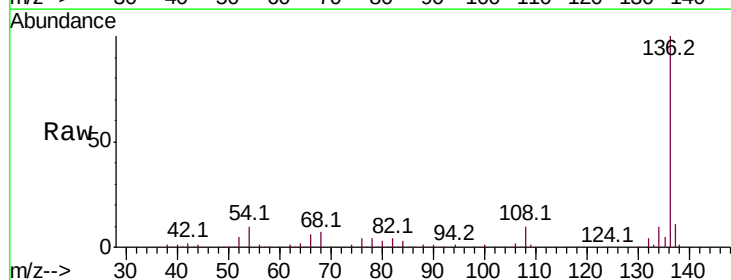

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



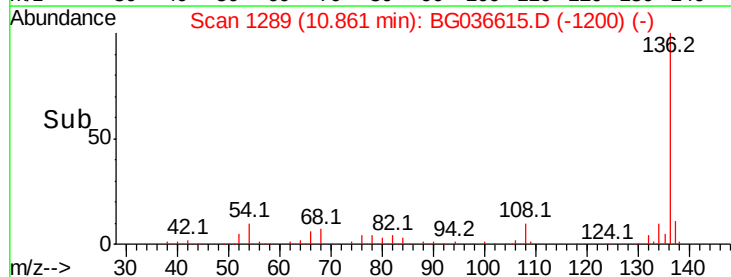
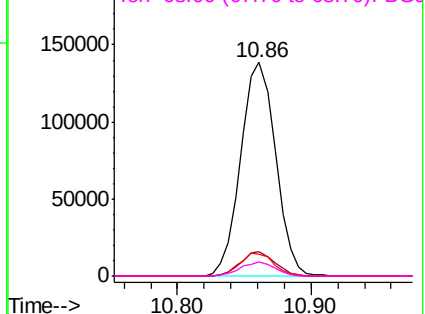


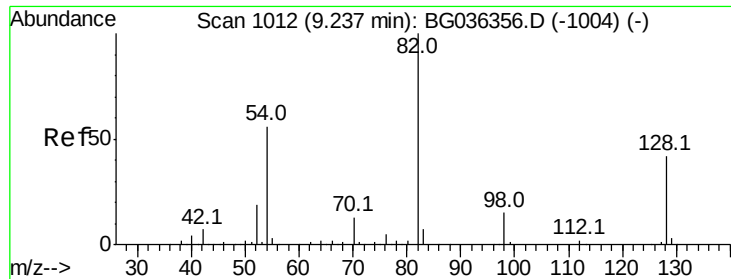

#23
Nitrobenzene-d5
Concen: 111.964 ng
RT: 9.22 min Scan# 1009
Delta R.T. -0.00 min
Lab File: BG036615.D
Acq: 8 Sep 2018 3:26




Instrument :
BNA_G
ClientSampleId :
090418-TIPC-E-U-M


Tot Ion: 82 Resp: 518244
Ion Ratio Lower Upper
82 100
128 43.1 33.3 49.9
54 54.4 45.1 67.7

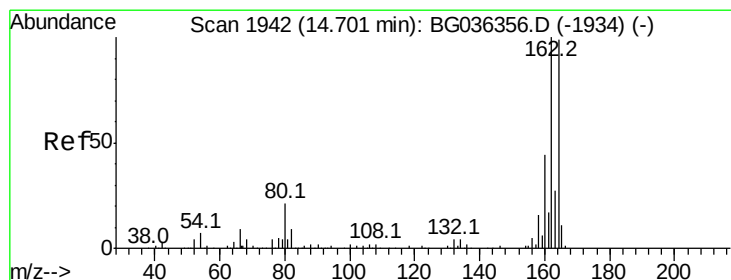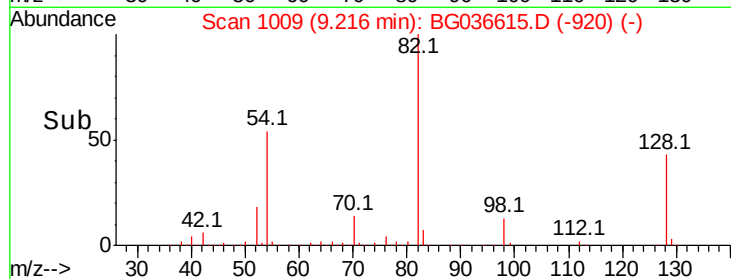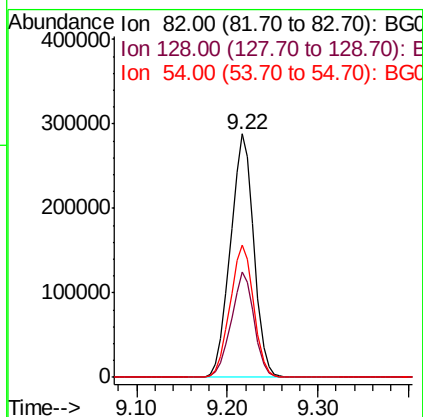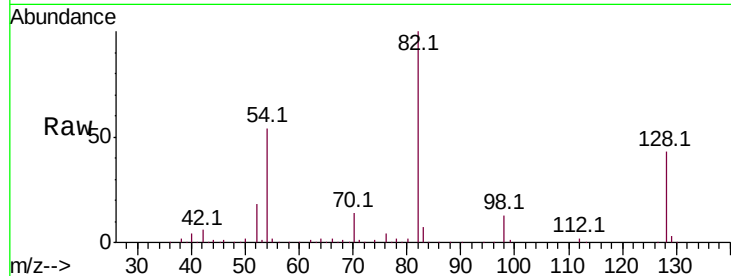

#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.68 min Scan# 1939
Delta R.T. -0.00 min
Lab File: BG036615.D
Acq: 8 Sep 2018 3:26

Tgt Ion:164 Resp: 170611
Ion Ratio Lower Upper
164 100
162 101.6 80.7 121.1
160 45.6 35.3 52.9

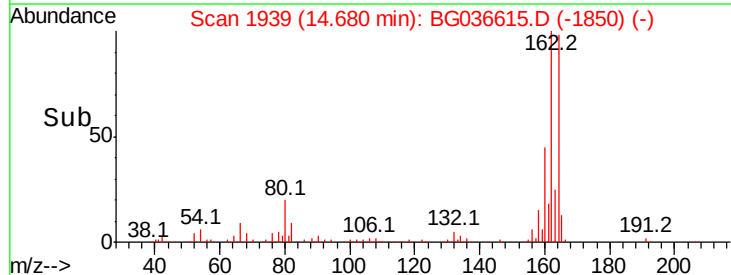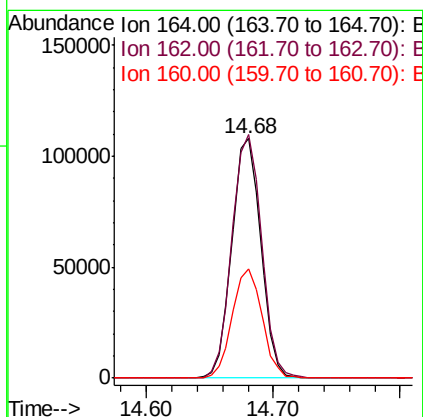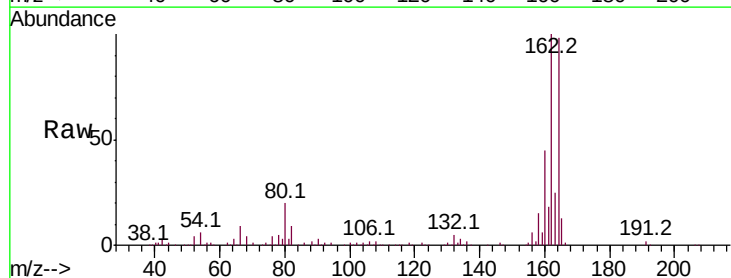


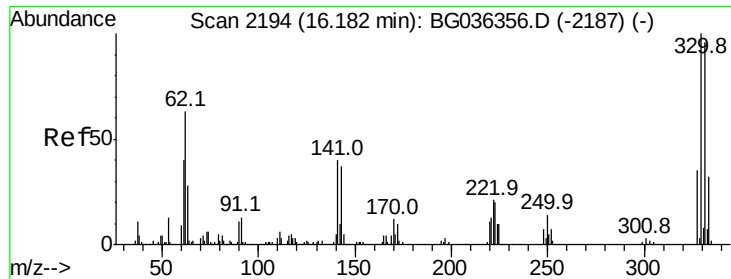

#41
 2,4,6-Tribromophenol
 Concen: 118.382 ng
 RT: 16.17 min Scan# 2192
 Delta R.T. -0.00 min
 Lab File: BG036615.D
 Acq: 8 Sep 2018 3:26

Instrument :
 BNA_G
 ClientSampleId :
 090418-TIPC-E-U-M

Tot Ion	Ratio	Lower	Upper
330	100		
332	93.7	75.4	113.2
141	34.9	30.7	46.1



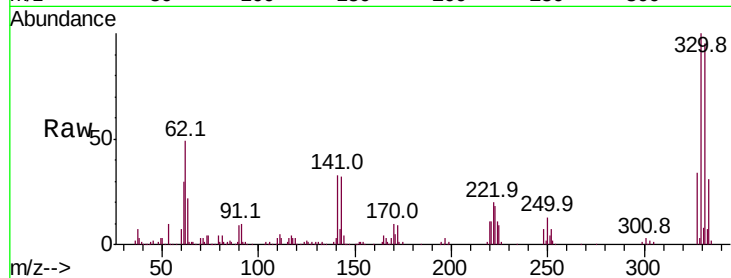


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

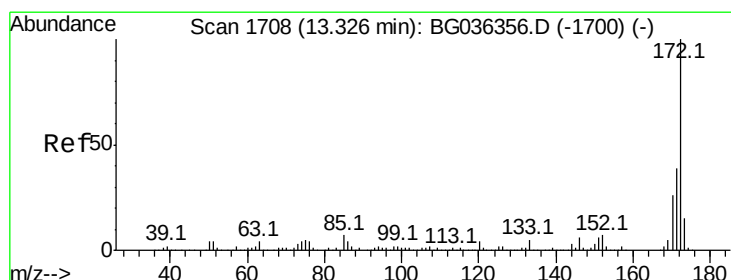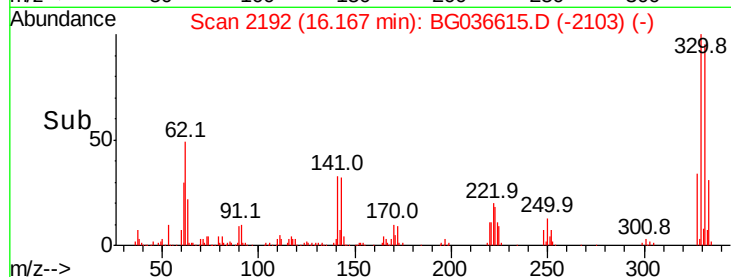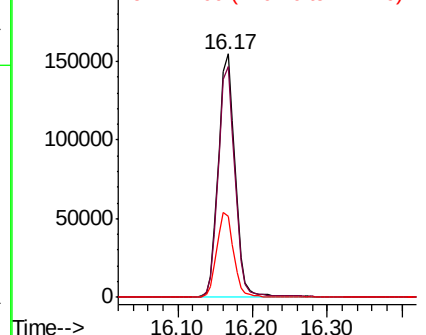

#44
 2-Fluorobiphenyl
 Concen: 99.032 ng
 RT: 13.31 min Scan# 1705
 Delta R.T. -0.00 min
 Lab File: BG036615.D
 Acq: 8 Sep 2018 3:26

Tgt Ion	Ratio	Lower	Upper
172	100		
171	38.5	31.3	46.9
170	25.2	21.0	31.6


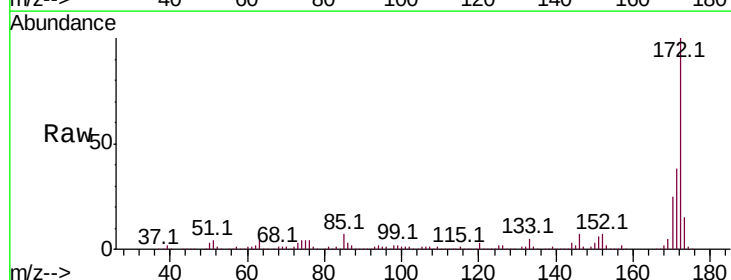



Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

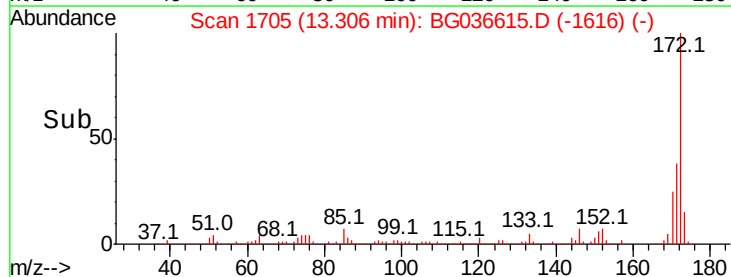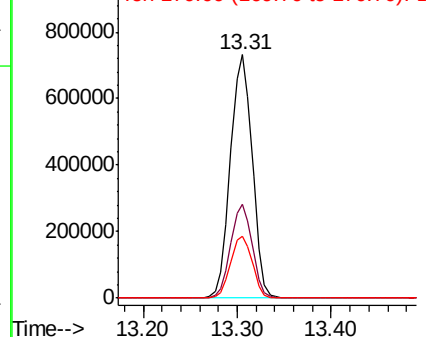

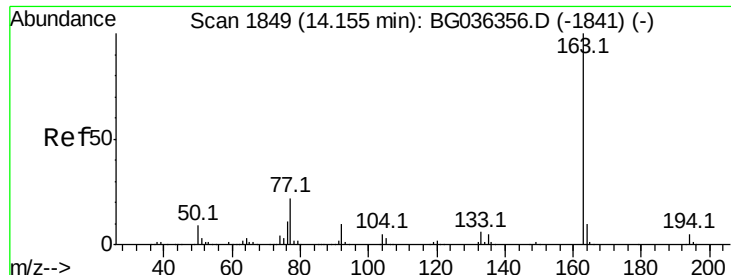

#49

Dimethylphthalate

Concen: 4.712 ng

RT: 14.13 min Scan# 1845

Delta R.T. -0.01 min

Lab File: BG036615.D

Acq: 8 Sep 2018 3:26

Instrument :

BNA_G

ClientSampleId :

090418-TIPC-E-U-M


Tot Ion:163 Resp: 65650

Ion Ratio Lower Upper




163 100

194 5.3 4.0 6.0

164 9.1 8.1 12.1

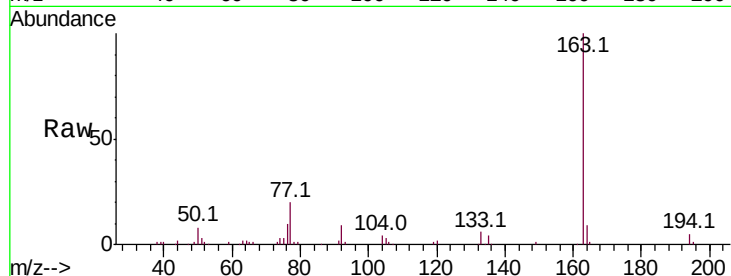

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

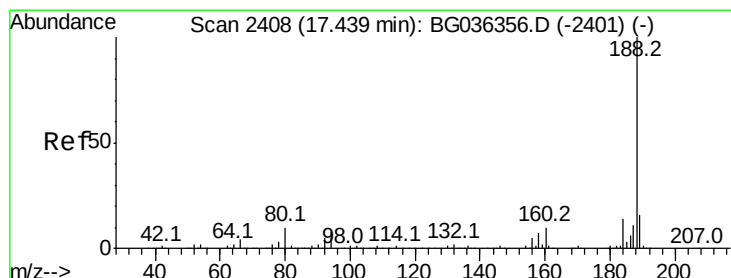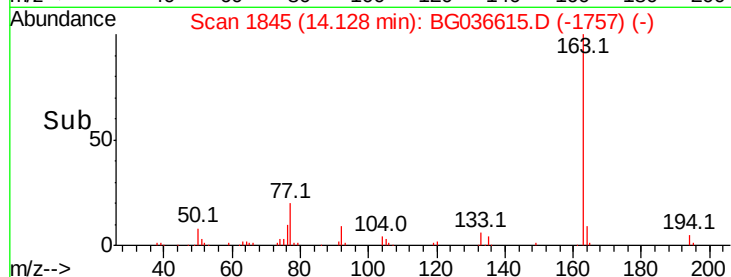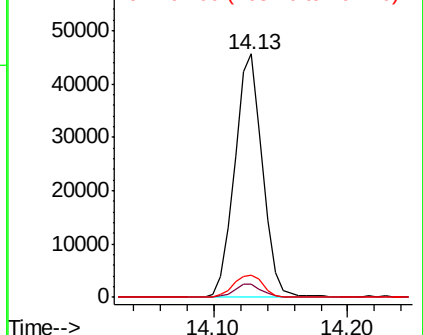

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.42 min Scan# 2406

Delta R.T. -0.00 min

Lab File: BG036615.D

Acq: 8 Sep 2018 3:26


Tgt Ion:188 Resp: 429408

Ion Ratio Lower Upper



188 100


94 7.3 6.7 10.1

80 8.7 8.1 12.1

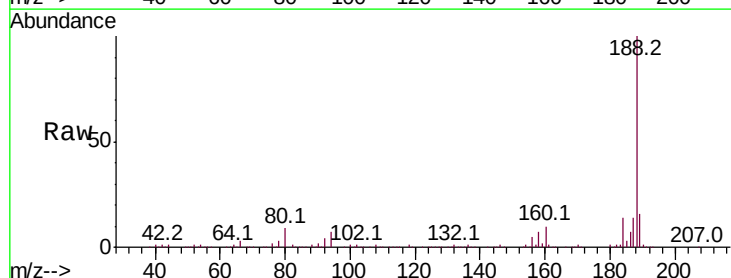

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BGC
Ion 80.00 (79.70 to 80.70): BGC

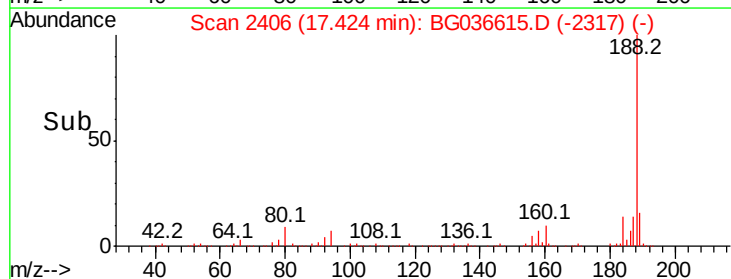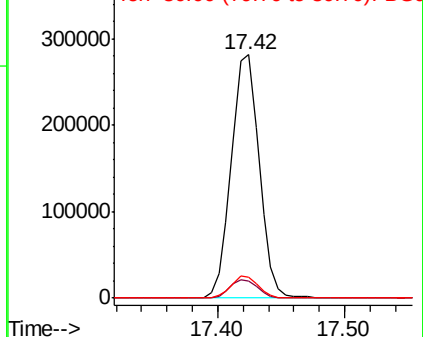

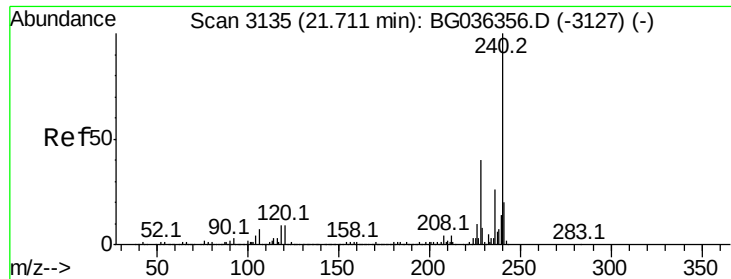

#75

Chrysene-d12

Concen: 20.000 ng

RT: 21.68 min Scan# 3131

Delta R.T. -0.01 min

Lab File: BG036615.D

Acq: 8 Sep 2018 3:26

Instrument :

BNA_G

ClientSampleId :

090418-TIPC-E-U-M


Tot Ion:240 Resp: 429398

Ion Ratio Lower Upper

240 100

120 7.7 6.9 10.3




236 26.7 21.2 31.8

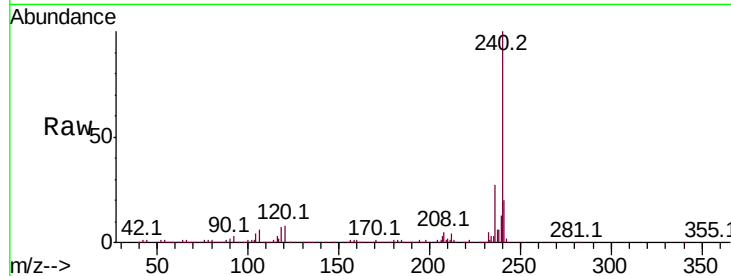

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

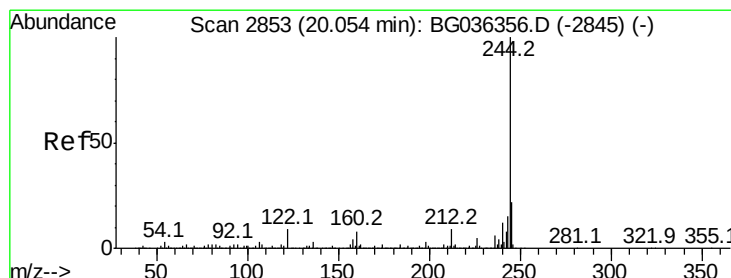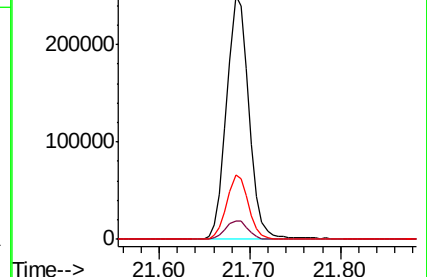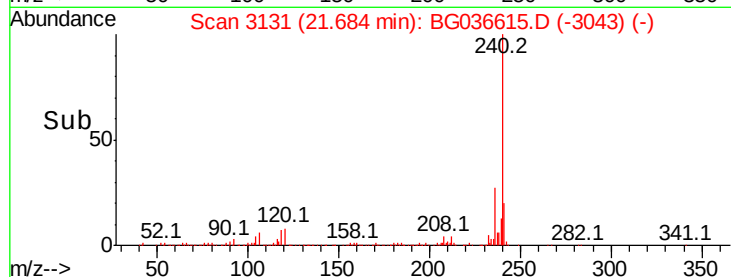

#78

Terphenyl-d14

Concen: 97.371 ng

RT: 20.03 min Scan# 2849

Delta R.T. -0.00 min

Lab File: BG036615.D

Acq: 8 Sep 2018 3:26


Tgt Ion:244 Resp: 1788820

Ion Ratio Lower Upper

244 100

212 9.6 7.0 10.6



122 9.8 7.1 10.7

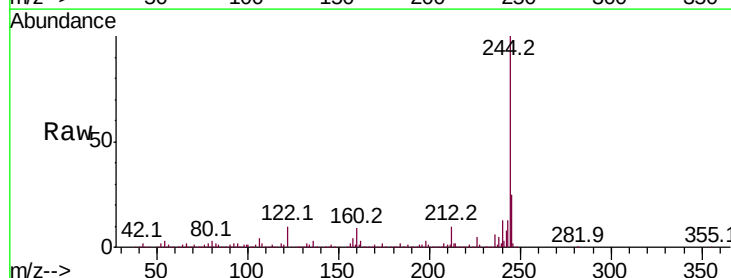


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

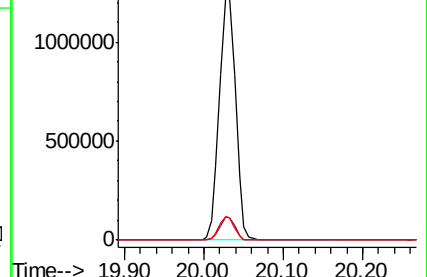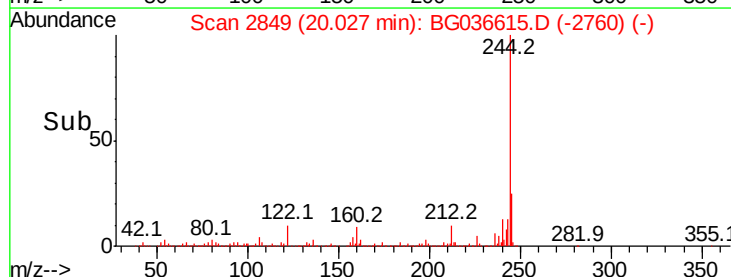


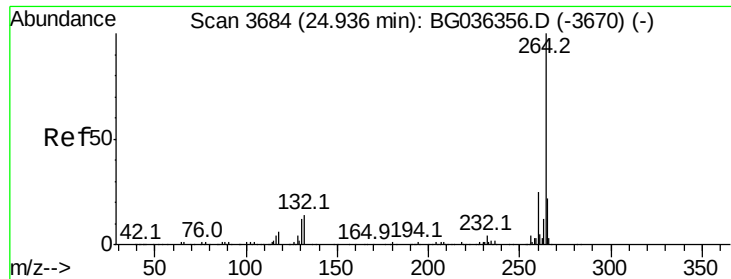

#86
Pervlene-d12
Concen: 20.000 ng
RT: 24.90 min Scan# 3678
Delta R.T. -0.00 min
Lab File: BG036615.D
Acq: 8 Sep 2018 3:26

Instrument :
BNA_G
ClientSampleId :
090418-TIPC-E-U-M

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.1	19.6	29.4
265	20.2	17.4	26.0

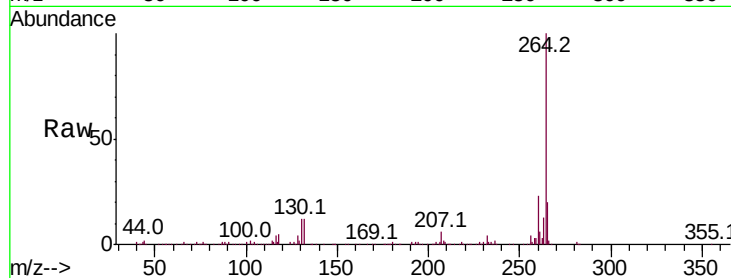

Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

