


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG090718\
 Data File : BG036593.D
 Acq On : 7 Sep 2018 12:29
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 31 13:03:20 2018

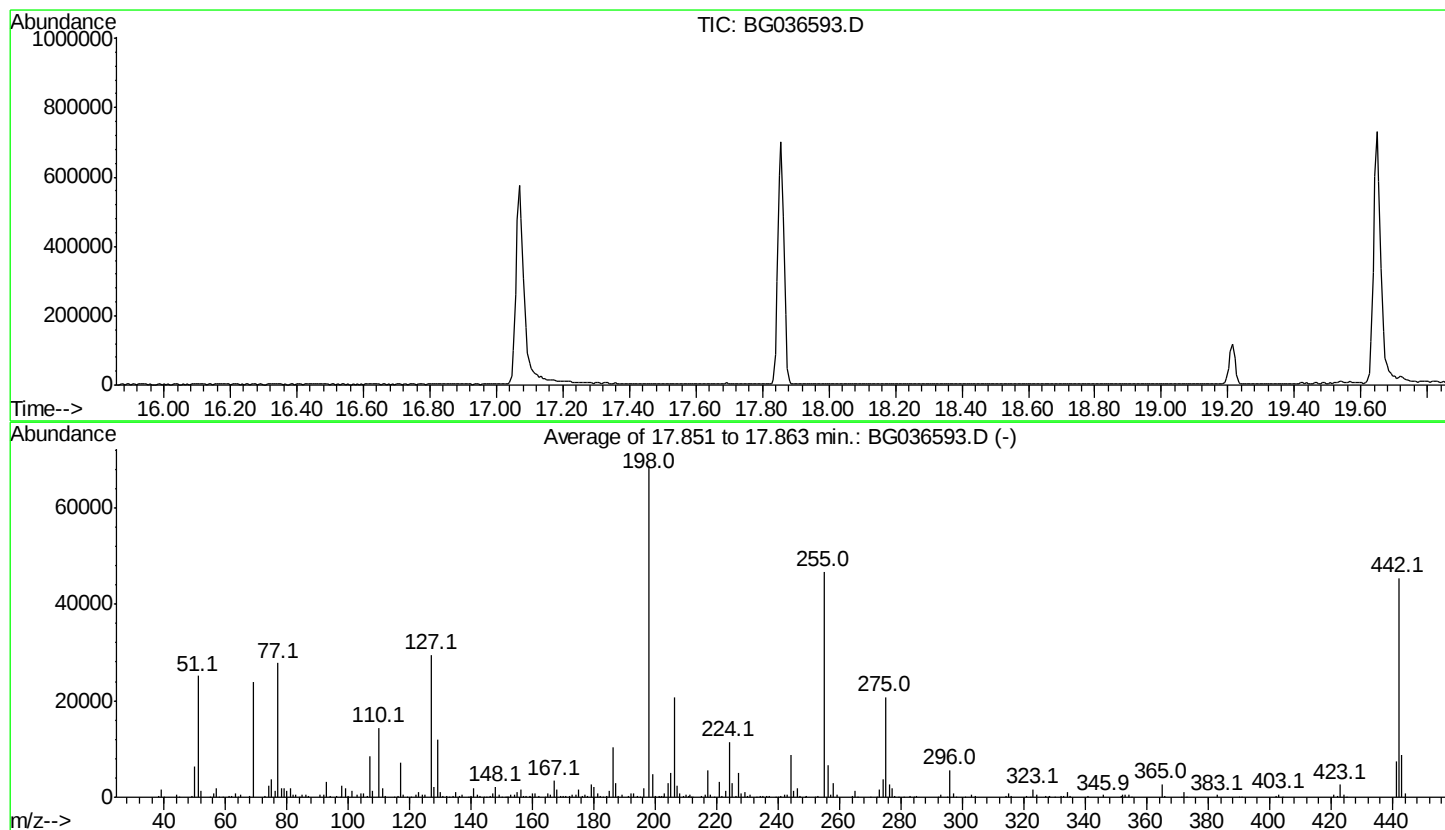

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.5	25104	PASS
68	69	0.00	2	0.8	199	PASS
69	198	0.00	100	34.6	23765	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.9	29509	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	68725	PASS
199	198	5	9	7.1	4853	PASS
275	198	10	60	30.3	20829	PASS
365	198	1	100	4.0	2782	PASS
441	198	0.01	100	10.7	7370	PASS
442	198	50	100	66.0	45378	PASS
443	442	15	24	19.1	8653	PASS